

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090123\
Data File : FE044080.D
Signal(s) : FID1B.ch
Acq On : 01 Sep 2023 09:12
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 01 23:59:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.736	4335327	25.450 ug/ml
12) N-OCTACOSANE	17.198	3955461	25.302 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090123\
Data File : FE044080.D
Signal(s) : FID1B.ch
Acq On : 01 Sep 2023 09:12
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 01 23:59:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

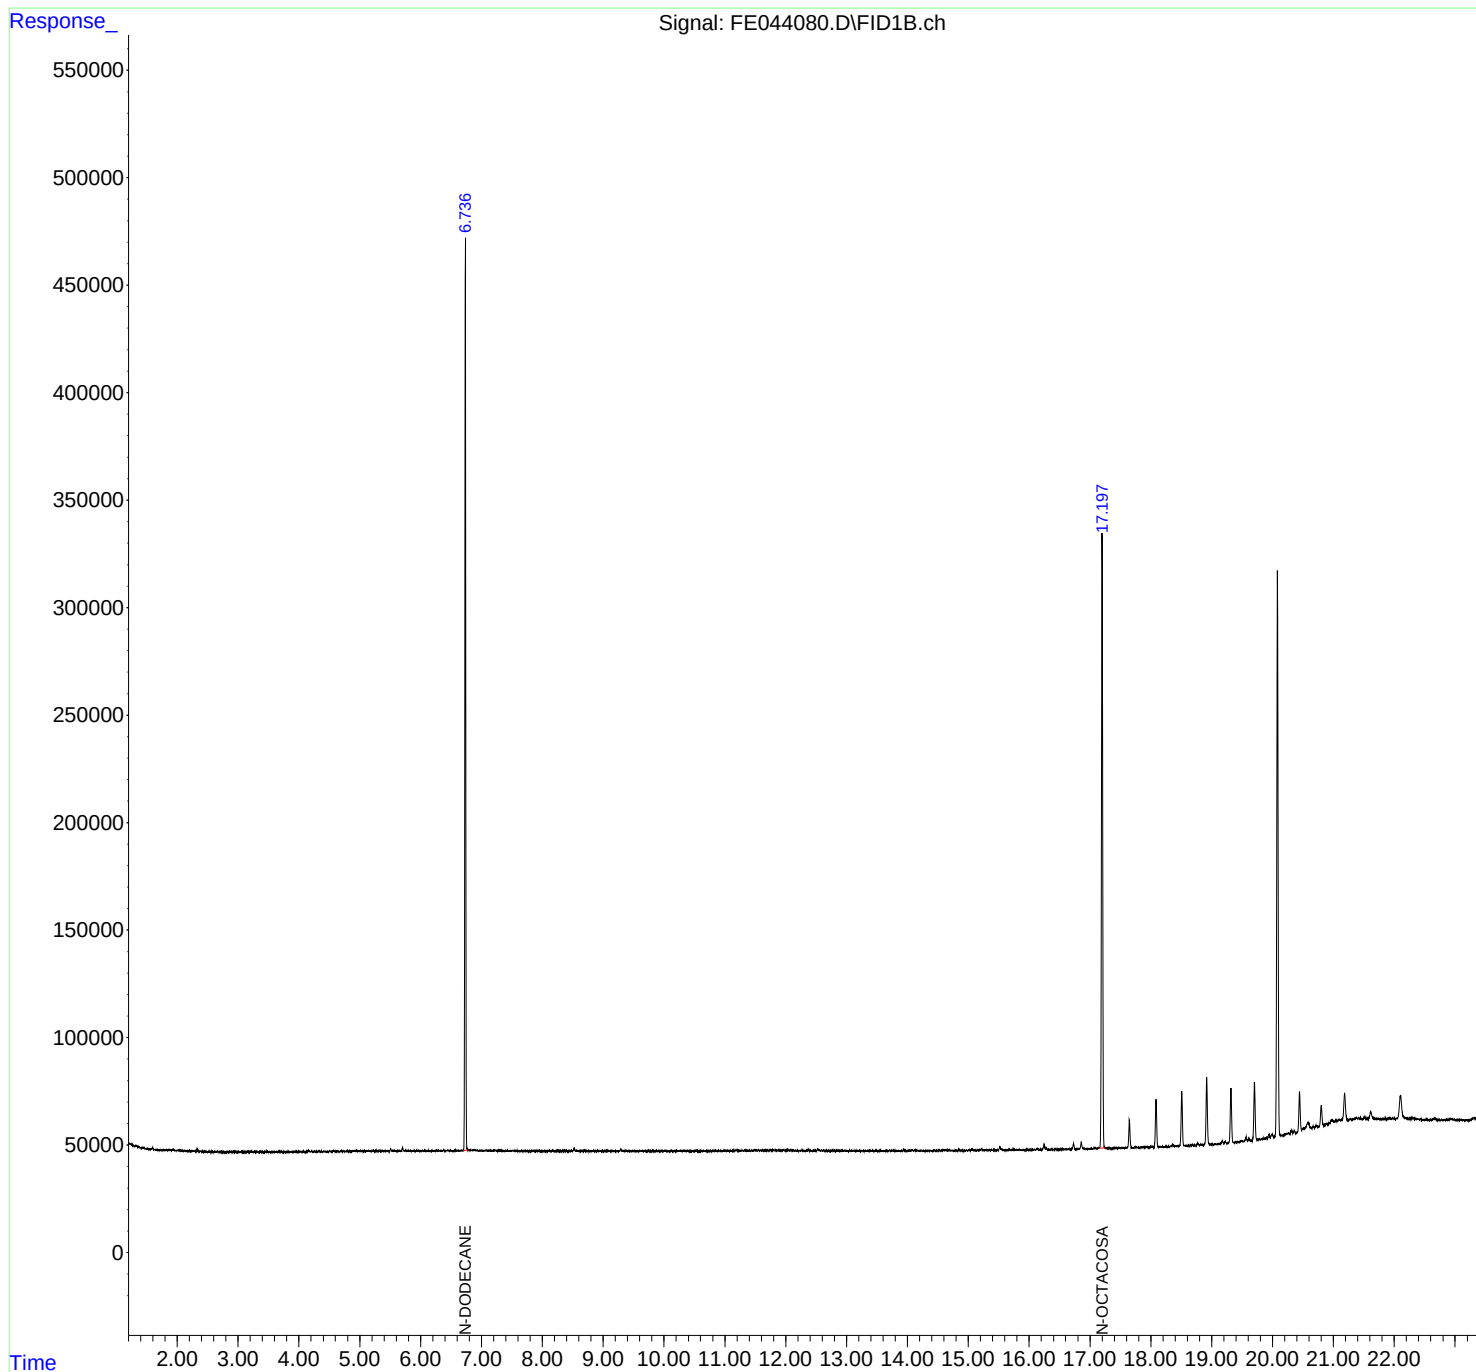


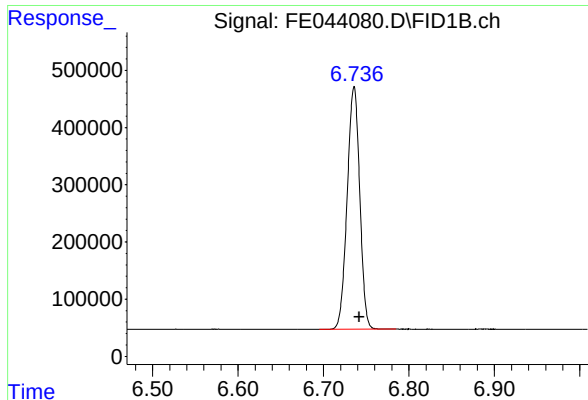

#3 N-DODECANE


R.T.: 6.736 min
Delta R.T.: -0.006 min
Response: 4335327
Conc: 25.45 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

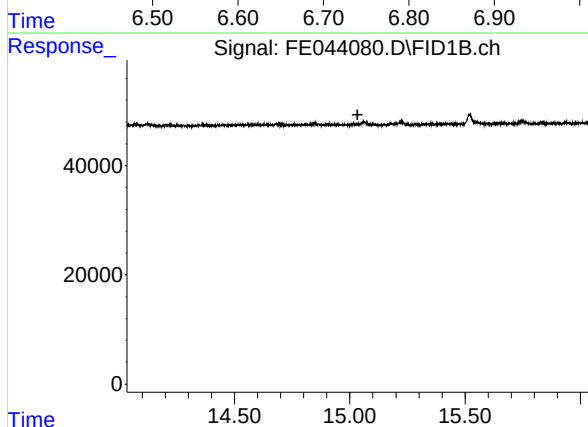

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.034 min
Response: 0
Conc: N.D.

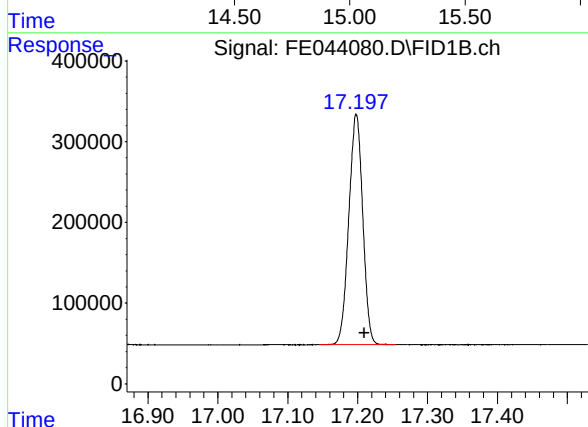

#12 N-OCTACOSANE

R.T.: 17.198 min
Delta R.T.: -0.011 min
Response: 3955461
Conc: 25.30 ug/ml