

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090220\
 Data File : FE032684.D
 Signal(s) : FID1B.CH
 Acq On : 02 Sep 2020 17:57
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Sep 03 01:18:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
 Quant Title :
 QLast Update : Thu Aug 13 11:46:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.707	17811970	55.346 ug/ml
Target Compounds			
2) N-DECANE	4.448	21599145	60.154 ug/ml
3) N-DODECANE	6.464	21770987	60.229 ug/ml
4) N-TETRADECANE	8.259	21647785	59.939 ug/ml
5) N-HEXADECANE	9.860	21519827	58.992 ug/ml
6) N-OCTADECANE	11.303	21611722	58.179 ug/ml
7) N-EICOSANE	12.612	21223098	57.295 ug/ml
8) N-DOCOSANE	13.810	20823713	56.142 ug/ml
10) N-TETRACOSANE	14.912	20547147	54.880 ug/ml
11) N-HEXACOSANE	15.931	19796446	53.342 ug/ml
12) N-OCTACOSANE	16.881	19387291	52.044 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090220\
Data File : FE032684.D
Signal(s) : FID1B.CH
Acq On : 02 Sep 2020 17:57
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Sep 03 01:18:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
Quant Title :
QLast Update : Thu Aug 13 11:46:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

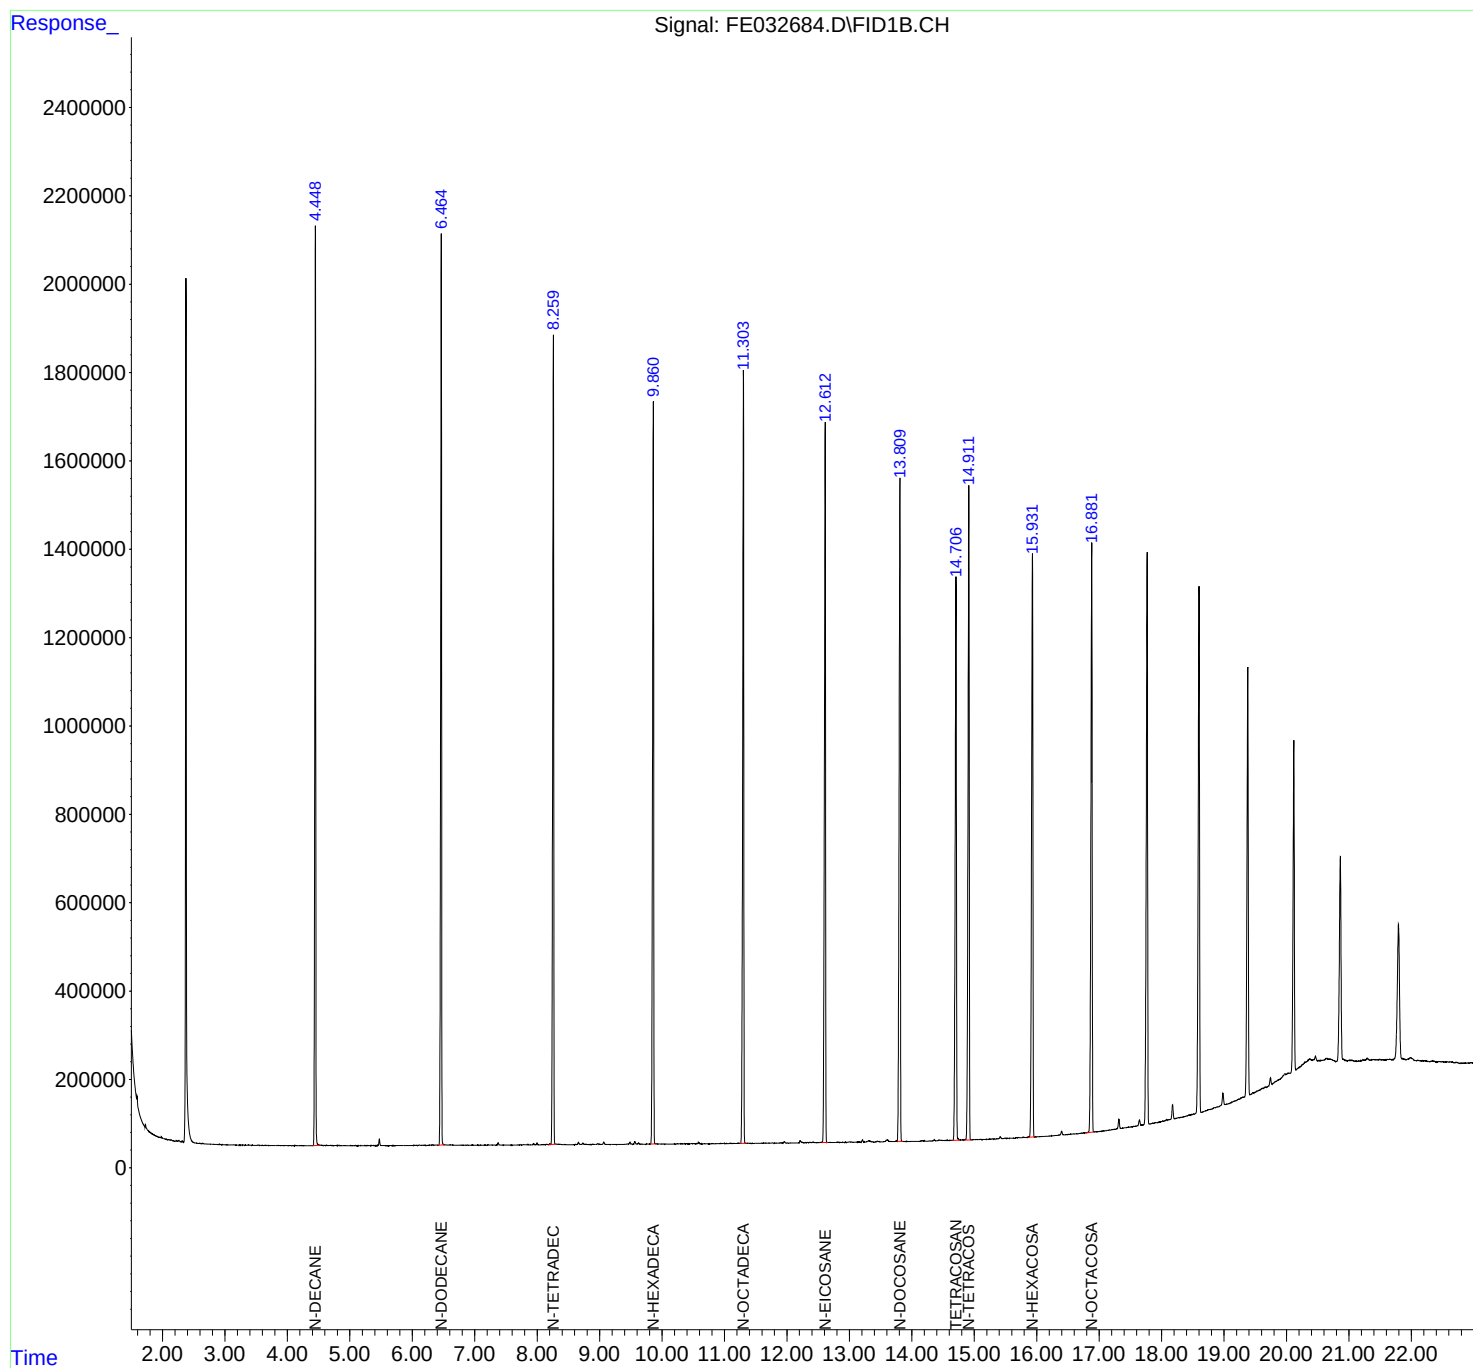

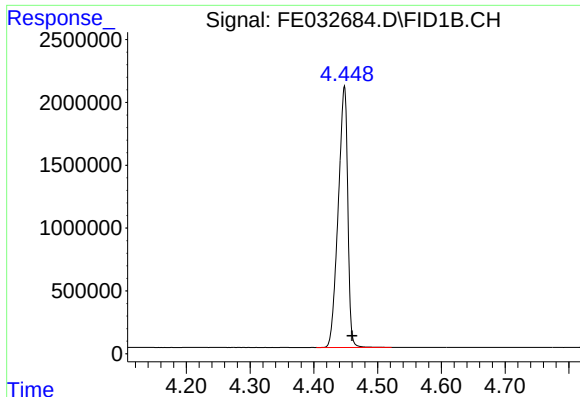


#2 N-DECANE

R.T.: 4.448 min
Delta R.T.: -0.012 min
Response: 21599145
Conc: 60.15 ug/ml

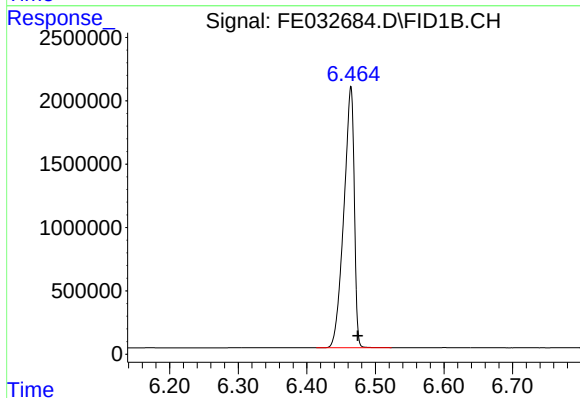


#3 N-DODECANE

R.T.: 6.464 min
Delta R.T.: -0.010 min
Response: 21770987
Conc: 60.23 ug/ml

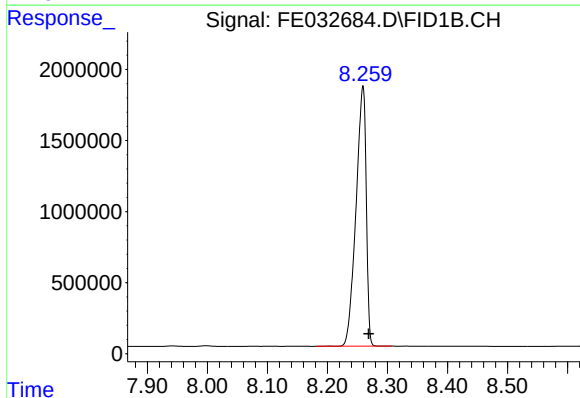


#4 N-TETRADECANE

R.T.: 8.259 min
Delta R.T.: -0.009 min
Response: 21647785
Conc: 59.94 ug/ml

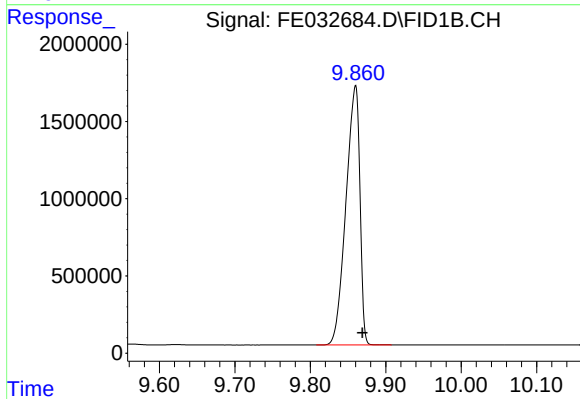


#5 N-HEXADECANE

R.T.: 9.860 min
Delta R.T.: -0.009 min
Response: 21519827
Conc: 58.99 ug/ml

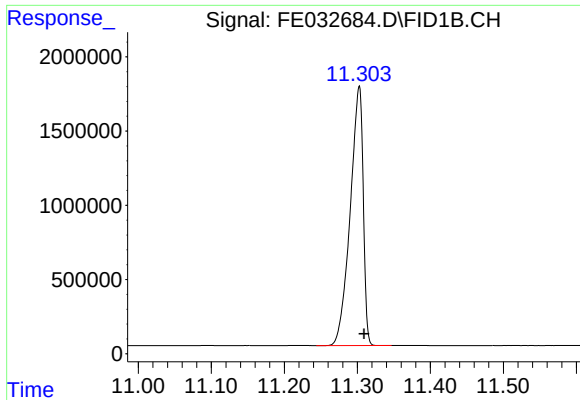


#6 N-OCTADECANE

R.T.: 11.303 min
Delta R.T.: -0.006 min
Response: 21611722
Conc: 58.18 ug/ml

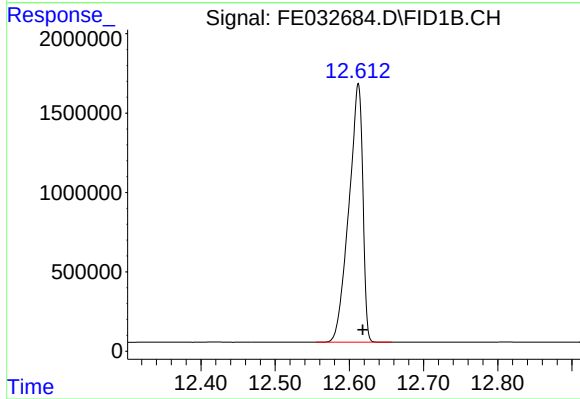


#7 N-EICOSANE

R.T.: 12.612 min
Delta R.T.: -0.006 min
Response: 21223098
Conc: 57.29 ug/ml

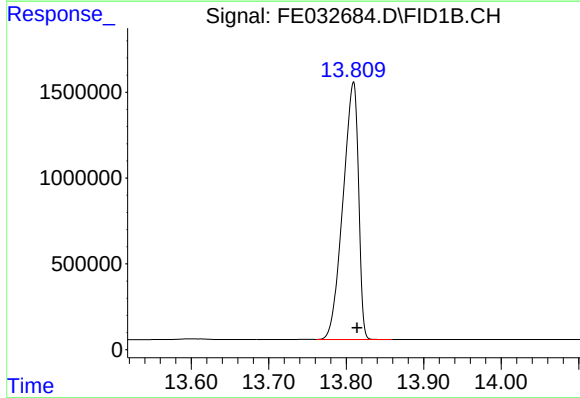


#8 N-DOCOSANE

R.T.: 13.810 min
Delta R.T.: -0.004 min
Response: 20823713
Conc: 56.14 ug/ml

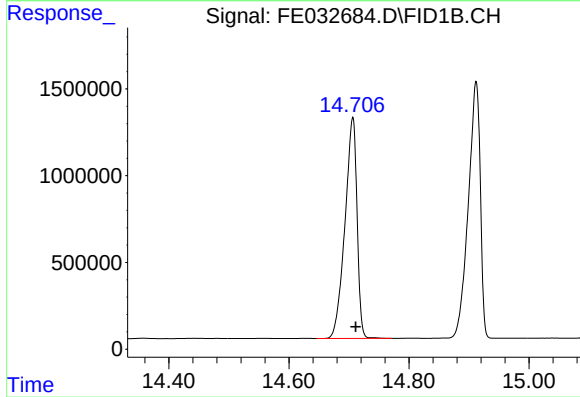


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.707 min
Delta R.T.: -0.004 min
Response: 17811970
Conc: 55.35 ug/ml

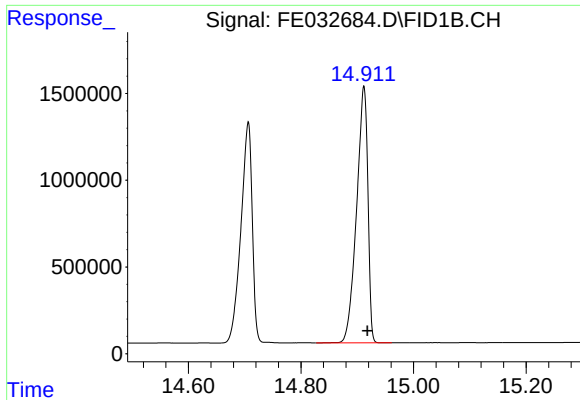


#10 N-TETRACOSANE

R.T.: 14.912 min
Delta R.T.: -0.006 min
Response: 20547147
Conc: 54.88 ug/ml

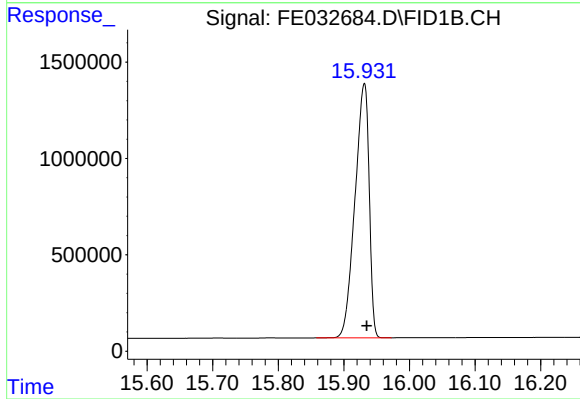

#11 N-HEXACOSANE

R.T.: 15.931 min
Delta R.T.: -0.004 min
Response: 19796446
Conc: 53.34 ug/ml

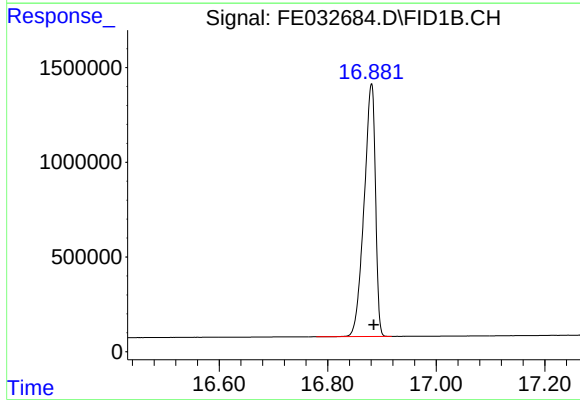

#12 N-OCTACOSANE

R.T.: 16.881 min
Delta R.T.: -0.004 min
Response: 19387291
Conc: 52.04 ug/ml