

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090524AL\
 Data File : FE049924.D
 Signal(s) : FID1B.ch
 Acq On : 05 Sep 2024 06:06
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 06 01:29:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 11:05:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.468	346185	2.360 ug/ml
13) T	n-Docosane (C22)	14.057	94501	0.648 ug/ml
14) T	n-Tetracosane (C24)	15.160	225011	1.547 ug/ml
15) T	n-Hexacosane (C26)	16.185	116332	0.806 ug/ml
16) T	n-Octacosane (C28)	17.130	205829	1.429 ug/ml
17) T	n-Tricontane (C30)	18.017	259203	1.731 ug/ml
18) T	n-Dotriacontane (C32)	18.849	318694	2.107 ug/ml
19) T	n-Tetratriacontane (C34)	19.630	166993	1.092 ug/ml
20) T	n-Hexatriacontane (C36)	20.370	133291	0.878 ug/ml
21) T	n-Octatriacontane (C38)	21.095	18022	0.115 ug/ml
22) T	n-Tetracontane (C40)	21.971	174056	1.140 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090524AL\
Data File : FE049924.D
Signal(s) : FID1B.ch
Acq On : 05 Sep 2024 06:06
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 01:29:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 11:05:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

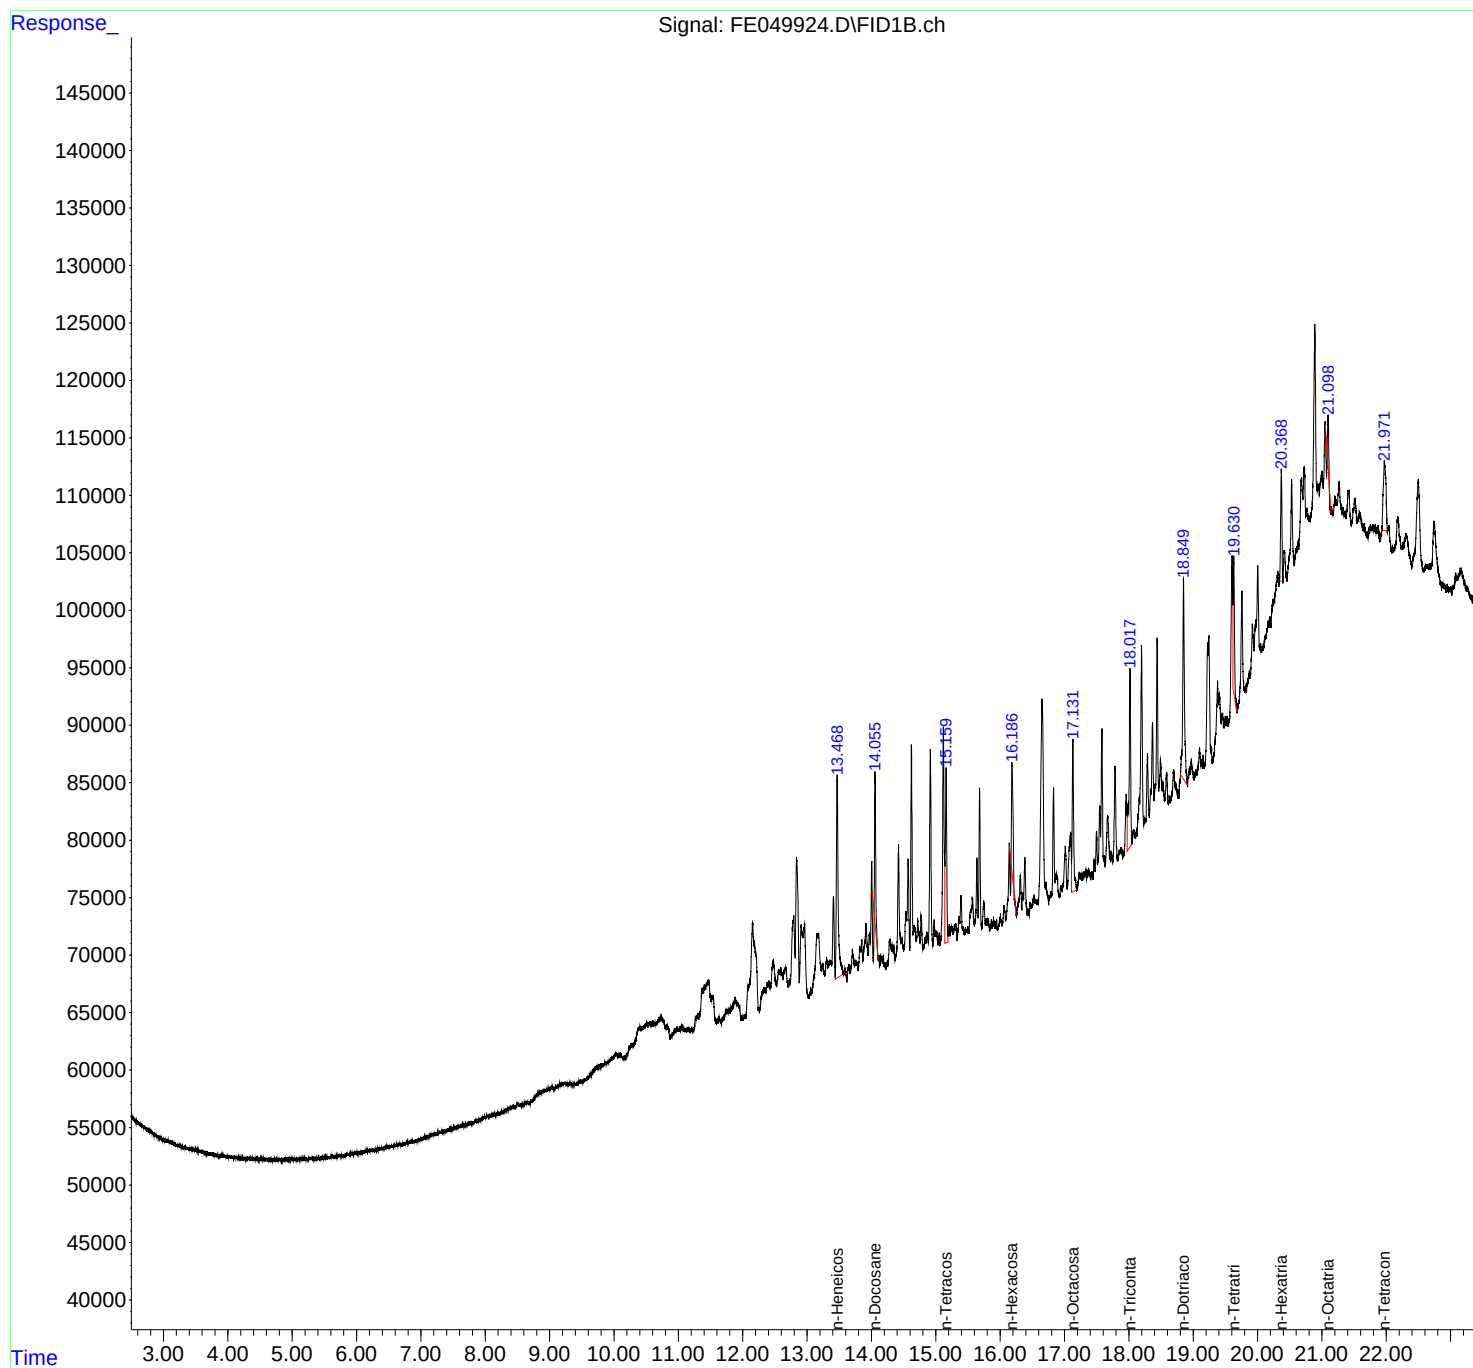


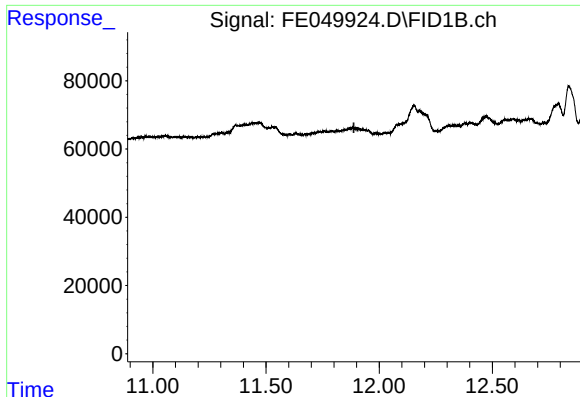

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.888 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

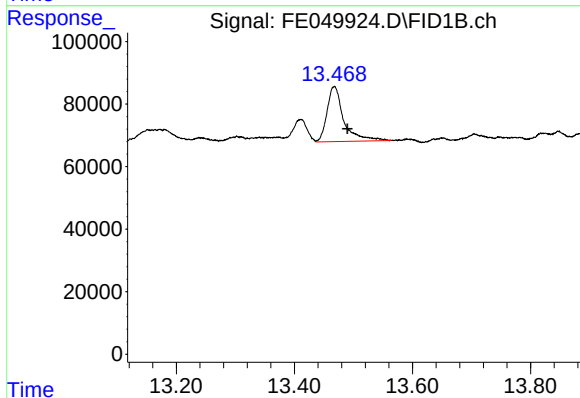


#11 n-Heneicosane (C21)

R.T.: 13.468 min
Delta R.T.: -0.022 min
Response: 346185
Conc: 2.36 ug/ml

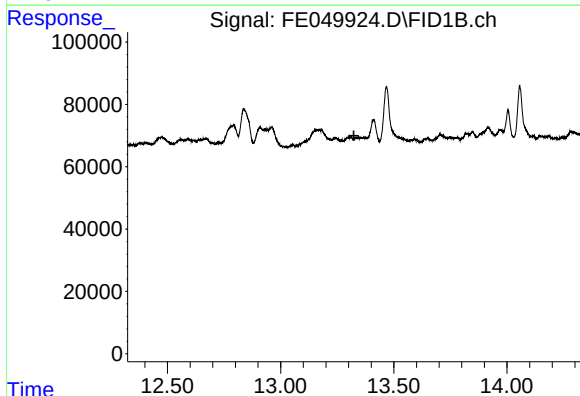


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.323 min
Response: 0
Conc: N.D.

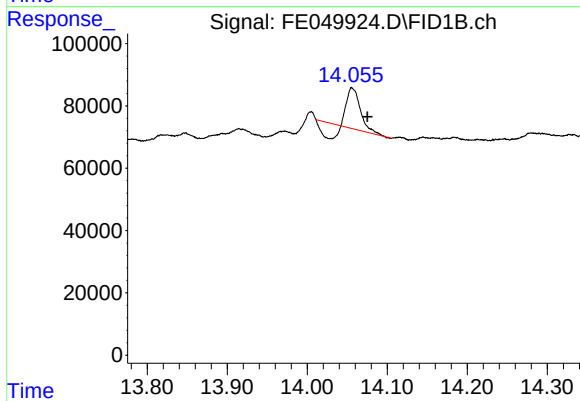

#13 n-Docosane (C22)


R.T.: 14.057 min
Delta R.T.: -0.019 min
Response: 94501
Conc: 0.65 ug/ml

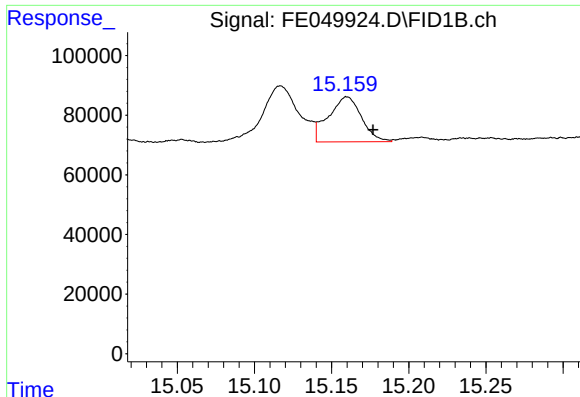

#14 n-Tetracosane (C24)


R.T.: 15.160 min
Delta R.T.: -0.017 min
Response: 225011
Conc: 1.55 ug/ml

Instrument :
FID_E
ClientSampleId :

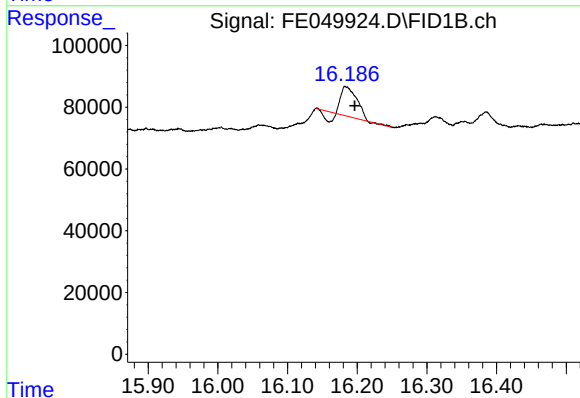


#15 n-Hexacosane (C26)

R.T.: 16.185 min
Delta R.T.: -0.012 min
Response: 116332
Conc: 0.81 ug/ml

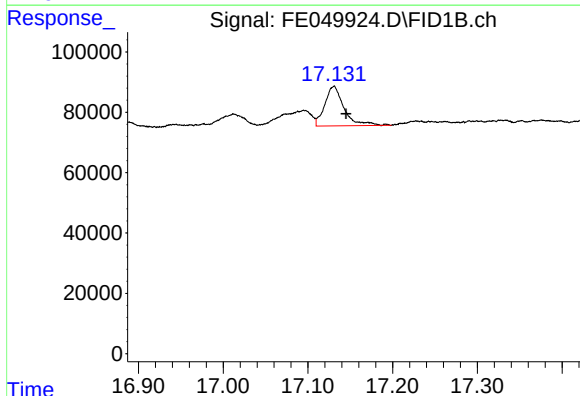


#16 n-Octacosane (C28)

R.T.: 17.130 min
Delta R.T.: -0.014 min
Response: 205829
Conc: 1.43 ug/ml

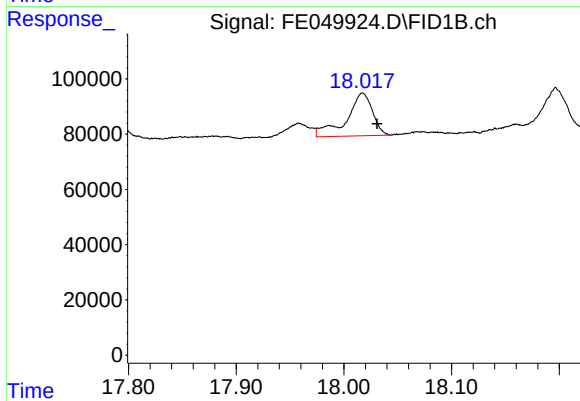

#17 n-Tricontane (C30)


R.T.: 18.017 min
Delta R.T.: -0.014 min
Response: 259203
Conc: 1.73 ug/ml

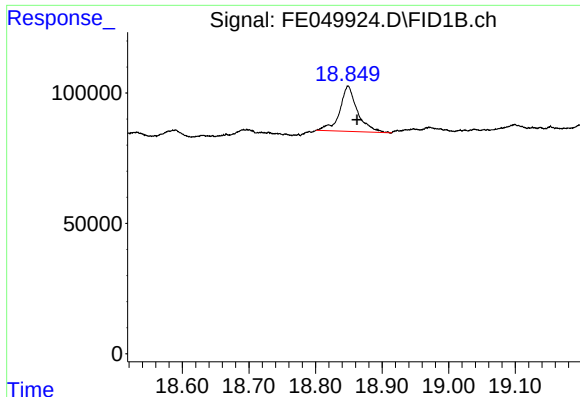

#18 n-Dotriacontane (C32)


R.T.: 18.849 min
Delta R.T.: -0.013 min
Response: 318694
Conc: 2.11 ug/ml

Instrument :
FID_E
ClientSampleId :

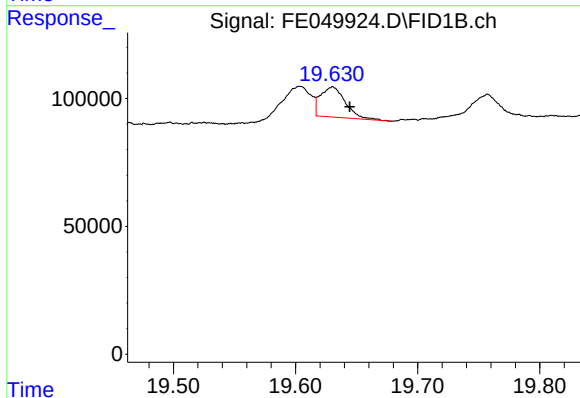


#19 n-Tetratriacontane (C34)

R.T.: 19.630 min
Delta R.T.: -0.014 min
Response: 166993
Conc: 1.09 ug/ml

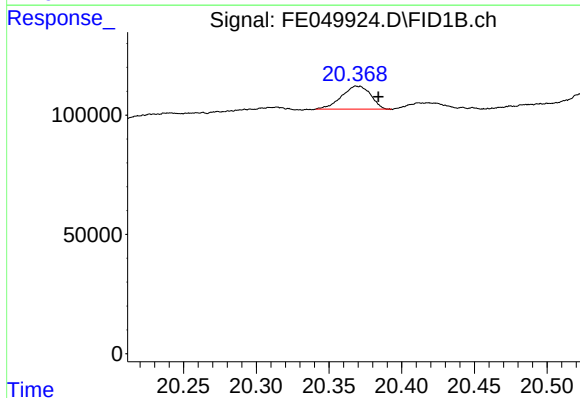


#20 n-Hexatriacontane (C36)

R.T.: 20.370 min
Delta R.T.: -0.014 min
Response: 133291
Conc: 0.88 ug/ml

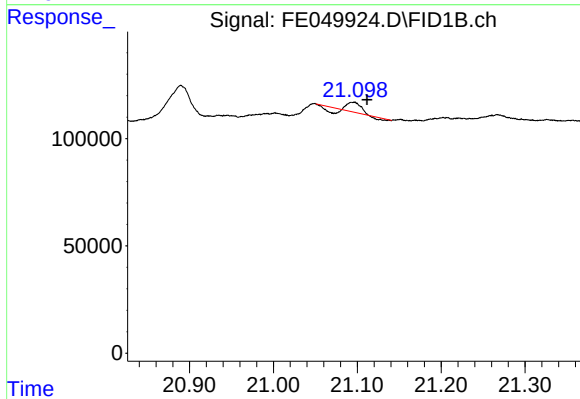

#21 n-Octatriacontane (C38)

R.T.: 21.095 min
Delta R.T.: -0.017 min
Response: 18022
Conc: 0.11 ug/ml

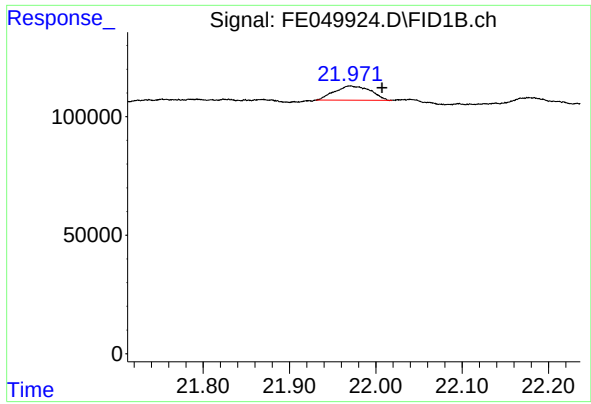

#22 n-Tetracontane (C40)

R.T.: 21.971 min
Delta R.T.: -0.037 min
Response: 174056
Conc: 1.14 ug/ml

Instrument :

FID_E

ClientSampleId :