

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090524AL\
Data File : FE049925.D
Signal(s) : FID1B.ch
Acq On : 05 Sep 2024 07:31
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 01:30:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 11:05:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.016	46584	0.311 ug/ml
18) T	n-Dotriacontane (C32)	18.849	62763	0.415 ug/ml
19) T	n-Tetratriacontane (C34)	19.633	64616	0.423 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090524AL\
Data File : FE049925.D
Signal(s) : FID1B.ch
Acq On : 05 Sep 2024 07:31
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 01:30:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 11:05:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

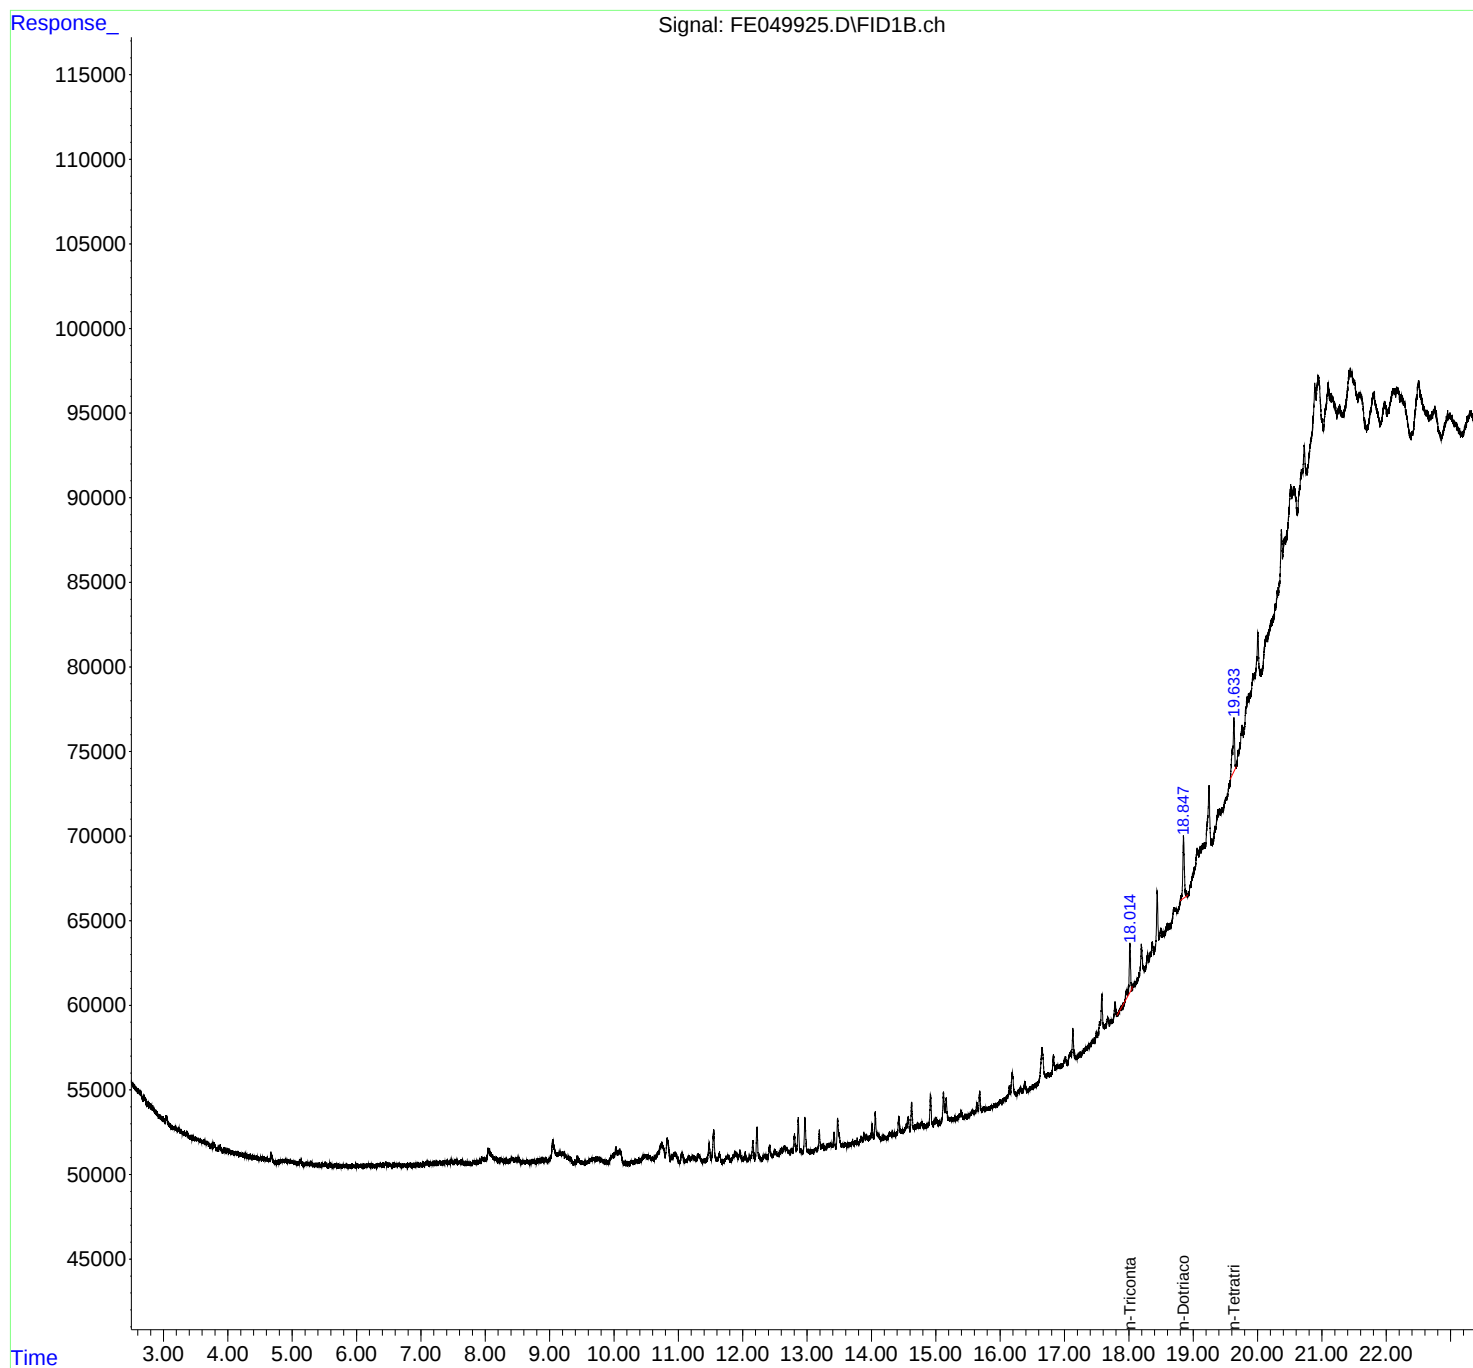


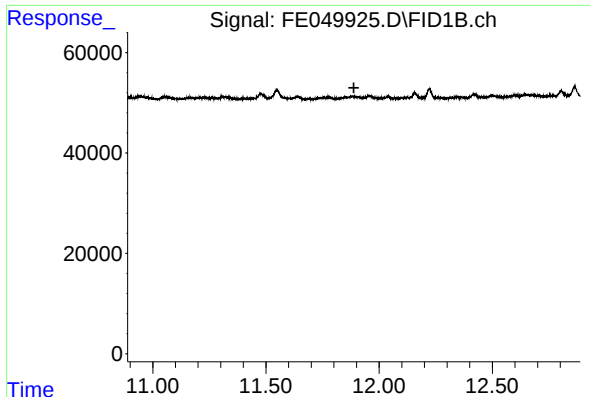

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T. : 11.888 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

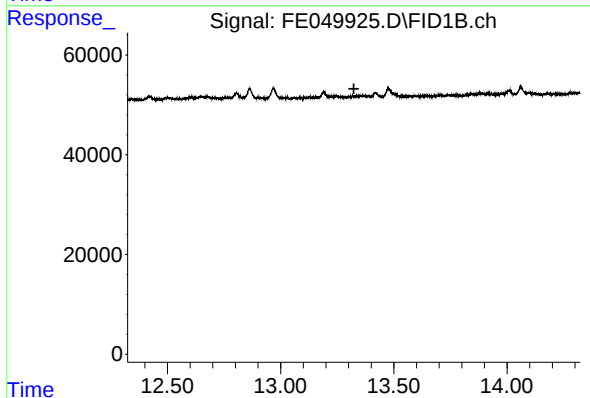


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T. : 13.323 min
Response: 0
Conc: N.D.

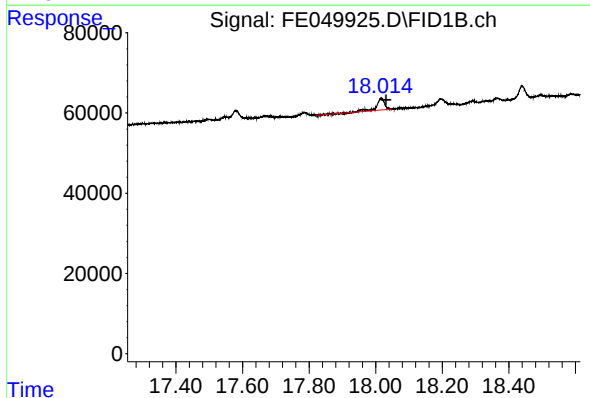


#17 n-Tricontane (C30)

R.T.: 18.016 min
Delta R.T.: -0.015 min
Response: 46584
Conc: 0.31 ug/ml

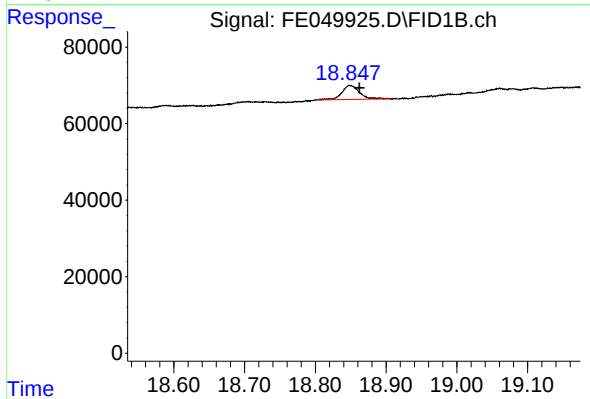

#18 n-Dotriacontane (C32)

R.T.: 18.849 min
Delta R.T.: -0.013 min
Response: 62763
Conc: 0.41 ug/ml

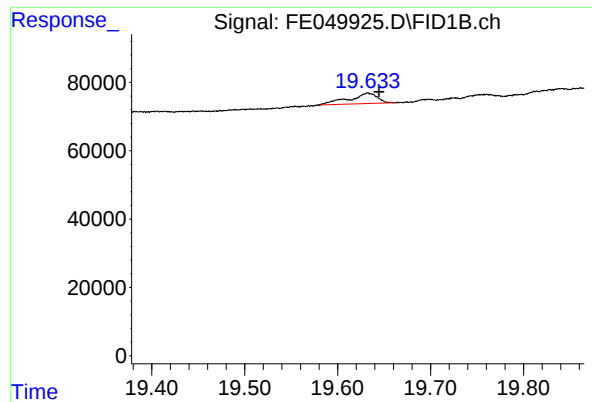

#19 n-Tetratriacontane (C34)

R.T.: 19.633 min
Delta R.T.: -0.012 min
Response: 64616
Conc: 0.42 ug/ml

Instrument :
FID_E
ClientSampleId :