

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090722AL\
 Data File : FE037432.D
 Signal(s) : FID1B.ch
 Acq On : 07 Sep 2022 08:32
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 07 14:53:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.598	186450	1.178 ug/ml
11) T	n-Heneicosane (C21)	13.221	184412	1.169 ug/ml
13) T	n-Docosane (C22)	13.808	184177	1.183 ug/ml
14) T	n-Tetracosane (C24)	14.910	160793	1.069 ug/ml
15) T	n-Hexacosane (C26)	15.928	113951	0.787 ug/ml
16) T	n-Octacosane (C28)	16.875	87130	0.629 ug/ml
17) T	n-Tricontane (C30)	17.757	100085	0.736 ug/ml
18) T	n-Dotriacontane (C32)	18.587	58678	0.439 ug/ml
19) T	n-Tetratriacontane (C34)	19.371	210032	1.660 ug/ml
20) T	n-Hexatriacontane (C36)	20.142	31840	0.248 ug/ml
22) T	n-Tetracontane (C40)	21.596	1352223	10.489 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090722AL\
Data File : FE037432.D
Signal(s) : FID1B.ch
Acq On : 07 Sep 2022 08:32
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 14:53:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

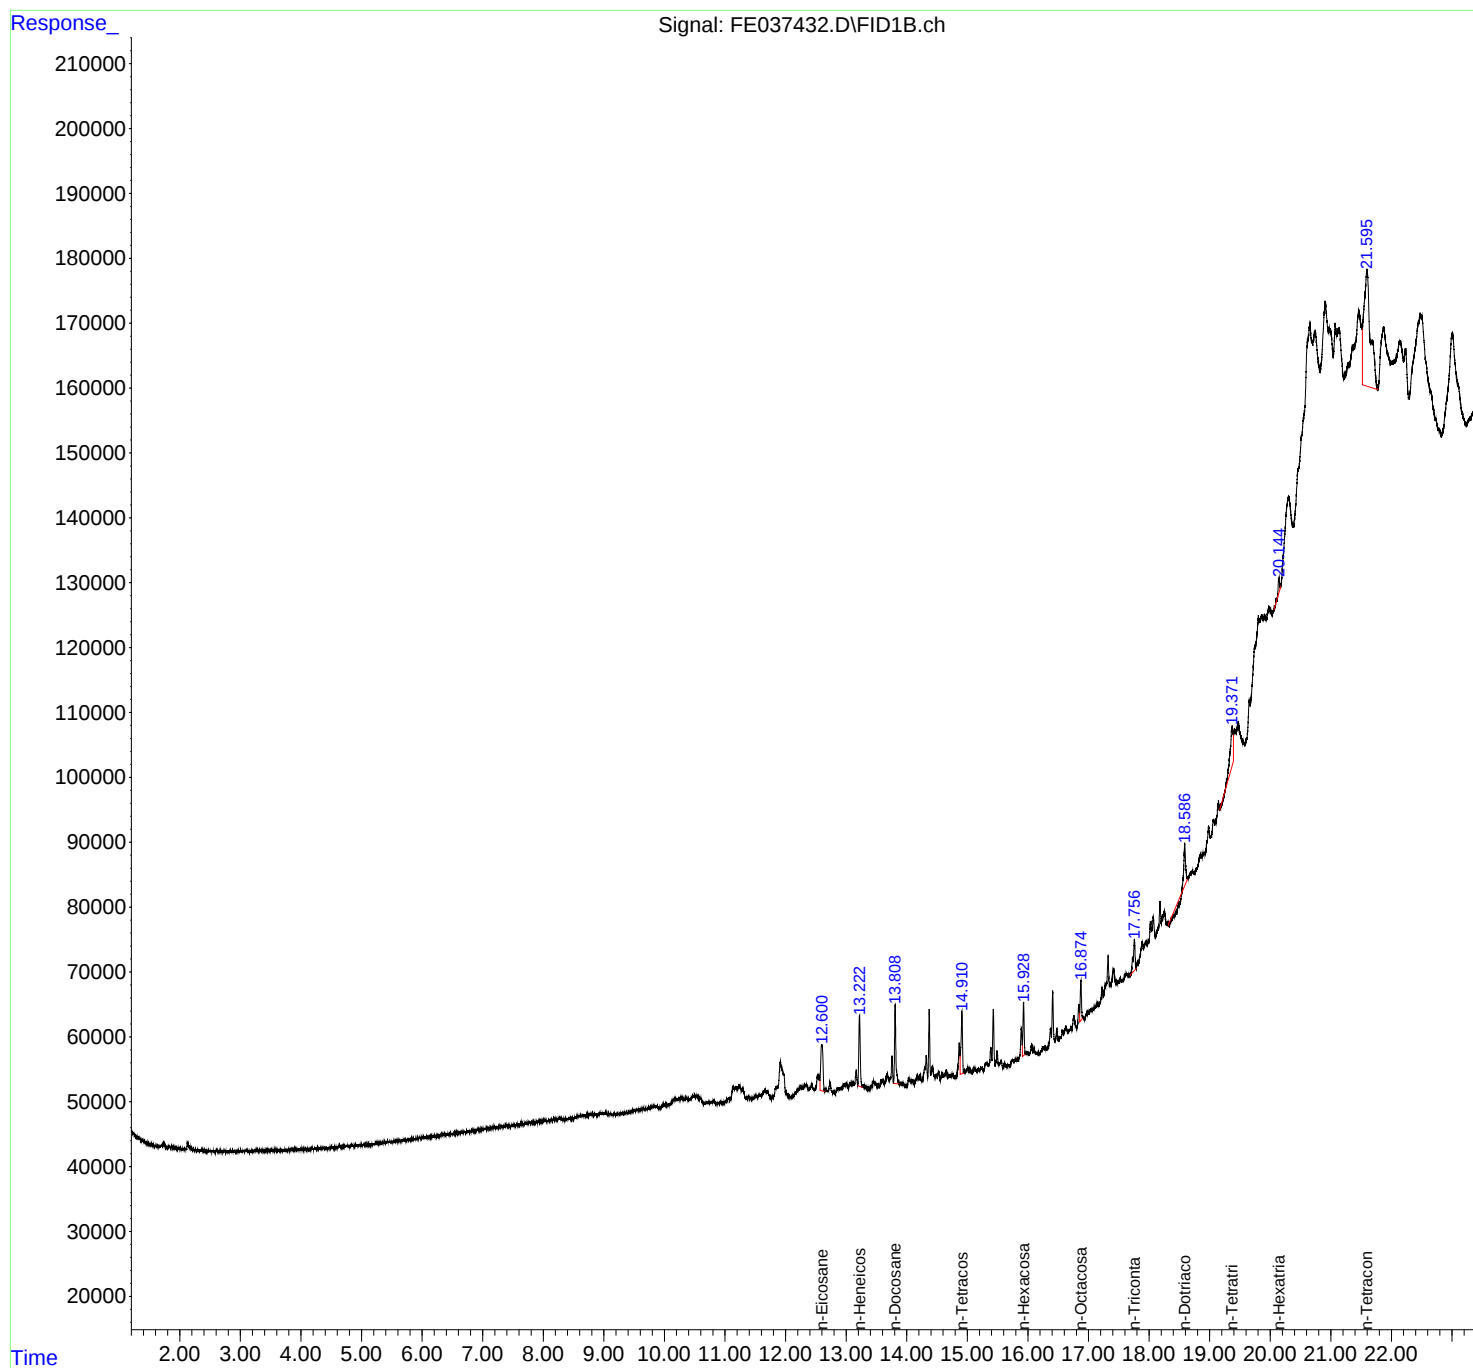


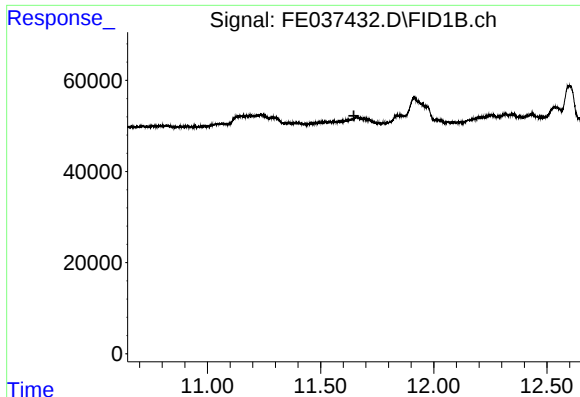

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.647 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

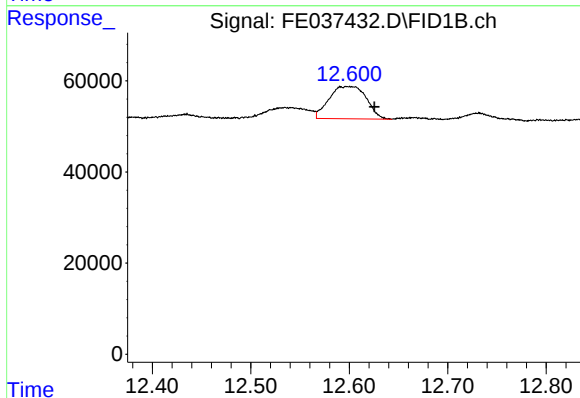


#10 n-Eicosane (C20)

R.T.: 12.598 min
Delta R.T.: -0.027 min
Response: 186450
Conc: 1.18 ug/ml

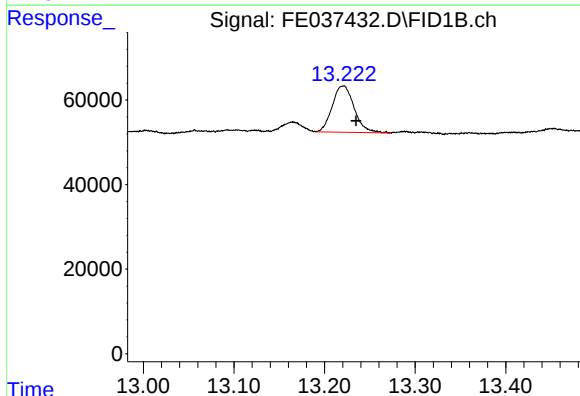


#11 n-Heneicosane (C21)

R.T.: 13.221 min
Delta R.T.: -0.014 min
Response: 184412
Conc: 1.17 ug/ml

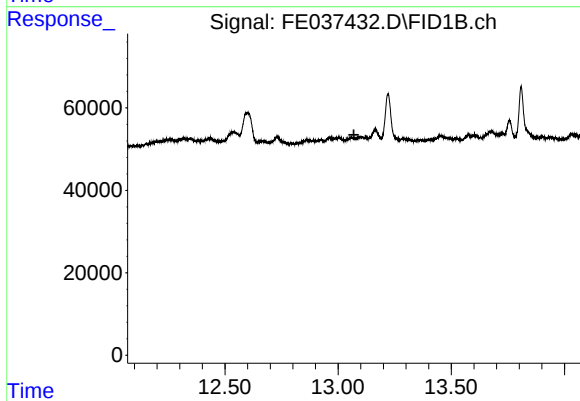

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.070 min
Response: 0
Conc: N.D.

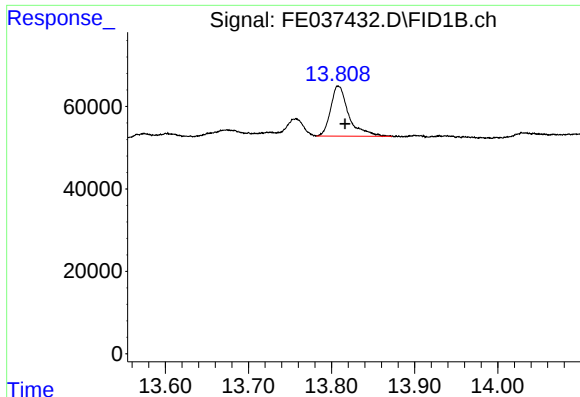

#13 n-Docosane (C22)


R.T.: 13.808 min
Delta R.T.: -0.008 min
Response: 184177
Conc: 1.18 ug/ml

Instrument :
FID_E
ClientSampleId :

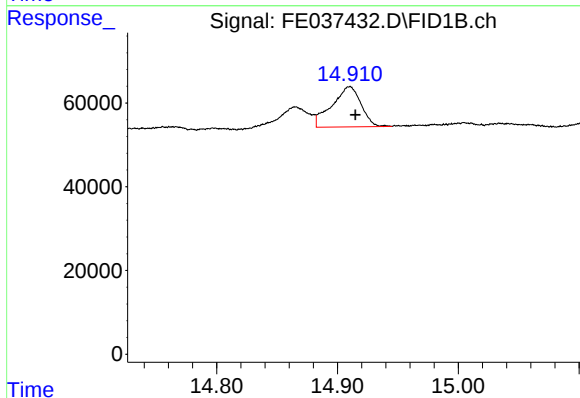


#14 n-Tetracosane (C24)

R.T.: 14.910 min
Delta R.T.: -0.005 min
Response: 160793
Conc: 1.07 ug/ml

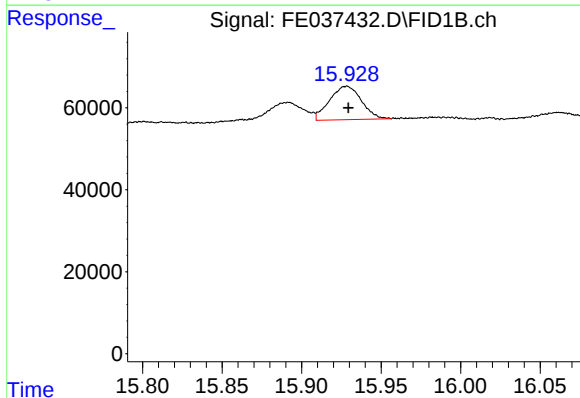


#15 n-Hexacosane (C26)

R.T.: 15.928 min
Delta R.T.: -0.001 min
Response: 113951
Conc: 0.79 ug/ml

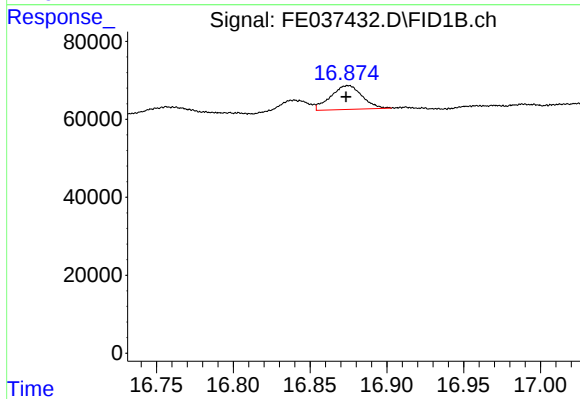

#16 n-Octacosane (C28)


R.T.: 16.875 min
Delta R.T.: 0.001 min
Response: 87130
Conc: 0.63 ug/ml

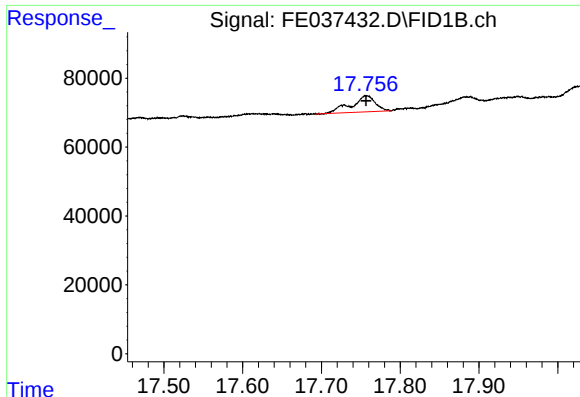

#17 n-Tricontane (C30)


R.T.: 17.757 min
Delta R.T.: 0.000 min
Response: 100085
Conc: 0.74 ug/ml

Instrument :
FID_E
ClientSampleId :

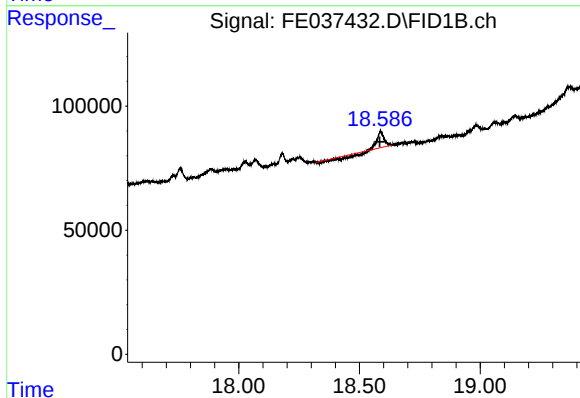


#18 n-Dotriacontane (C32)

R.T.: 18.587 min
Delta R.T.: 0.003 min
Response: 58678
Conc: 0.44 ug/ml

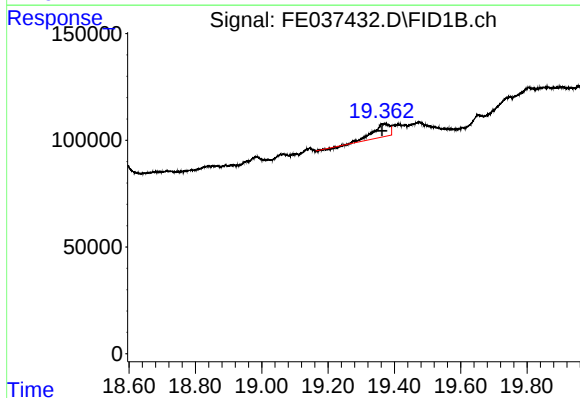


#19 n-Tetratriacontane (C34)

R.T.: 19.371 min
Delta R.T.: 0.008 min
Response: 210032
Conc: 1.66 ug/ml

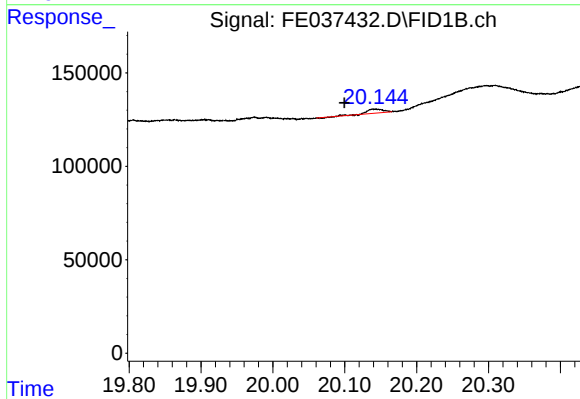

#20 n-Hexatriacontane (C36)

R.T.: 20.142 min
Delta R.T.: 0.042 min
Response: 31840
Conc: 0.25 ug/ml

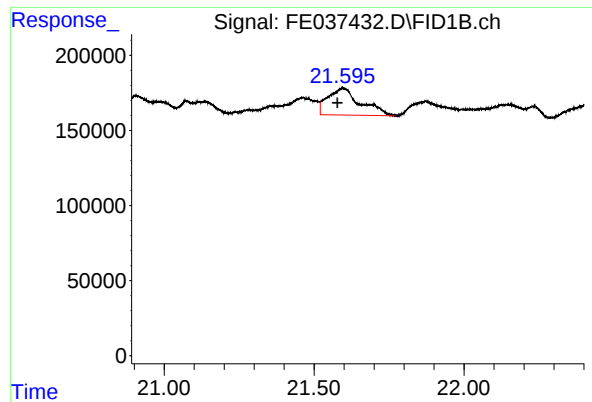

#22 n-Tetracontane (C40)

R.T.: 21.596 min
Delta R.T.: 0.018 min
Response: 1352223
Conc: 10.49 ug/ml

Instrument :
FID_E
ClientSampleId :