

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090723AL\
Data File : FE044120.D
Signal(s) : FID1B.ch
Acq On : 07 Sep 2023 09:07
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 08 01:15:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 083023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 31 03:37:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13) T	n-Docosane (C22)	14.119	163736	1.025 ug/ml
14) T	n-Tetracosane (C24)	15.231	120089	0.768 ug/ml
15) T	n-Hexacosane (C26)	16.256	104612	0.694 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090723AL\
Data File : FE044120.D
Signal(s) : FID1B.ch
Acq On : 07 Sep 2023 09:07
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 08 01:15:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 083023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 31 03:37:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

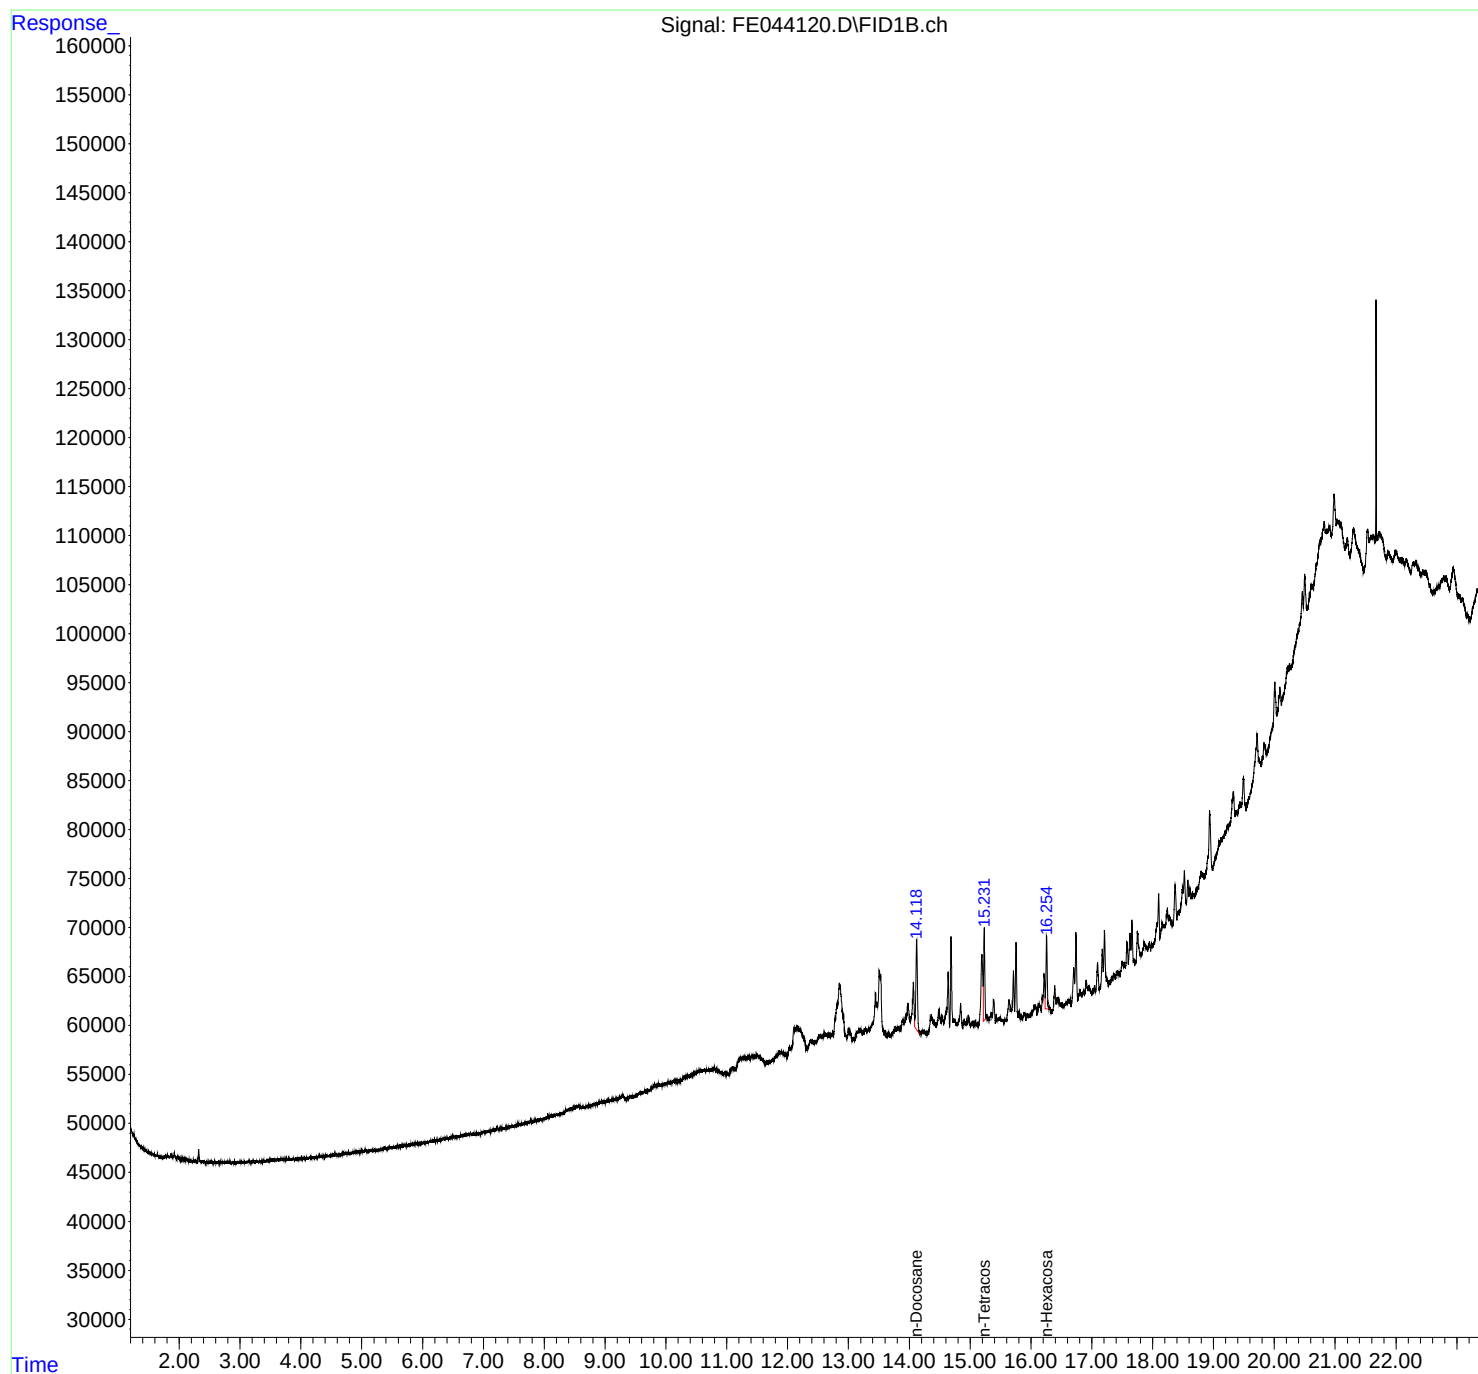


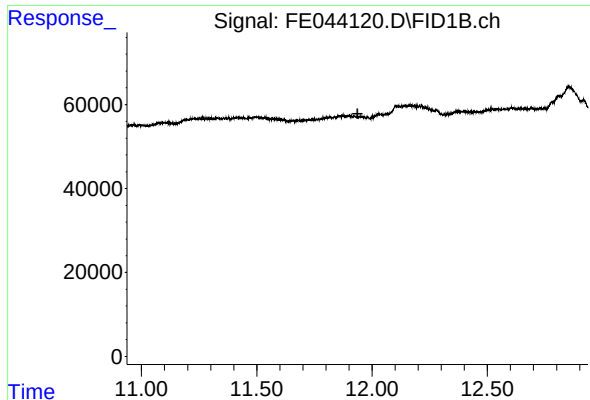

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.937 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

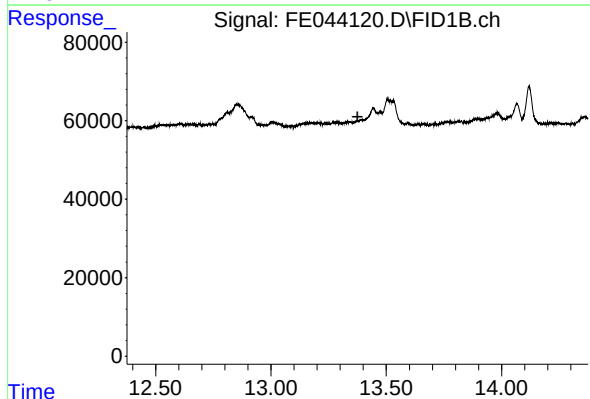


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.375 min
Response: 0
Conc: N.D.

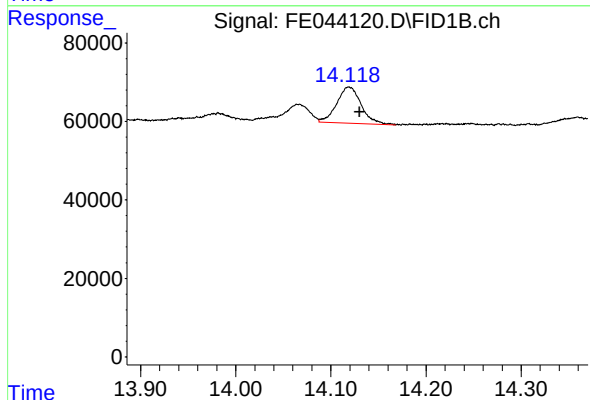


#13 n-Docosane (C22)

R.T.: 14.119 min
Delta R.T.: -0.011 min
Response: 163736
Conc: 1.02 ug/ml

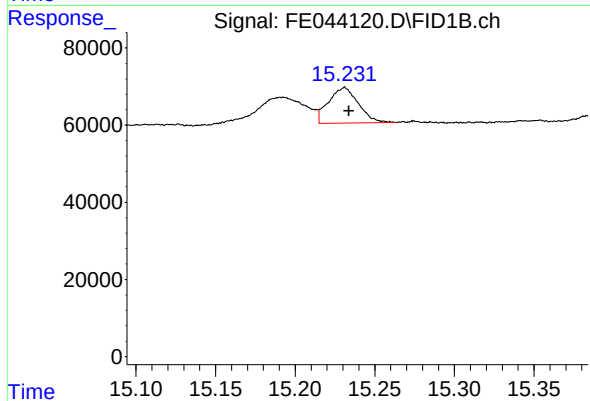

#14 n-Tetracosane (C24)

R.T.: 15.231 min
Delta R.T.: -0.003 min
Response: 120089
Conc: 0.77 ug/ml

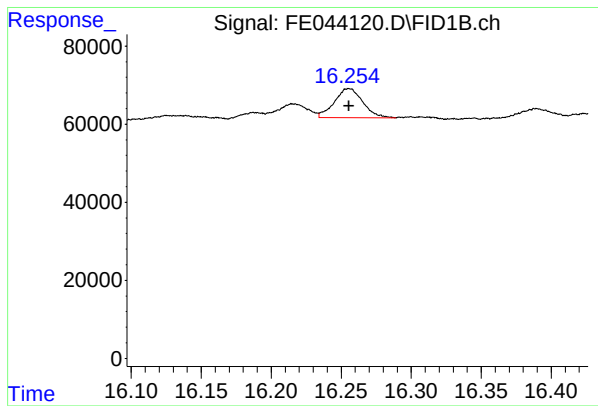

#15 n-Hexacosane (C26)

R.T.: 16.256 min
Delta R.T.: 0.000 min
Response: 104612
Conc: 0.69 ug/ml

Instrument :

FID_E

ClientSampleId :