

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090819\
 Data File : FE030348.D
 Signal(s) : FID1B.CH
 Acq On : 07 Sep 2019 12:37
 Operator : DD\AJ
 Sample : 4400 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 07 13:30:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Sat Sep 07 13:29:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.567	10388141	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.342	73423157	400.000 ug/ml
2) N-NONANE	3.307	74986351	400.000 ug/ml
3) N-DECANE	4.362	115952035	400.000 ug/ml
4) N-UNDECANE	5.392	117292606	600.000 ug/ml
5) N-DODECANE	6.373	117558559	600.000 ug/ml
6) N-TETRADECANE	8.171	119609258	600.000 ug/ml
7) N-HEXADECANE	9.767	100298965	500.000 ug/ml
8) N-OCTADECANE	11.189	50149559	250.000 ug/ml
9) N-EICOSANE	12.479	20056049	100.000 ug/ml
10) N-TETRACOSANE	14.783	19887694	100.000 ug/ml
11) N-OCTACOSANE	16.742	9683622	50.000 ug/ml
12) N-DOTRIACONTANE	18.464	9046048	50.000 ug/ml
14) N-HEXATRIACONTANE	19.987	8024751	50.000 ug/ml
15) N-TETRACONTANE	21.559	6515699	50.000 ug/ml
16) N-TETRTETRACOOCTANE	24.114	4790650	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090819\
Data File : FE030348.D
Signal(s) : FID1B.CH
Acq On : 07 Sep 2019 12:37
Operator : DD\AJ
Sample : 4400 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 07 13:30:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Sat Sep 07 13:29:51 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

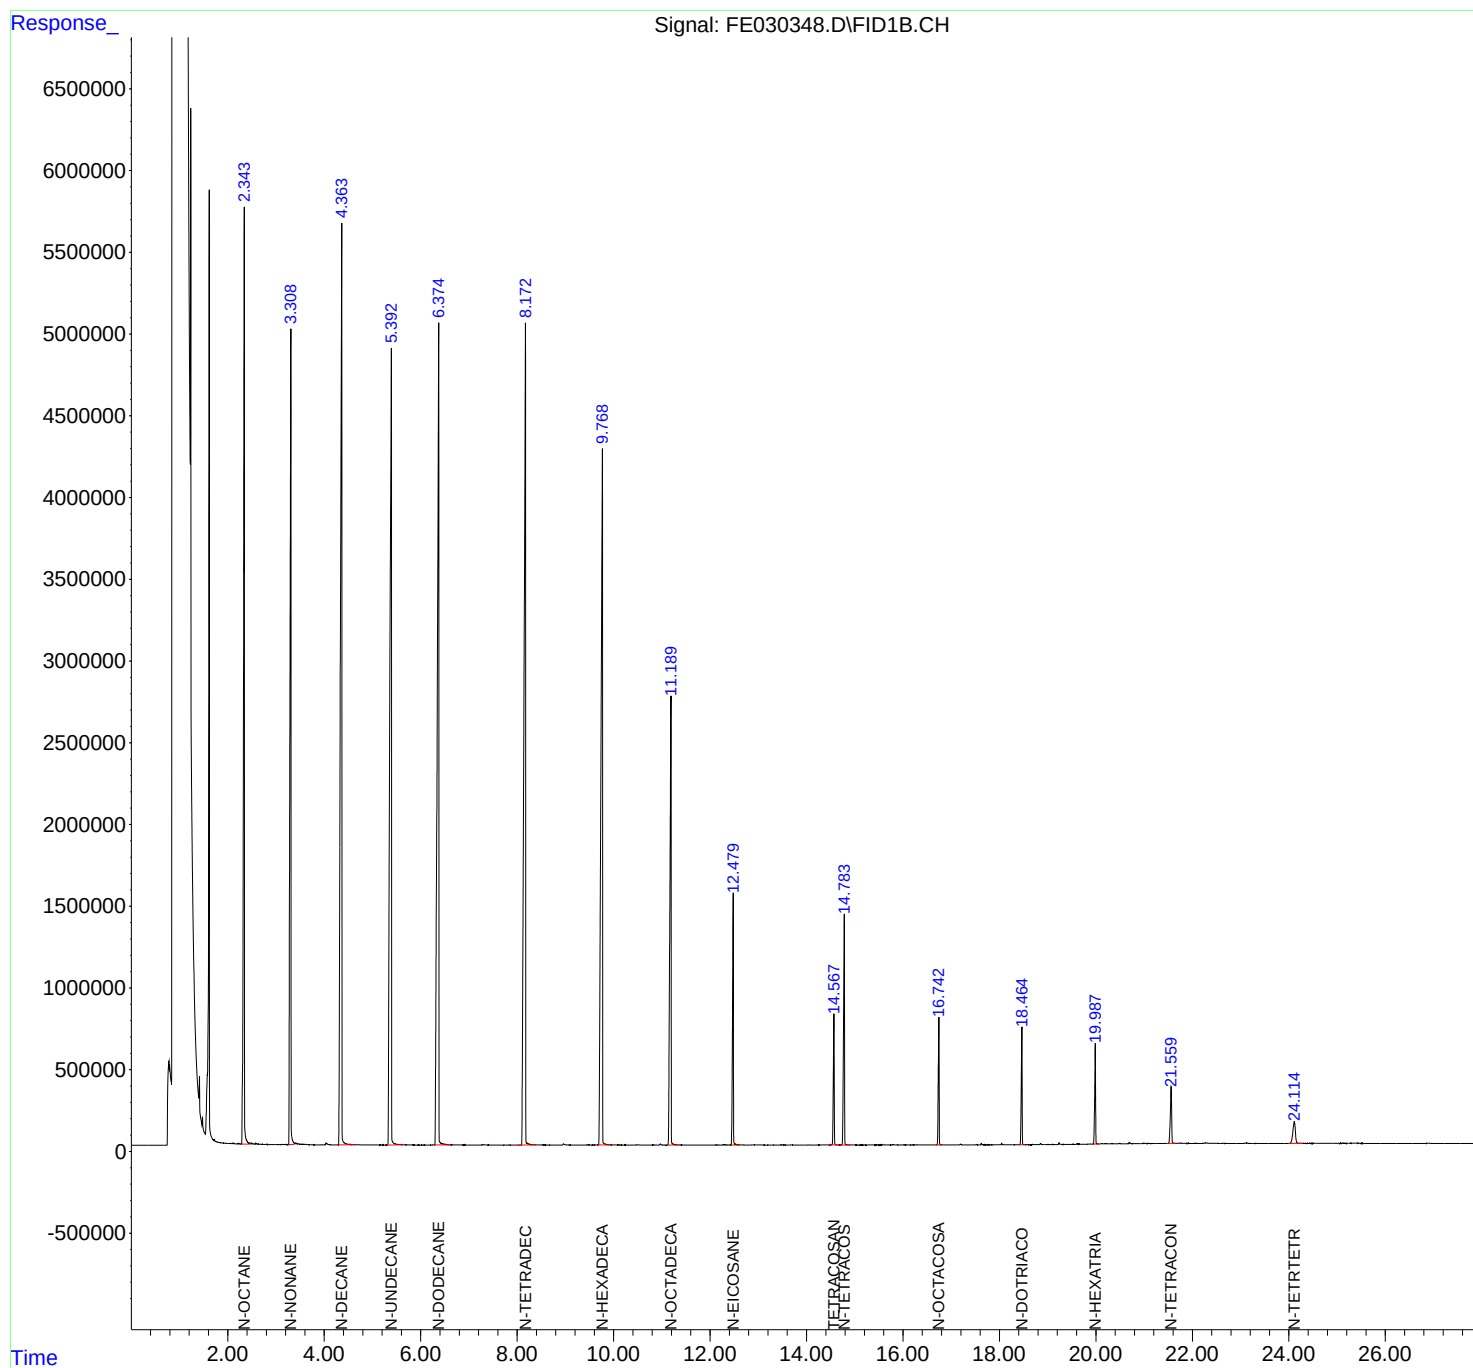

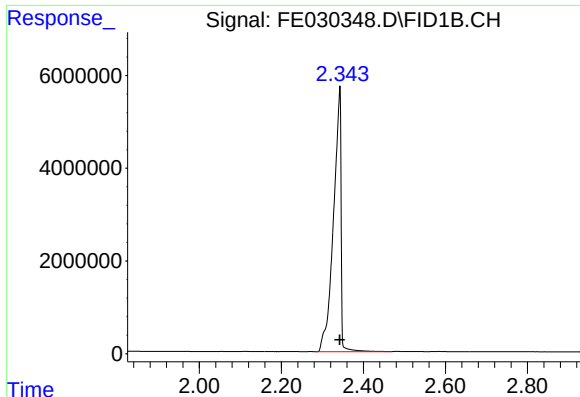


#1 N-OCTANE

R.T.: 2.342 min
Delta R.T.: 0.000 min
Response: 73423157
Conc: 400.00 ug/ml

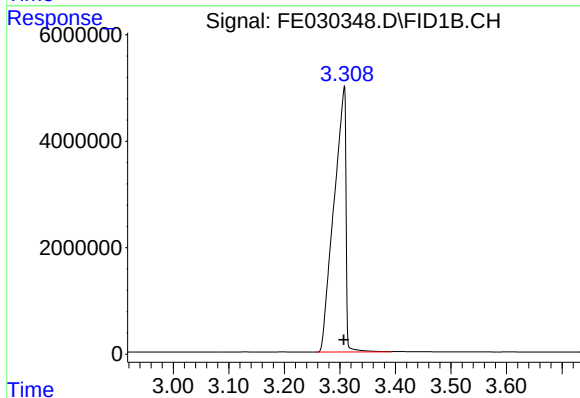


#2 N-NONANE

R.T.: 3.307 min
Delta R.T.: 0.000 min
Response: 74986351
Conc: 400.00 ug/ml

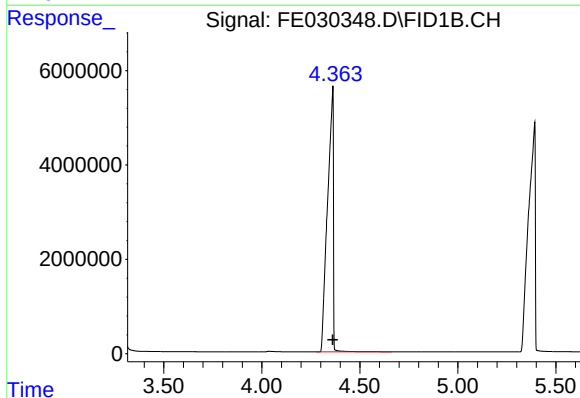


#3 N-DECANE

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 115952035
Conc: 400.00 ug/ml

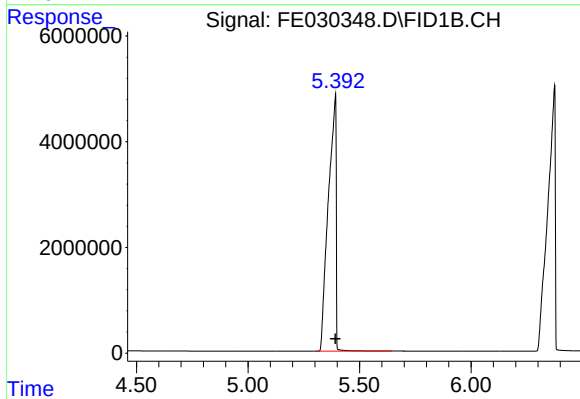


#4 N-UNDECANE

R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 117292606
Conc: 600.00 ug/ml

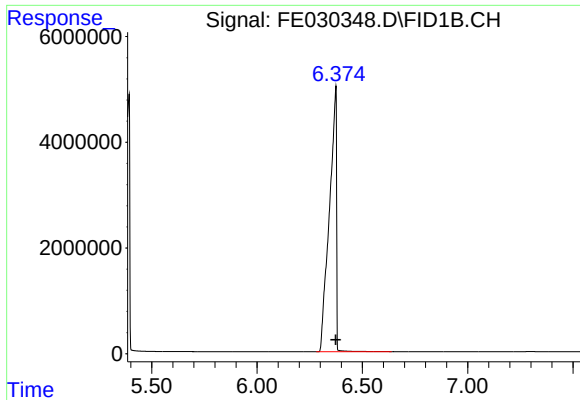


#5 N-DODECANE

R.T.: 6.373 min
Delta R.T.: 0.000 min
Response: 117558559
Conc: 600.00 ug/ml

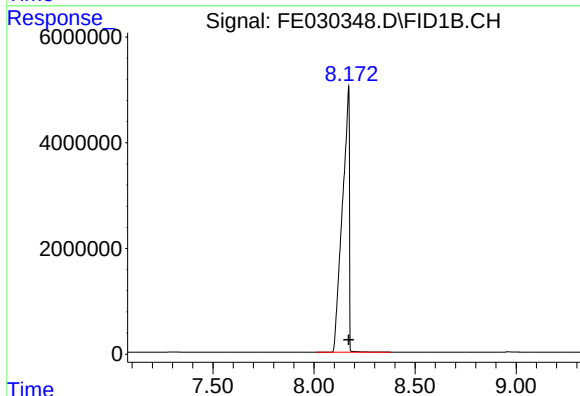


#6 N-TETRADECANE

R.T.: 8.171 min
Delta R.T.: 0.000 min
Response: 119609258
Conc: 600.00 ug/ml

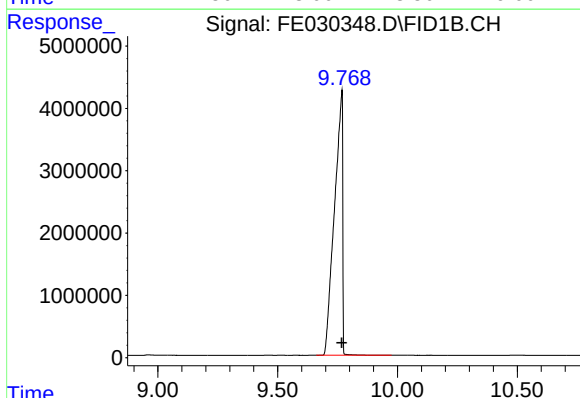


#7 N-HEXADECANE

R.T.: 9.767 min
Delta R.T.: 0.000 min
Response: 100298965
Conc: 500.00 ug/ml

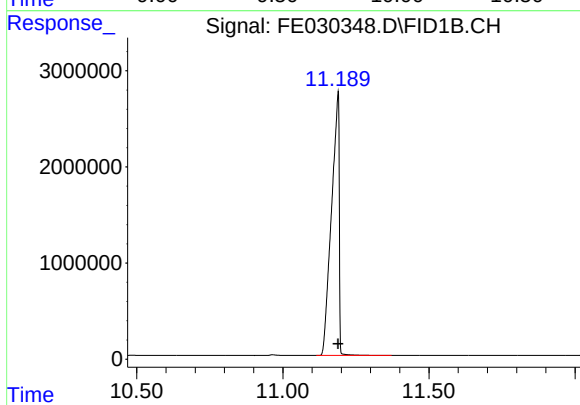


#8 N-OCTADECANE

R.T.: 11.189 min
Delta R.T.: 0.000 min
Response: 50149559
Conc: 250.00 ug/ml

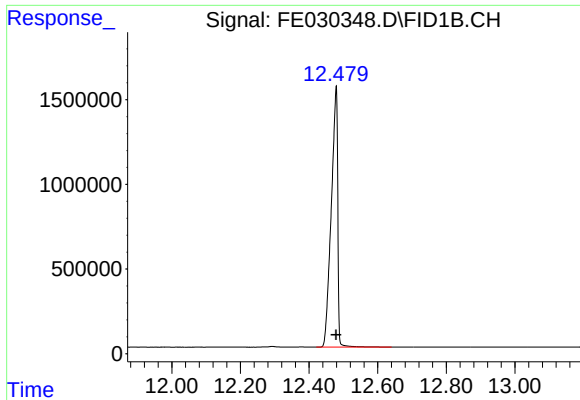


#9 N-EICOSANE

R.T.: 12.479 min
Delta R.T.: 0.000 min
Response: 20056049
Conc: 100.00 ug/ml

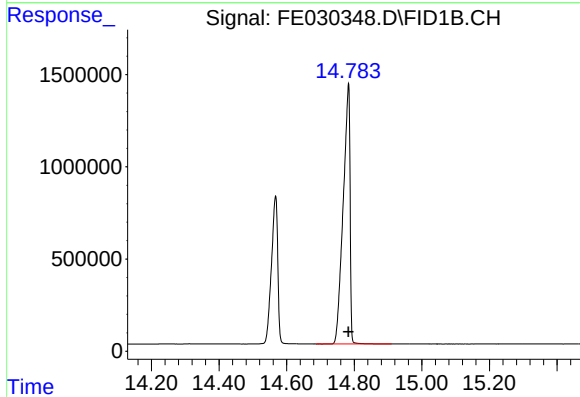


#10 N-TETRACOSANE

R.T.: 14.783 min
Delta R.T.: 0.000 min
Response: 19887694
Conc: 100.00 ug/ml

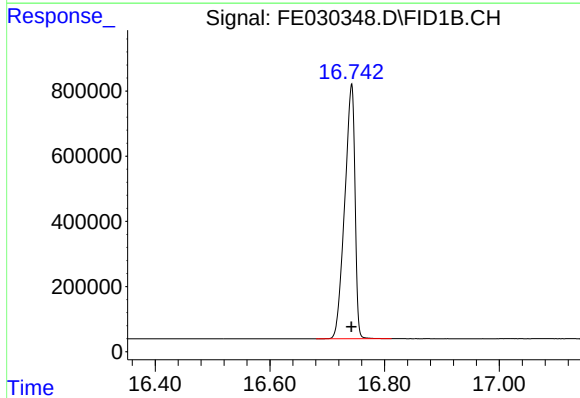


#11 N-OCTACOSANE

R.T.: 16.742 min
Delta R.T.: 0.000 min
Response: 9683622
Conc: 50.00 ug/ml

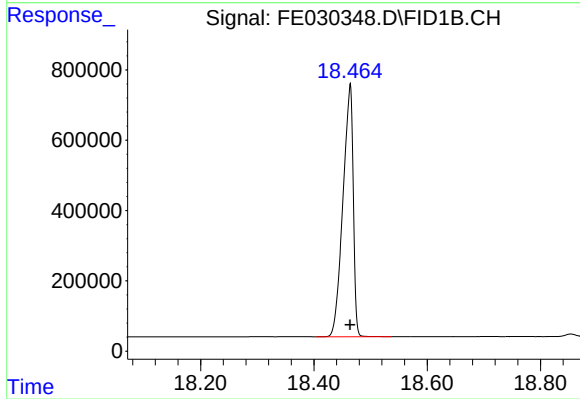


#12 N-DOTRIACONTANE

R.T.: 18.464 min
Delta R.T.: 0.000 min
Response: 9046048
Conc: 50.00 ug/ml

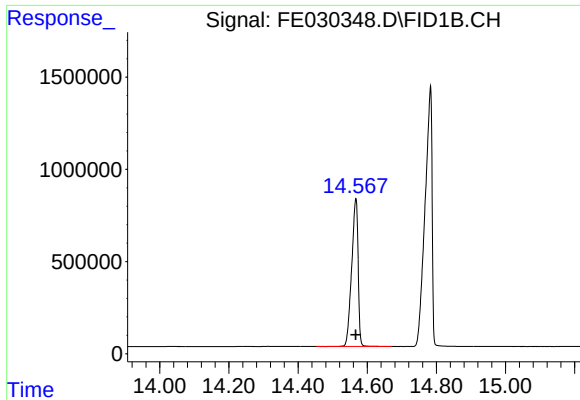


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.567 min
Delta R.T.: 0.000 min
Response: 10388141
Conc: 50.00 ug/ml

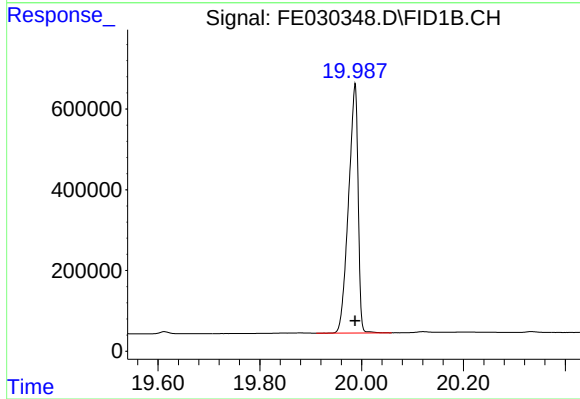


#14 N-HEXATRIACONTANE

R.T.: 19.987 min
Delta R.T.: 0.000 min
Response: 8024751
Conc: 50.00 ug/ml

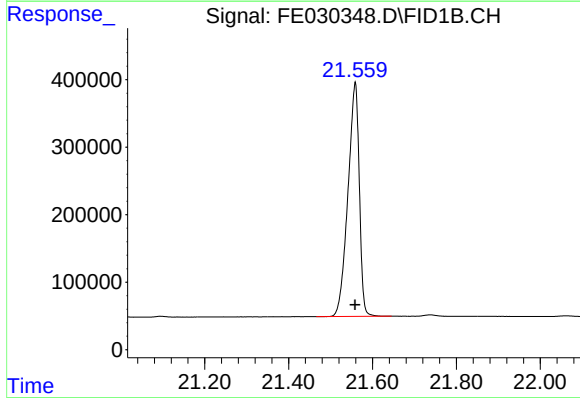

#15 N-TETRACONTANE

R.T.: 21.559 min
Delta R.T.: 0.000 min
Response: 6515699
Conc: 50.00 ug/ml

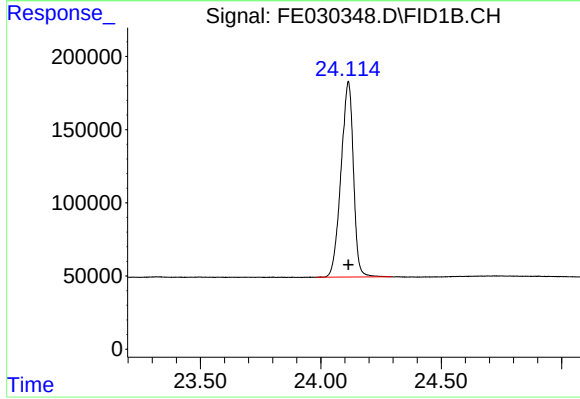

#16 N-TETRTETRACOOCTANE

R.T.: 24.114 min
Delta R.T.: 0.000 min
Response: 4790650
Conc: 50.00 ug/ml