

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090822AL\
 Data File : FE037473.D
 Signal(s) : FID1B.ch
 Acq On : 08 Sep 2022 21:01
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 09 08:19:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.589	36864	0.276 ug/ml
19) T	n-Tetratriacontane (C34)	19.372	83195	0.658 ug/ml
20) T	n-Hexatriacontane (C36)	20.055	26326	0.205 ug/ml
21) T	n-Octatriacontane (C38)	20.810	407360	3.273 ug/ml
22) T	n-Tetracontane (C40)	21.608	839108	6.509 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090822AL\
Data File : FE037473.D
Signal(s) : FID1B.ch
Acq On : 08 Sep 2022 21:01
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 09 08:19:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

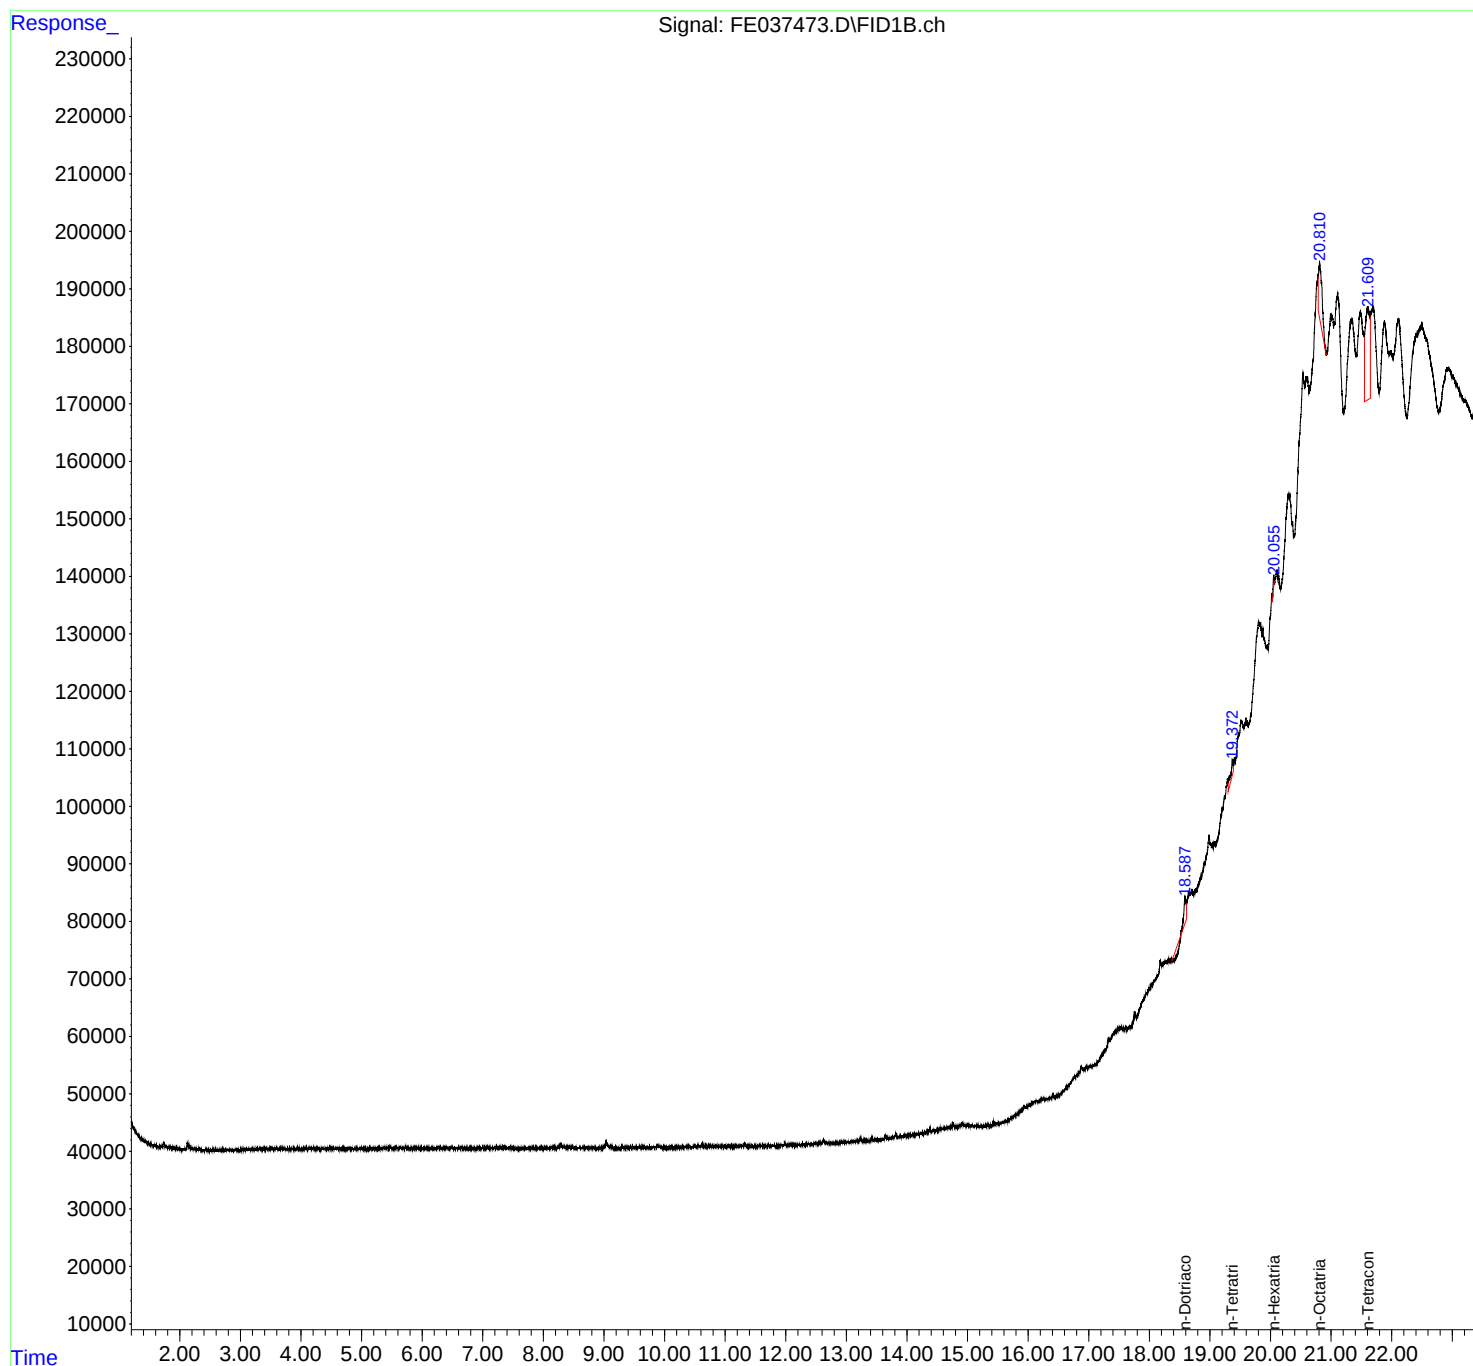


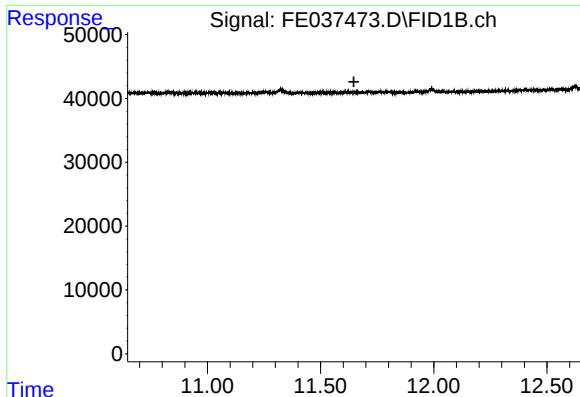

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.647 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

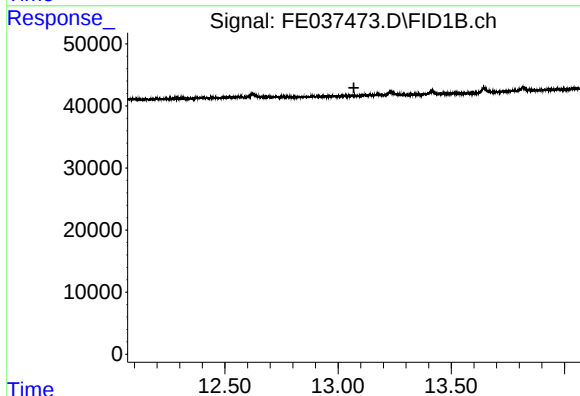


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.070 min
Response: 0
Conc: N.D.

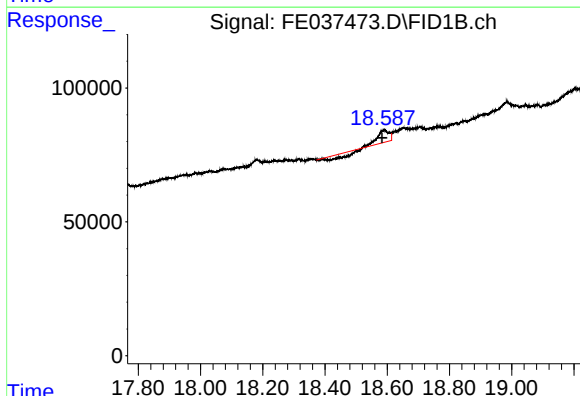


#18 n-Dotriacontane (C32)

R.T.: 18.589 min
Delta R.T.: 0.005 min
Response: 36864
Conc: 0.28 ug/ml

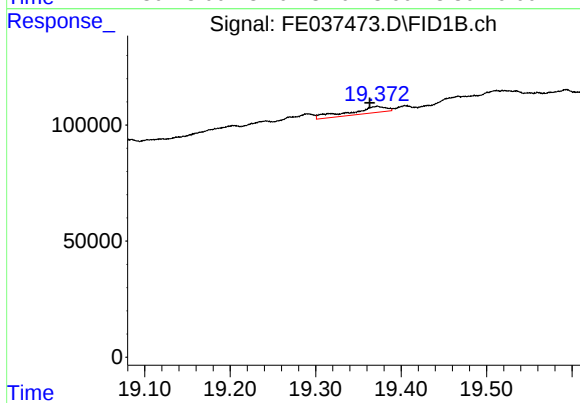

#19 n-Tetratriacontane (C34)


R.T.: 19.372 min
Delta R.T.: 0.009 min
Response: 83195
Conc: 0.66 ug/ml

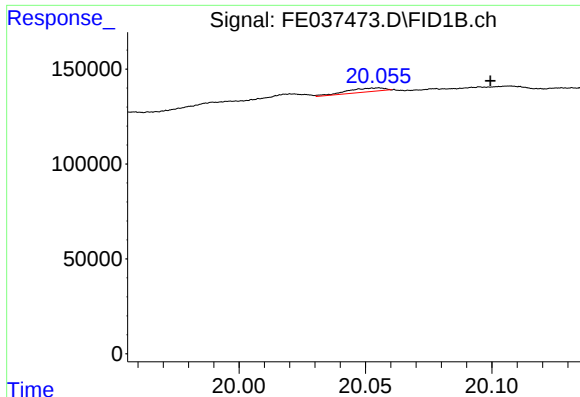

#20 n-Hexatriacontane (C36)


R.T.: 20.055 min
Delta R.T.: -0.044 min
Response: 26326
Conc: 0.20 ug/ml

Instrument :
FID_E
ClientSampleId :

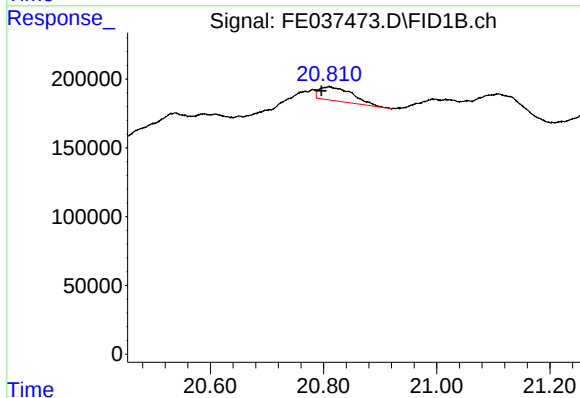

#21 n-Octatriacontane (C38)

R.T.: 20.810 min
Delta R.T.: 0.013 min
Response: 407360
Conc: 3.27 ug/ml

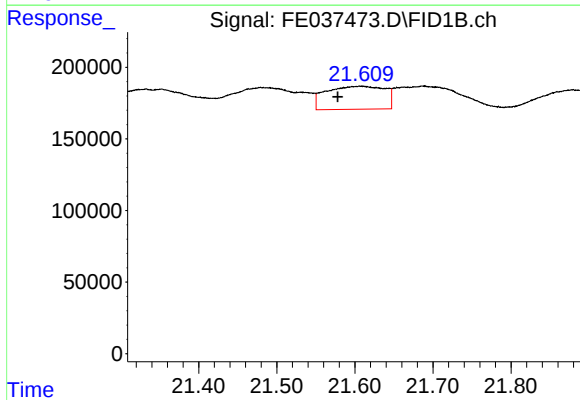

#22 n-Tetracontane (C40)

R.T.: 21.608 min
Delta R.T.: 0.030 min
Response: 839108
Conc: 6.51 ug/ml