

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090825AR\
 Data File : FG016562.D
 Signal(s) : FID1A.ch
 Acq On : 08 Sep 2025 11:42
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 09 03:55:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 082825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 29 05:03:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

14) T	Benzo[a]anthracene (C...	15.377	54070	0.422 ug/ml
15) T	Chrysene (C27.41)	15.377	54070	0.419 ug/ml
16) T	benzo[b]fluoranthene ...	16.912	4179	0.033 ug/ml
17) T	Bnezo[k]fluoranthene ...	16.912	4179	0.035 ug/ml
18) T	Benzo[a]pyrene (C31.34)	17.312	3248	0.026 ug/ml
19) T	Indeno[1,2,3-cd]pyren...	18.691	18891	0.164 ug/ml
20) T	Dibenz[a,h]anthracene...	18.691	18891	0.156 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG090825AR\
Data File : FG016562.D
Signal(s) : FID1A.ch
Acq On : 08 Sep 2025 11:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 09 03:55:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 082825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 05:03:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

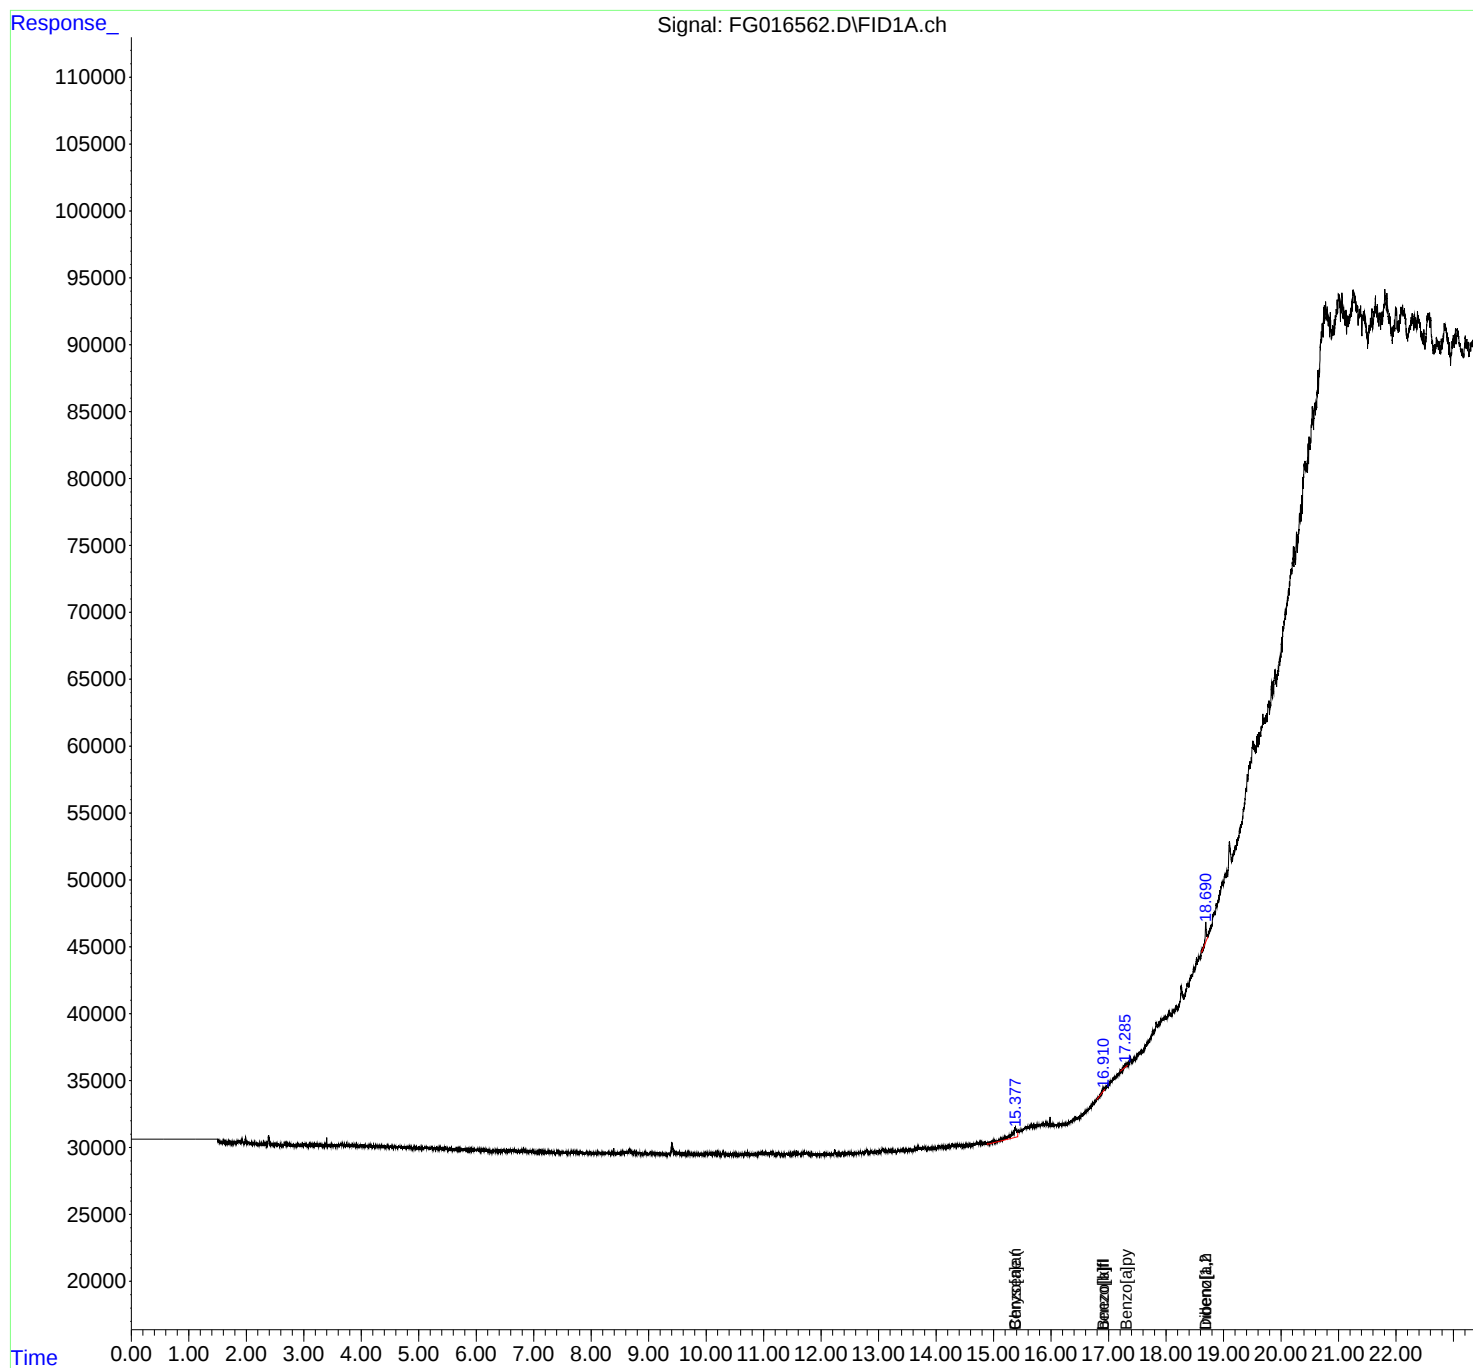


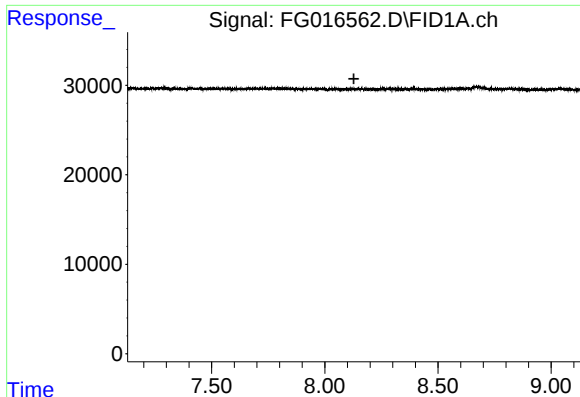

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

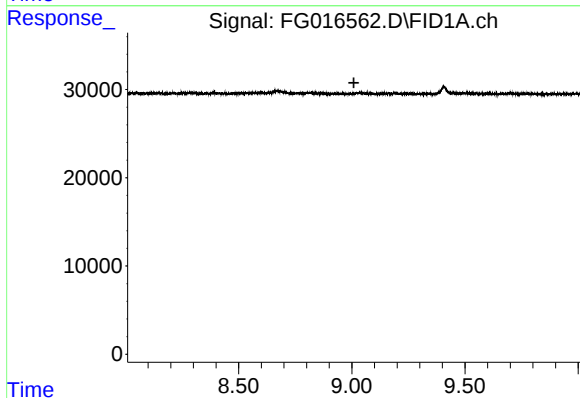


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 9.009 min
Response: 0
Conc: N.D.

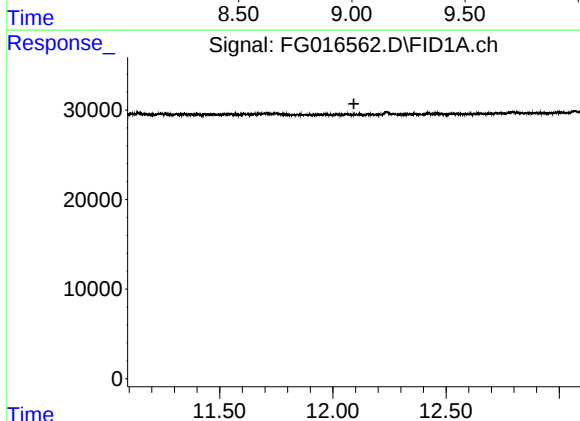


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 12.093 min
Response: 0
Conc: N.D.

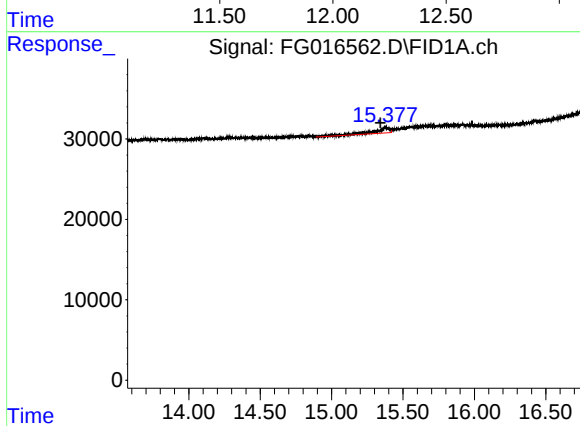

#14 Benzo[a]anthracene (C26.37)


R.T.: 15.377 min
Delta R.T.: 0.034 min
Response: 54070
Conc: 0.42 ug/ml

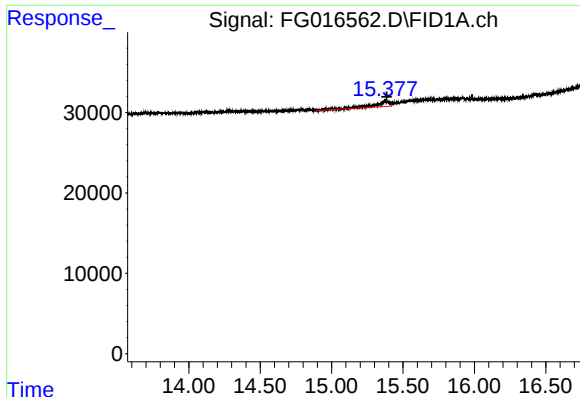

#15 Chrysene (C27.41)


R.T.: 15.377 min
Delta R.T.: -0.009 min
Response: 54070
Conc: 0.42 ug/ml

Instrument :
FID_E
ClientSampleId :

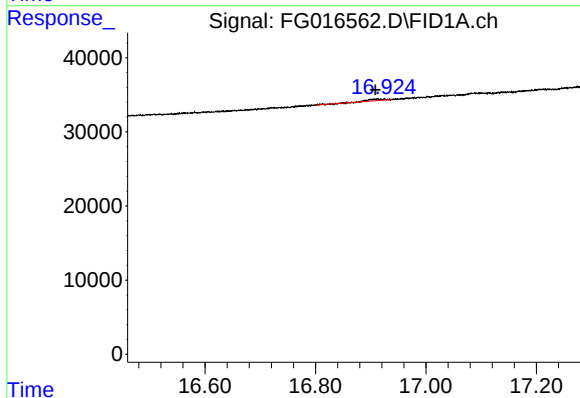


#16 benzo[b]fluoranthene (C30.41)

R.T.: 16.912 min
Delta R.T.: 0.003 min
Response: 4179
Conc: 0.03 ug/ml

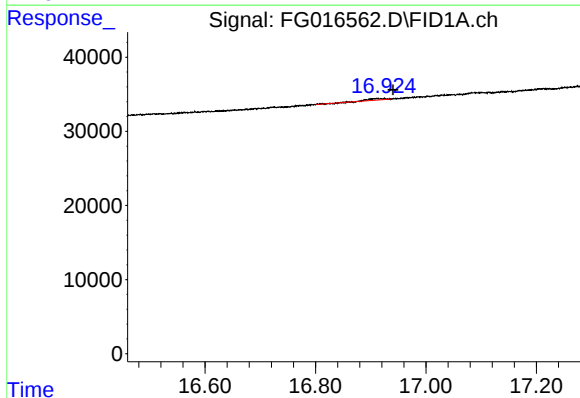


#17 Bnezo[k]fluoranthene (C30.14)

R.T.: 16.912 min
Delta R.T.: -0.029 min
Response: 4179
Conc: 0.03 ug/ml

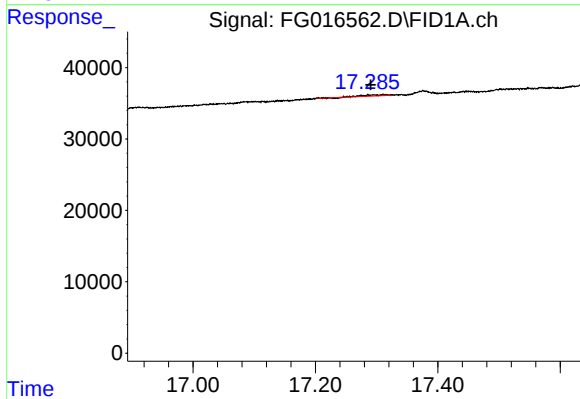

#18 Benzo[a]pyrene (C31.34)


R.T.: 17.312 min
Delta R.T.: 0.022 min
Response: 3248
Conc: 0.03 ug/ml

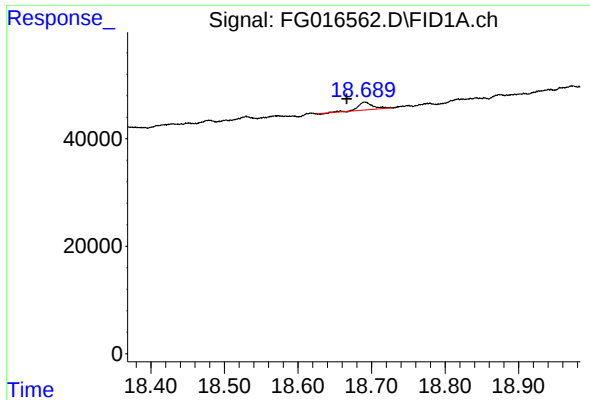

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.691 min
Delta R.T.: 0.025 min
Response: 18891
Conc: 0.16 ug/ml

Instrument :
FID_E
ClientSampleId :

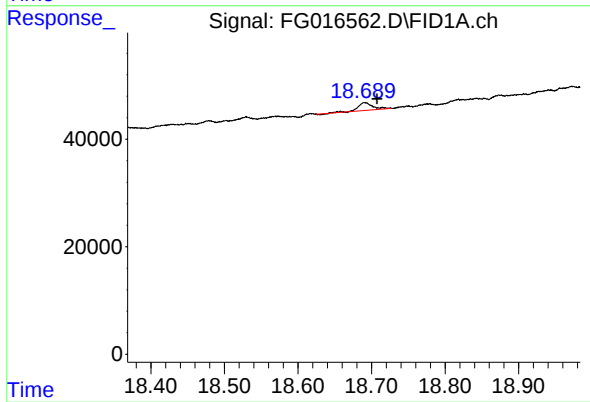

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.691 min
Delta R.T.: -0.016 min
Response: 18891
Conc: 0.16 ug/ml