

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030362.D
 Signal(s) : FID1B.CH
 Acq On : 09 Sep 2019 17:08
 Operator : DD\AJ
 Sample : K4757-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 A4

Integration File: autoint1.e
 Quant Time: Sep 10 05:46:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.552	3639835	18.290 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.756	77967	0.407 ug/ml
11) N-OCTACOSANE	16.722	275303	1.463 ug/ml
12) N-DOTRIACONTANE	18.439	354209	1.993 ug/ml
14) N-HEXATRIACONTANE	19.966	50451	0.318 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030362.D
Signal(s) : FID1B.CH
Acq On : 09 Sep 2019 17:08
Operator : DD\AJ
Sample : K4757-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
A4

Integration File: autoint1.e
Quant Time: Sep 10 05:46:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

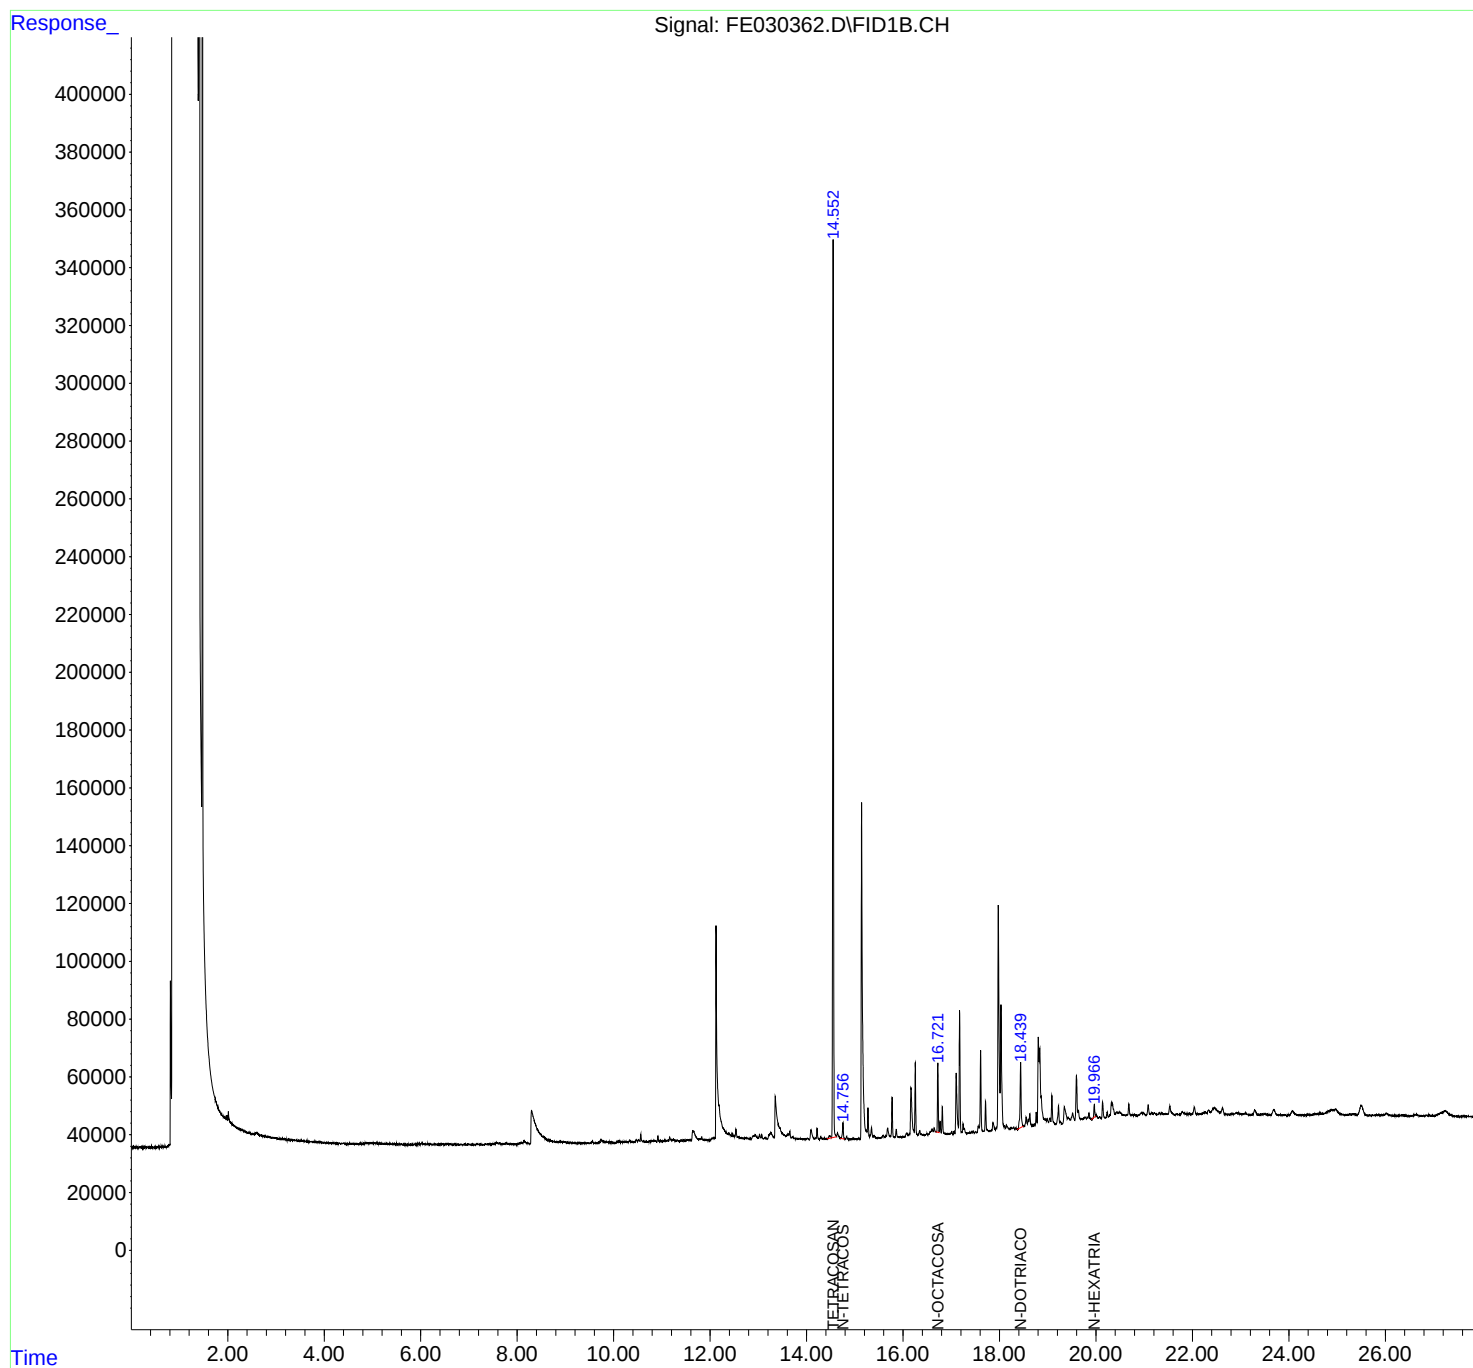


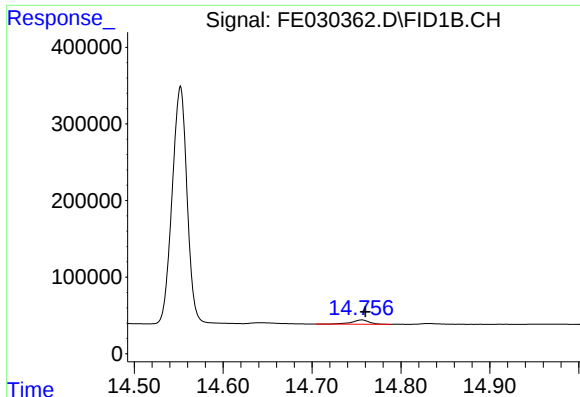

#10 N-TETRACOSANE


R.T.: 14.756 min
Delta R.T.: -0.004 min
Response: 77967
Conc: 0.41 ug/ml

Instrument :
FID_E
ClientSampleId :
A4

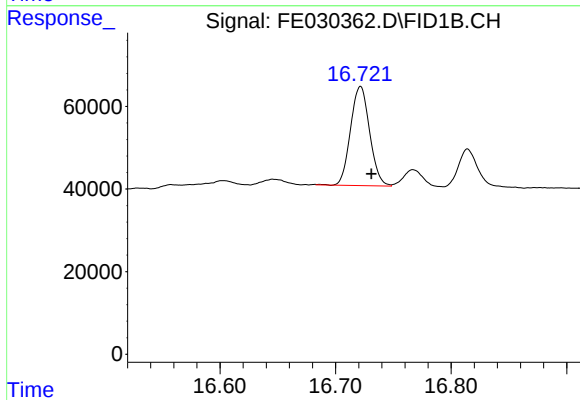


#11 N-OCTACOSANE

R.T.: 16.722 min
Delta R.T.: -0.009 min
Response: 275303
Conc: 1.46 ug/ml

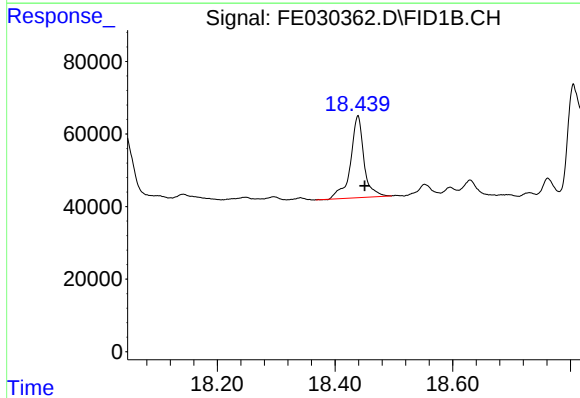


#12 N-DOTRIACONTANE

R.T.: 18.439 min
Delta R.T.: -0.011 min
Response: 354209
Conc: 1.99 ug/ml

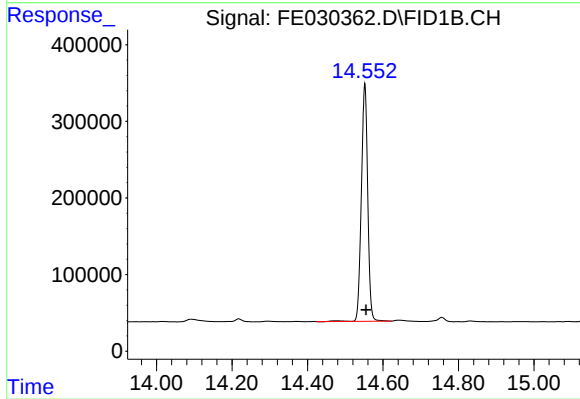

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.552 min
Delta R.T.: -0.003 min
Response: 3639835
Conc: 18.29 ug/ml

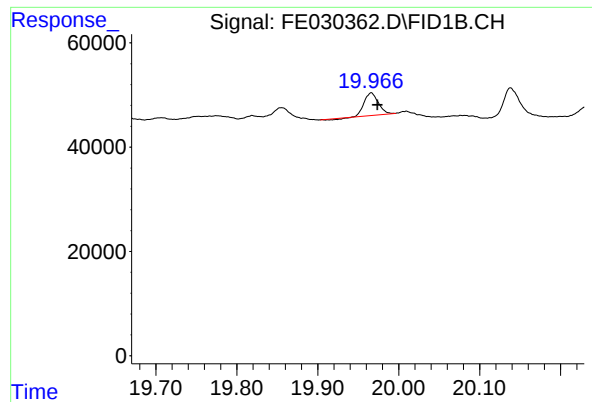

#14 N-HEXATRIACONTANE

R.T.: 19.966 min
Delta R.T.: -0.008 min
Response: 50451
Conc: 0.32 ug/ml

Instrument :
FID_E
ClientSampleId :
A4