

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030367.D
 Signal(s) : FID1B.CH
 Acq On : 09 Sep 2019 20:15
 Operator : DD\AJ
 Sample : K4757-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 A9

Integration File: autoint1.e
 Quant Time: Sep 10 05:47:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.552	4657932	23.406 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.754	68896	0.359 ug/ml
11)	N-OCTACOSANE	16.720	351575	1.868 ug/ml
12)	N-DOTRIACONTANE	18.436	463169	2.606 ug/ml
14)	N-HEXATRIACONTANE	19.963	73201	0.462 ug/ml
15)	N-TETRACONTANE	21.526	55120	0.395 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030367.D
Signal(s) : FID1B.CH
Acq On : 09 Sep 2019 20:15
Operator : DD\AJ
Sample : K4757-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
A9

Integration File: autoint1.e
Quant Time: Sep 10 05:47:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

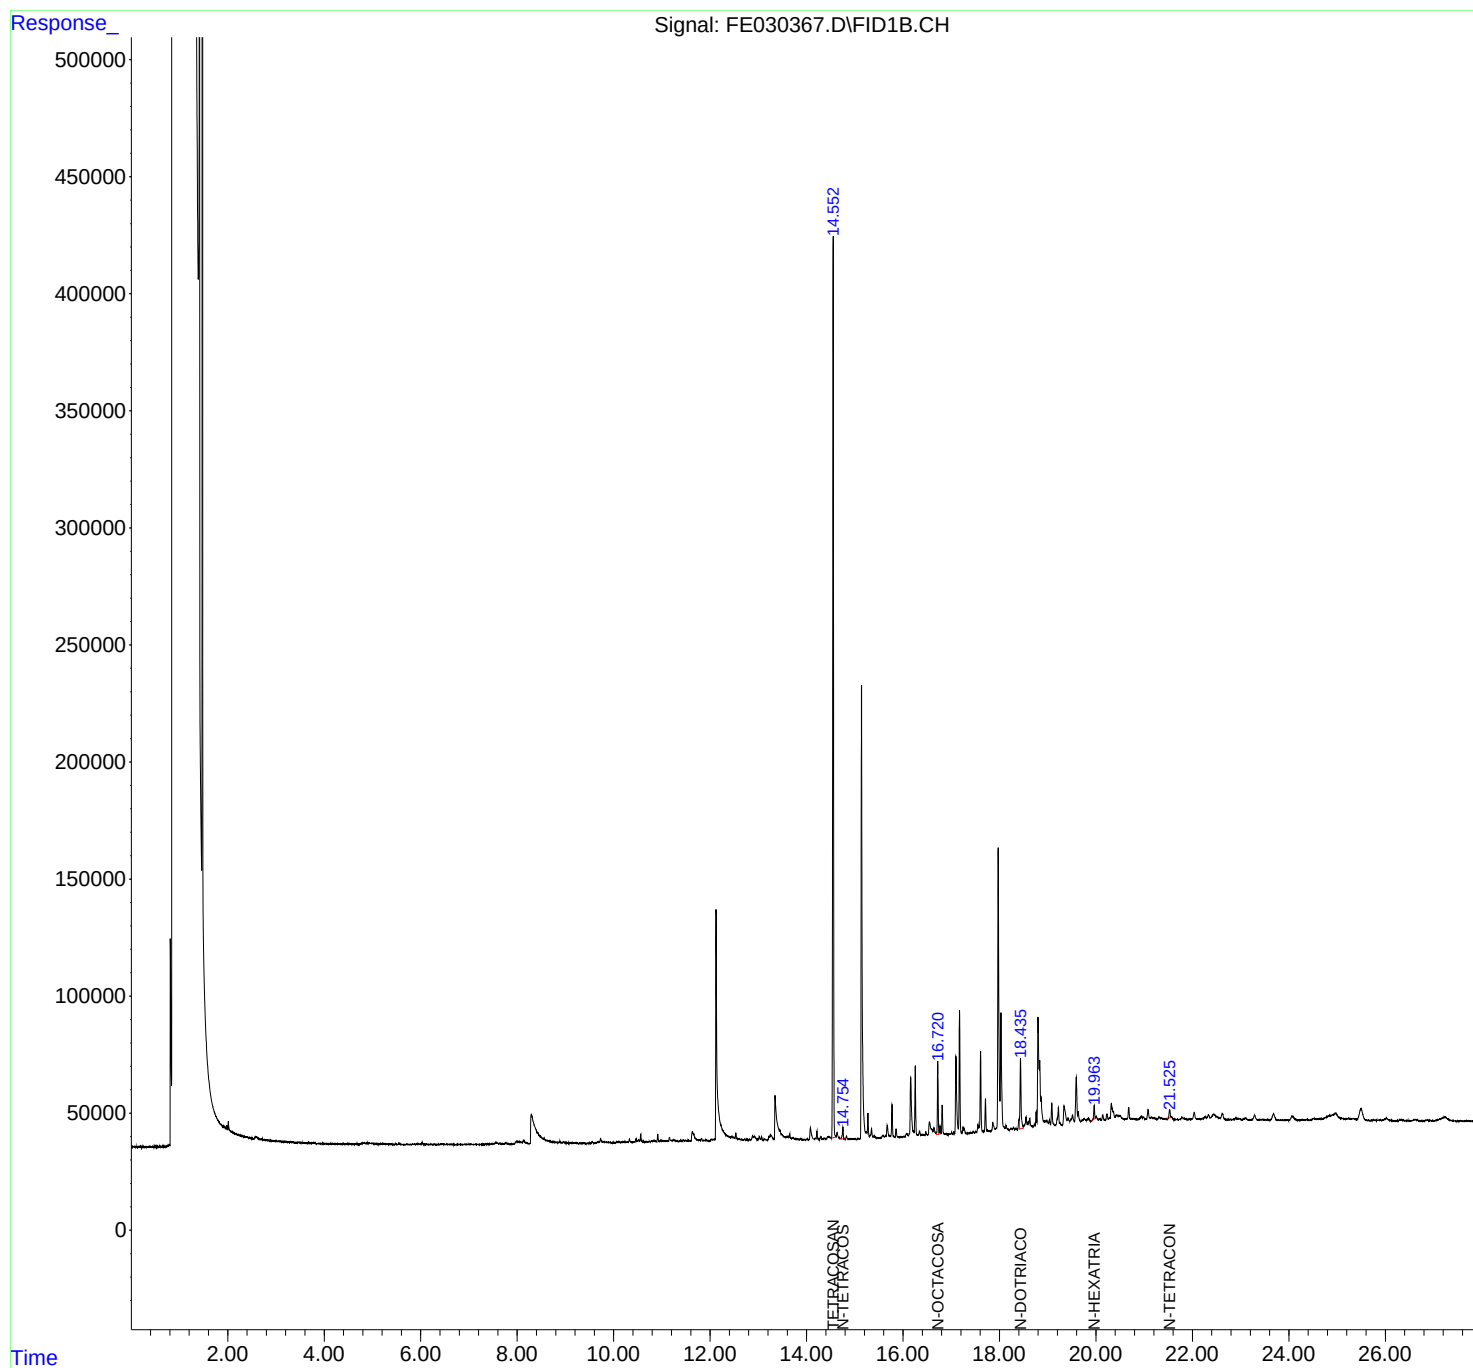


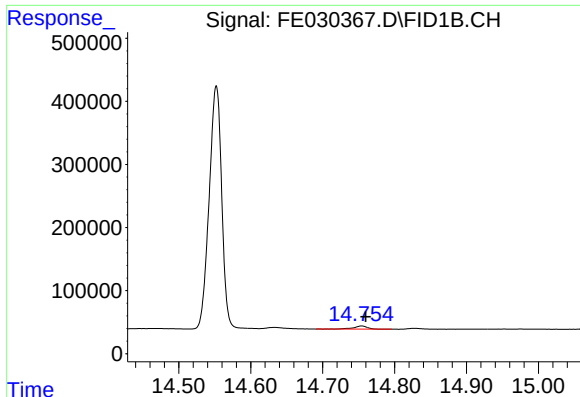

#10 N-TETRACOSANE


R.T.: 14.754 min
Delta R.T.: -0.006 min
Response: 68896
Conc: 0.36 ug/ml

Instrument :
FID_E
ClientSampleId :
A9

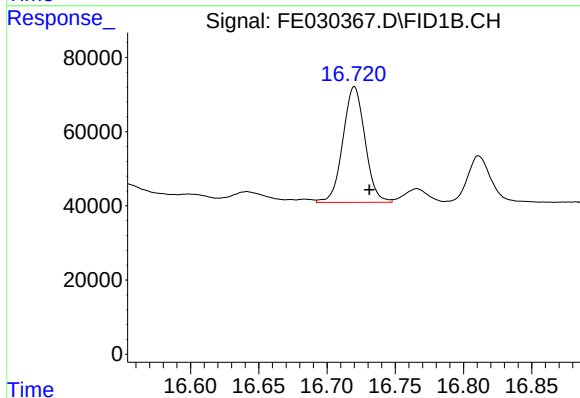


#11 N-OCTACOSANE

R.T.: 16.720 min
Delta R.T.: -0.011 min
Response: 351575
Conc: 1.87 ug/ml

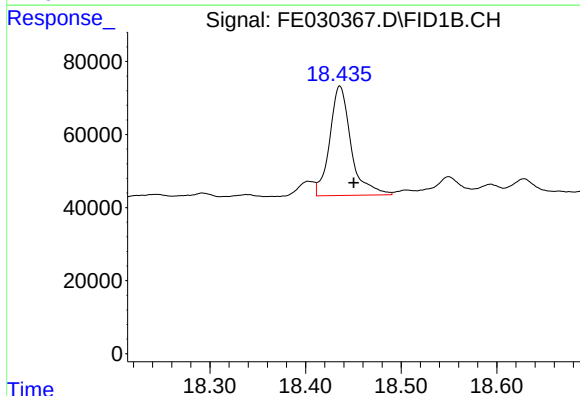


#12 N-DOTRIACONTANE

R.T.: 18.436 min
Delta R.T.: -0.015 min
Response: 463169
Conc: 2.61 ug/ml

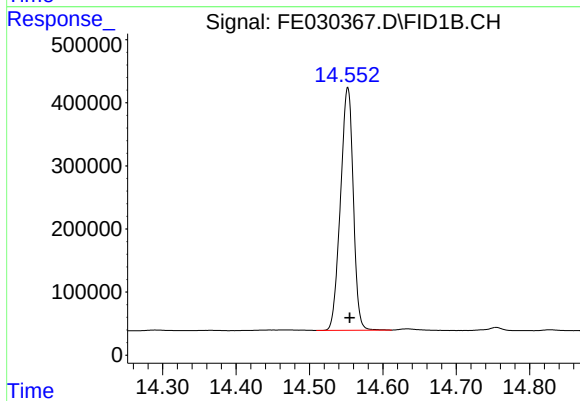

#13 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.552 min
Delta R.T.: -0.003 min
Response: 4657932
Conc: 23.41 ug/ml

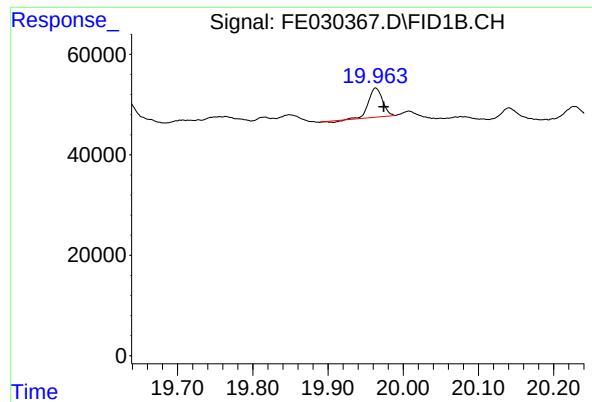

#14 N-HEXATRIACONTANE

R.T.: 19.963 min
Delta R.T.: -0.011 min
Response: 73201
Conc: 0.46 ug/ml

Instrument :
FID_E
ClientSampleId :
A9

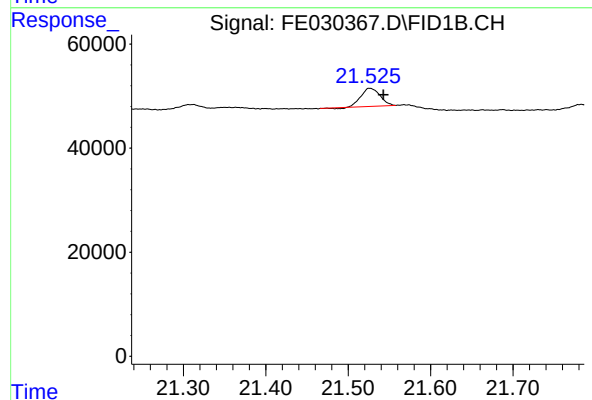

#15 N-TETRACONTANE

R.T.: 21.526 min
Delta R.T.: -0.016 min
Response: 55120
Conc: 0.39 ug/ml