

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE090919\  
 Data File : FE030370.D  
 Signal(s) : FID1B.CH  
 Acq On : 09 Sep 2019 22:44  
 Operator : DD\AJ  
 Sample : K4757-15  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 A11

Integration File: autoint1.e  
 Quant Time: Sep 10 05:48:07 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE090819.M  
 Quant Title :  
 QLast Update : Mon Sep 09 04:07:04 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20m x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units   |
|--------------------------------|--------|----------|--------------|
| -----                          |        |          |              |
| System Monitoring Compounds    |        |          |              |
| 13) S TETRACOSANE-d50 (SURR... | 14.549 | 2852553  | 14.334 ug/ml |
| Target Compounds               |        |          |              |
| 10) N-TETRACOSANE              | 14.754 | 81053    | 0.423 ug/ml  |
| 11) N-OCTACOSANE               | 16.720 | 523916   | 2.783 ug/ml  |
| 12) N-DOTRIACONTANE            | 18.438 | 468384   | 2.635 ug/ml  |
| 14) N-HEXATRIACONTANE          | 19.964 | 54385    | 0.343 ug/ml  |
| -----                          |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE090919\  
Data File : FE030370.D  
Signal(s) : FID1B.CH  
Acq On : 09 Sep 2019 22:44  
Operator : DD\AJ  
Sample : K4757-15  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
A11

Integration File: autoint1.e  
Quant Time: Sep 10 05:48:07 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE090819.M  
Quant Title :  
QLast Update : Mon Sep 09 04:07:04 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20m x 0.18mm x 0.18um

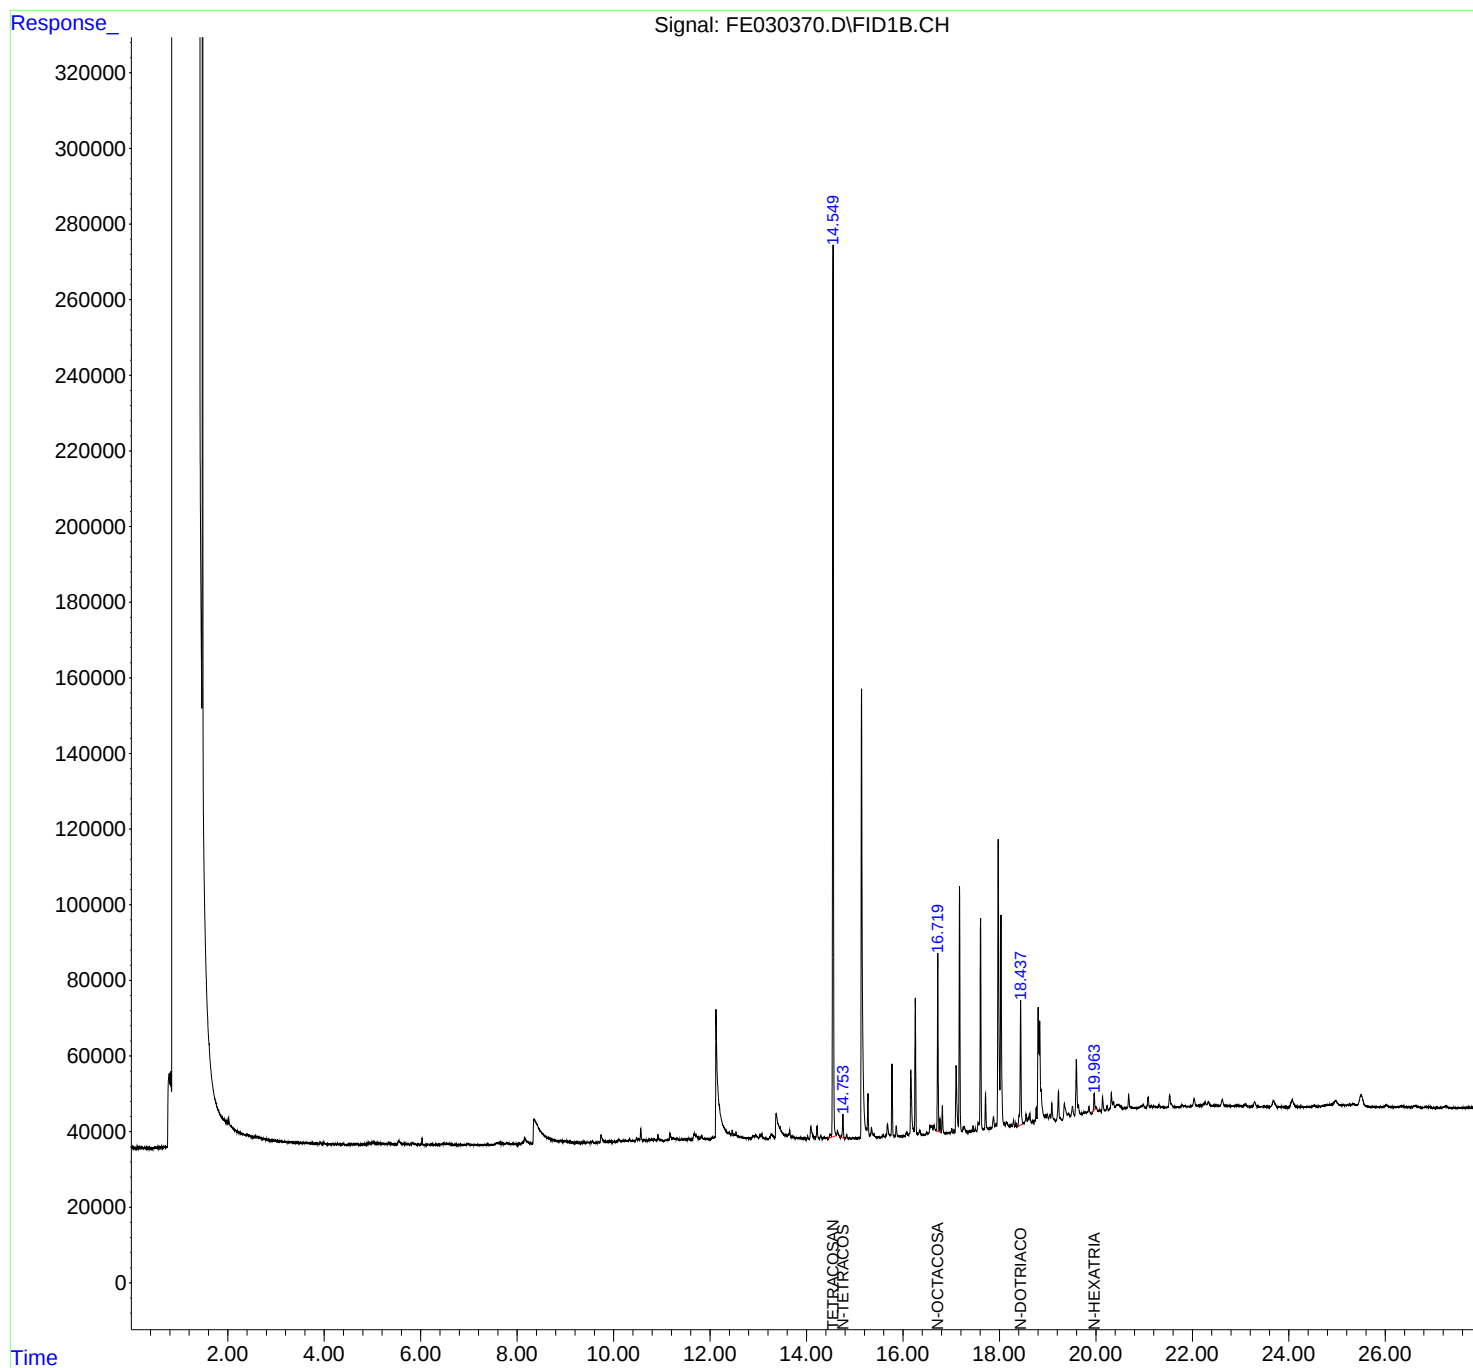


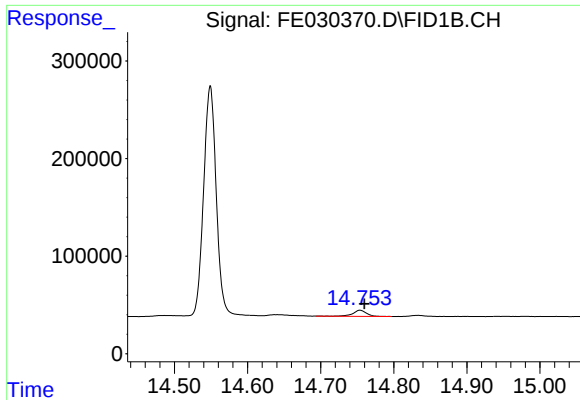

#10 N-TETRACOSANE


R.T.: 14.754 min  
Delta R.T.: -0.006 min  
Response: 81053  
Conc: 0.42 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
A11

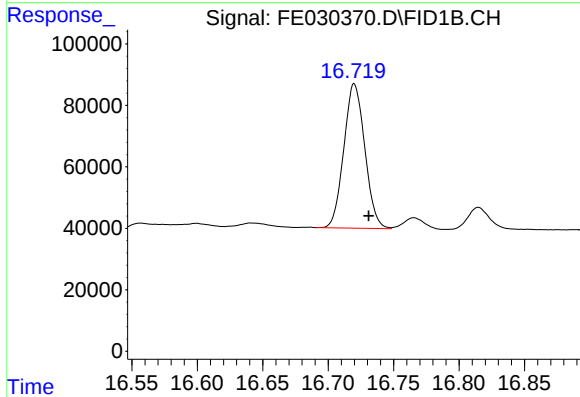


#11 N-OCTACOSANE

R.T.: 16.720 min  
Delta R.T.: -0.011 min  
Response: 523916  
Conc: 2.78 ug/ml

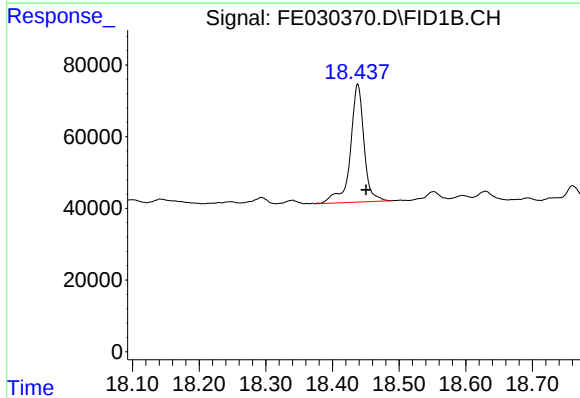


#12 N-DOTRIACONTANE

R.T.: 18.438 min  
Delta R.T.: -0.013 min  
Response: 468384  
Conc: 2.64 ug/ml

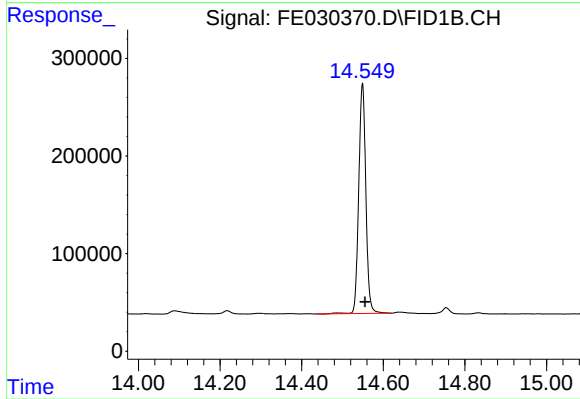

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.549 min  
Delta R.T.: -0.006 min  
Response: 2852553  
Conc: 14.33 ug/ml

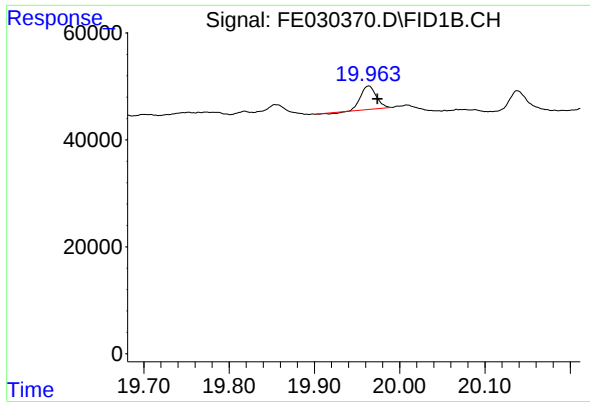

#14 N-HEXATRIACONTANE

R.T.: 19.964 min  
Delta R.T.: -0.010 min  
Response: 54385  
Conc: 0.34 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
A11