

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030373.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 00:36
Operator : DD\AJ
Sample : K4757-18
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
A14

Integration File: autoint1.e
Quant Time: Sep 10 05:48:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.551	4296321	21.589 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.754	52517	0.274 ug/ml
11)	N-OCTACOSANE	16.720	285047	1.514 ug/ml
12)	N-DOTRIACONTANE	18.437	360130	2.026 ug/ml
14)	N-HEXATRIACONTANE	19.964	58512	0.369 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030373.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 00:36
Operator : DD\AJ
Sample : K4757-18
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
A14

Integration File: autoint1.e
Quant Time: Sep 10 05:48:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

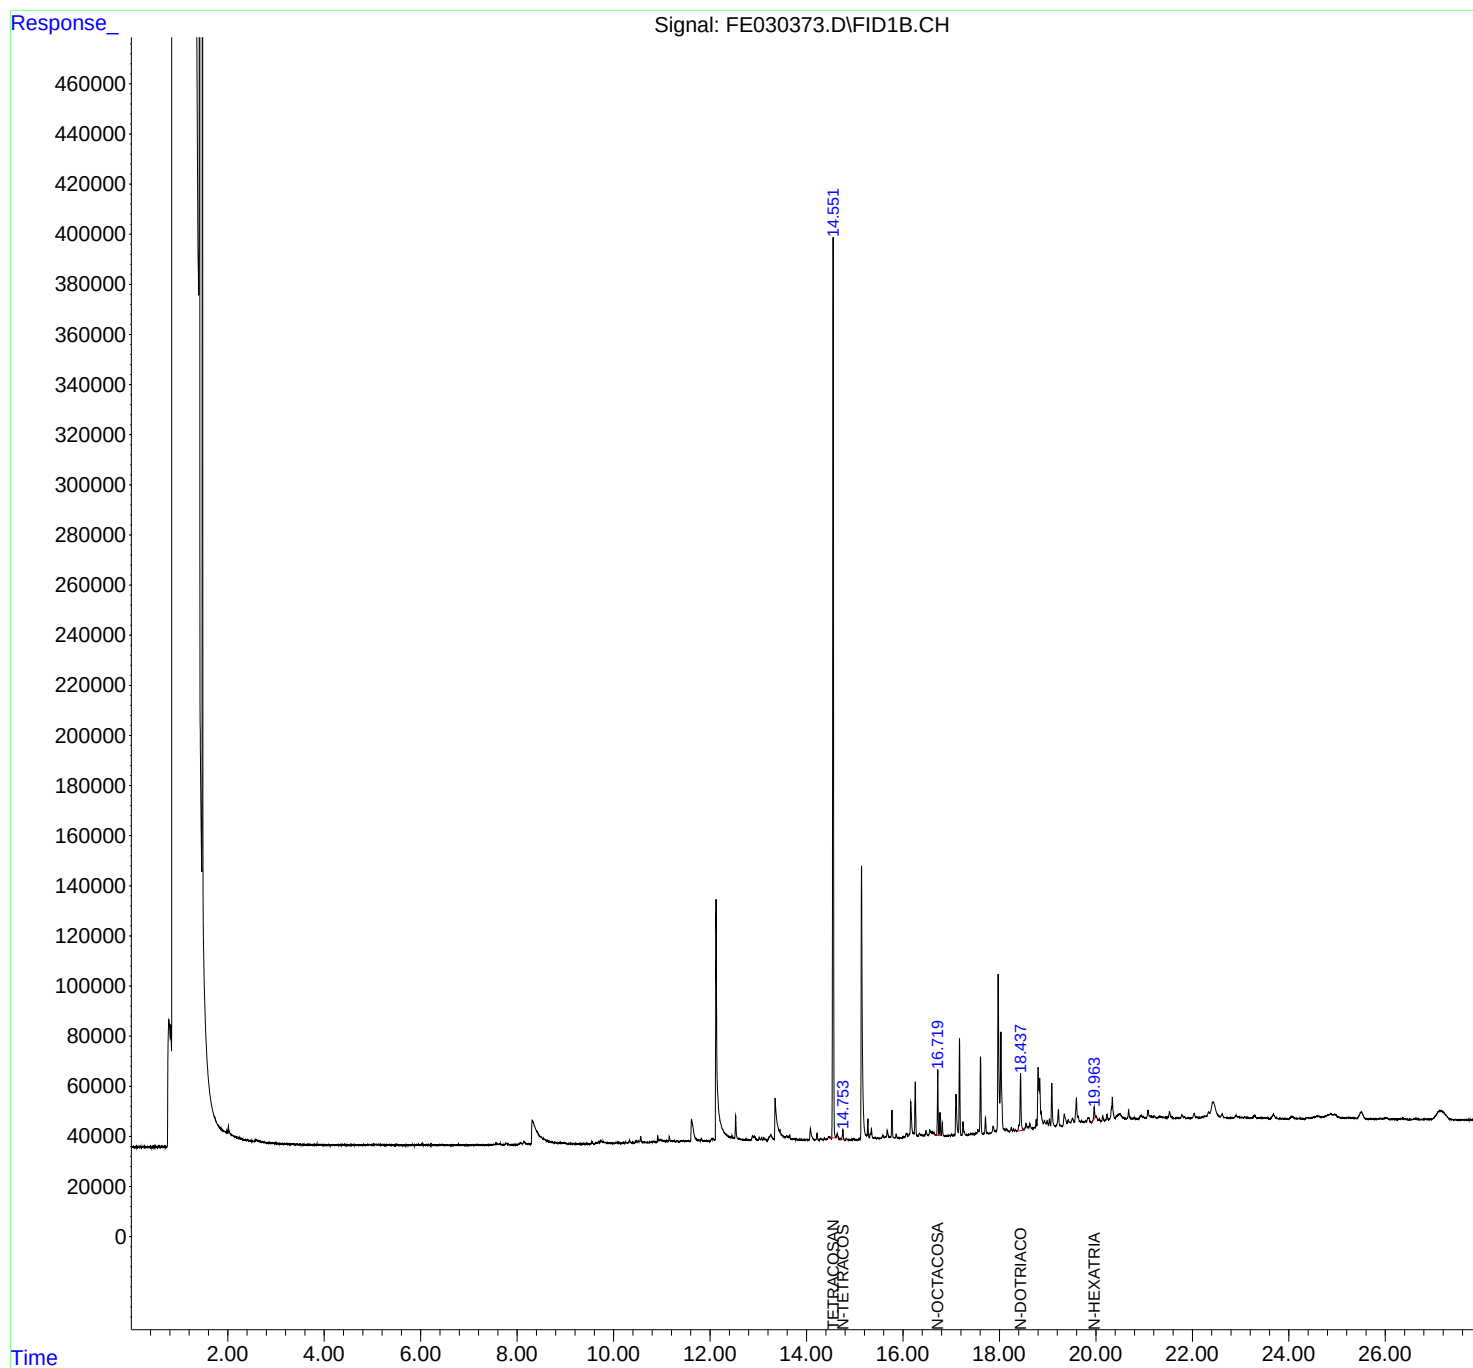


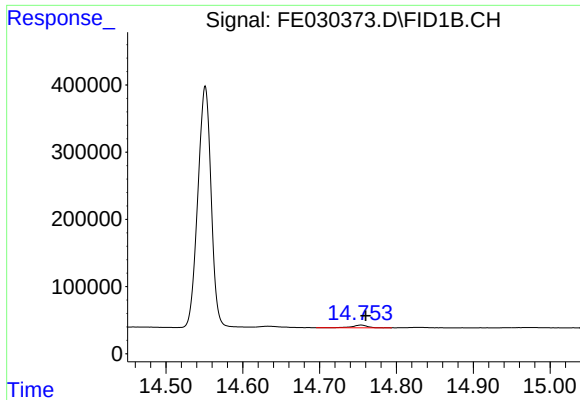

#10 N-TETRACOSANE


R.T.: 14.754 min
Delta R.T.: -0.006 min
Response: 52517
Conc: 0.27 ug/ml

Instrument :
FID_E
ClientSampleId :
A14

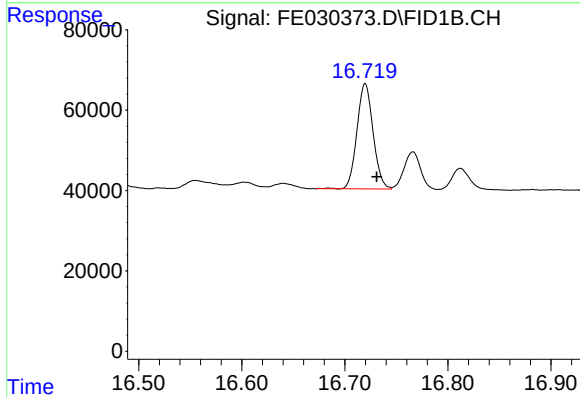


#11 N-OCTACOSANE

R.T.: 16.720 min
Delta R.T.: -0.011 min
Response: 285047
Conc: 1.51 ug/ml

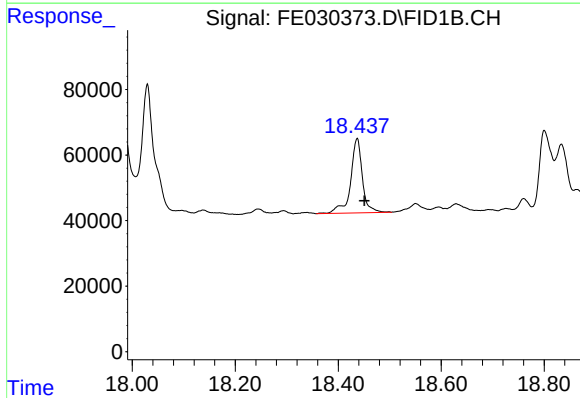


#12 N-DOTRIACONTANE

R.T.: 18.437 min
Delta R.T.: -0.014 min
Response: 360130
Conc: 2.03 ug/ml

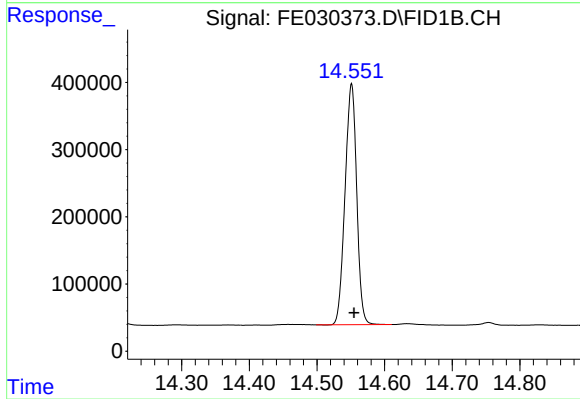

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.551 min
Delta R.T.: -0.004 min
Response: 4296321
Conc: 21.59 ug/ml

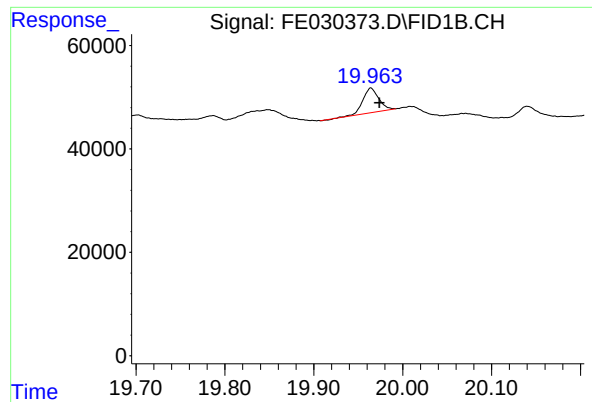

#14 N-HEXATRIACONTANE

R.T.: 19.964 min
Delta R.T.: -0.010 min
Response: 58512
Conc: 0.37 ug/ml

Instrument :
FID_E
ClientSampleId :
A14