

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030374.D
 Signal(s) : FID1B.CH
 Acq On : 10 Sep 2019 1:13
 Operator : DD\AJ
 Sample : K4757-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 A15

Integration File: autoint1.e
 Quant Time: Sep 10 05:49:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.551	4635541	23.293 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.753	51804	0.270 ug/ml
11) N-OCTACOSANE	16.720	222499	1.182 ug/ml
12) N-DOTRIACONTANE	18.435	370153	2.082 ug/ml
14) N-HEXATRIACONTANE	19.961	103635	0.654 ug/ml
15) N-TETRACONTANE	21.523	125912	0.901 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030374.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 1:13
Operator : DD\AJ
Sample : K4757-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
A15

Integration File: autoint1.e
Quant Time: Sep 10 05:49:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

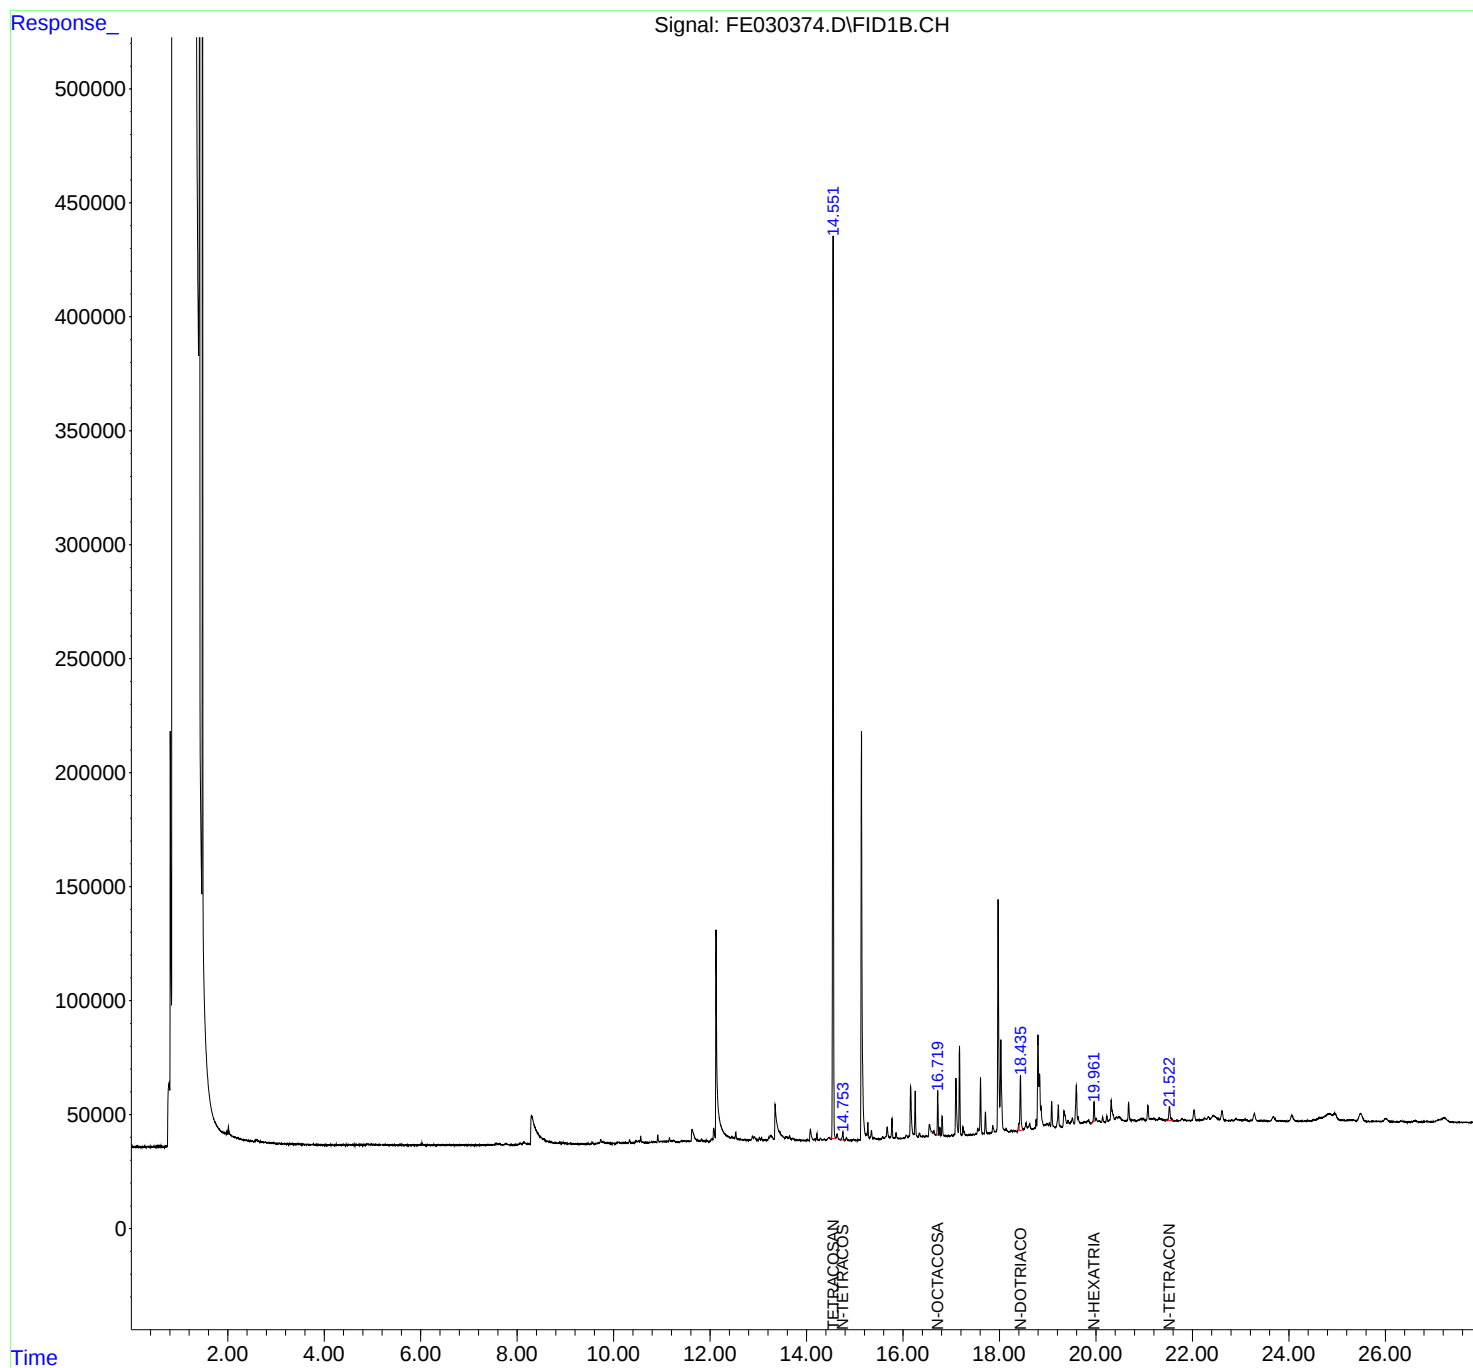


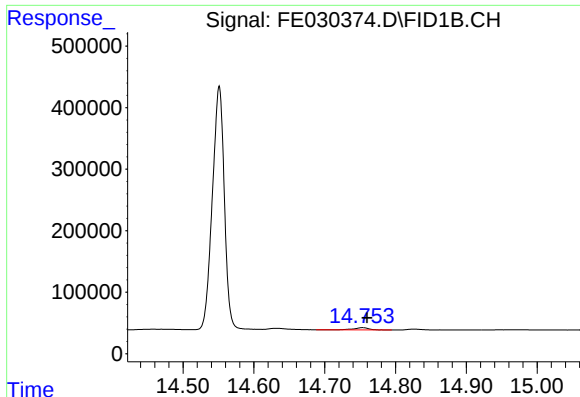

#10 N-TETRACOSANE


R.T.: 14.753 min
Delta R.T.: -0.007 min
Response: 51804
Conc: 0.27 ug/ml

Instrument :
FID_E
ClientSampleId :
A15

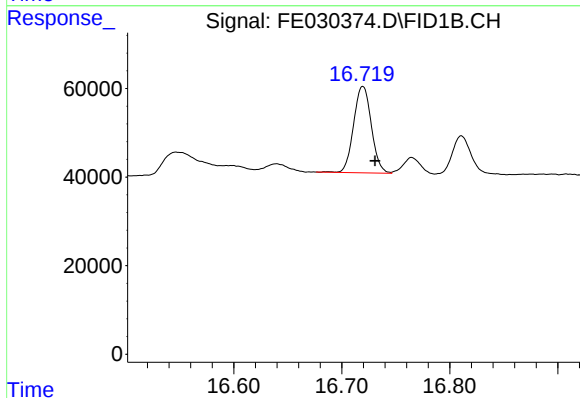


#11 N-OCTACOSANE

R.T.: 16.720 min
Delta R.T.: -0.011 min
Response: 222499
Conc: 1.18 ug/ml

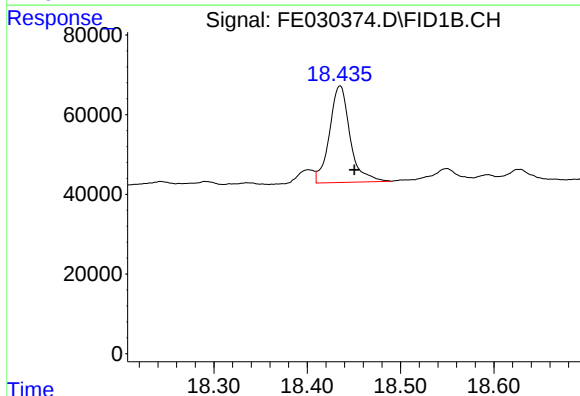


#12 N-DOTRIACONTANE

R.T.: 18.435 min
Delta R.T.: -0.015 min
Response: 370153
Conc: 2.08 ug/ml

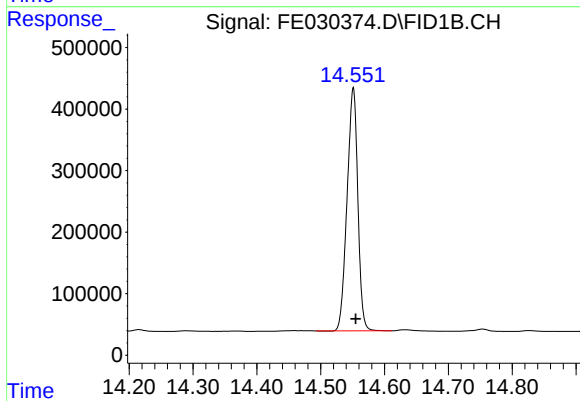

#13 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.551 min
Delta R.T.: -0.004 min
Response: 4635541
Conc: 23.29 ug/ml

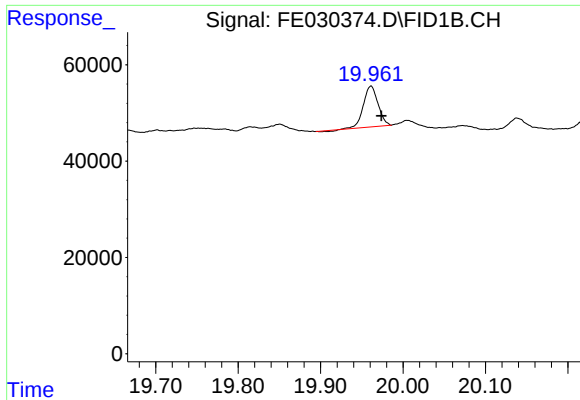

#14 N-HEXATRIACONTANE

R.T.: 19.961 min
Delta R.T.: -0.013 min
Response: 103635
Conc: 0.65 ug/ml

Instrument :
FID_E
ClientSampleId :
A15

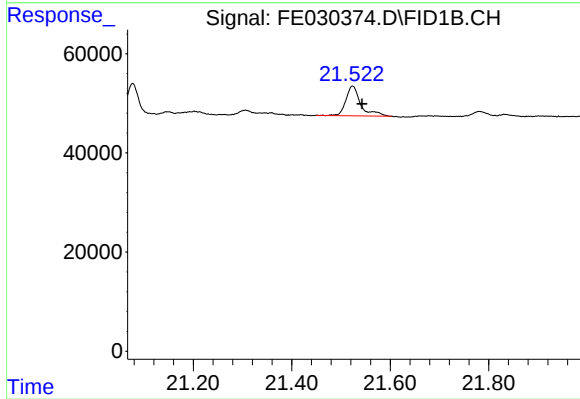

#15 N-TETRACONTANE

R.T.: 21.523 min
Delta R.T.: -0.019 min
Response: 125912
Conc: 0.90 ug/ml