

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030375.D
 Signal(s) : FID1B.CH
 Acq On : 10 Sep 2019 1:50
 Operator : DD\AJ
 Sample : K4757-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 A16

Integration File: autoint1.e
 Quant Time: Sep 10 05:49:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.551	4726005	23.748 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.753	67626	0.353 ug/ml
11)	N-OCTACOSANE	16.719	251220	1.335 ug/ml
12)	N-DOTRIACONTANE	18.433	506136	2.848 ug/ml
14)	N-HEXATRIACONTANE	19.961	80513	0.508 ug/ml
15)	N-TETRACONTANE	21.523	76551	0.548 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030375.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 1:50
Operator : DD\AJ
Sample : K4757-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
A16

Integration File: autoint1.e
Quant Time: Sep 10 05:49:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

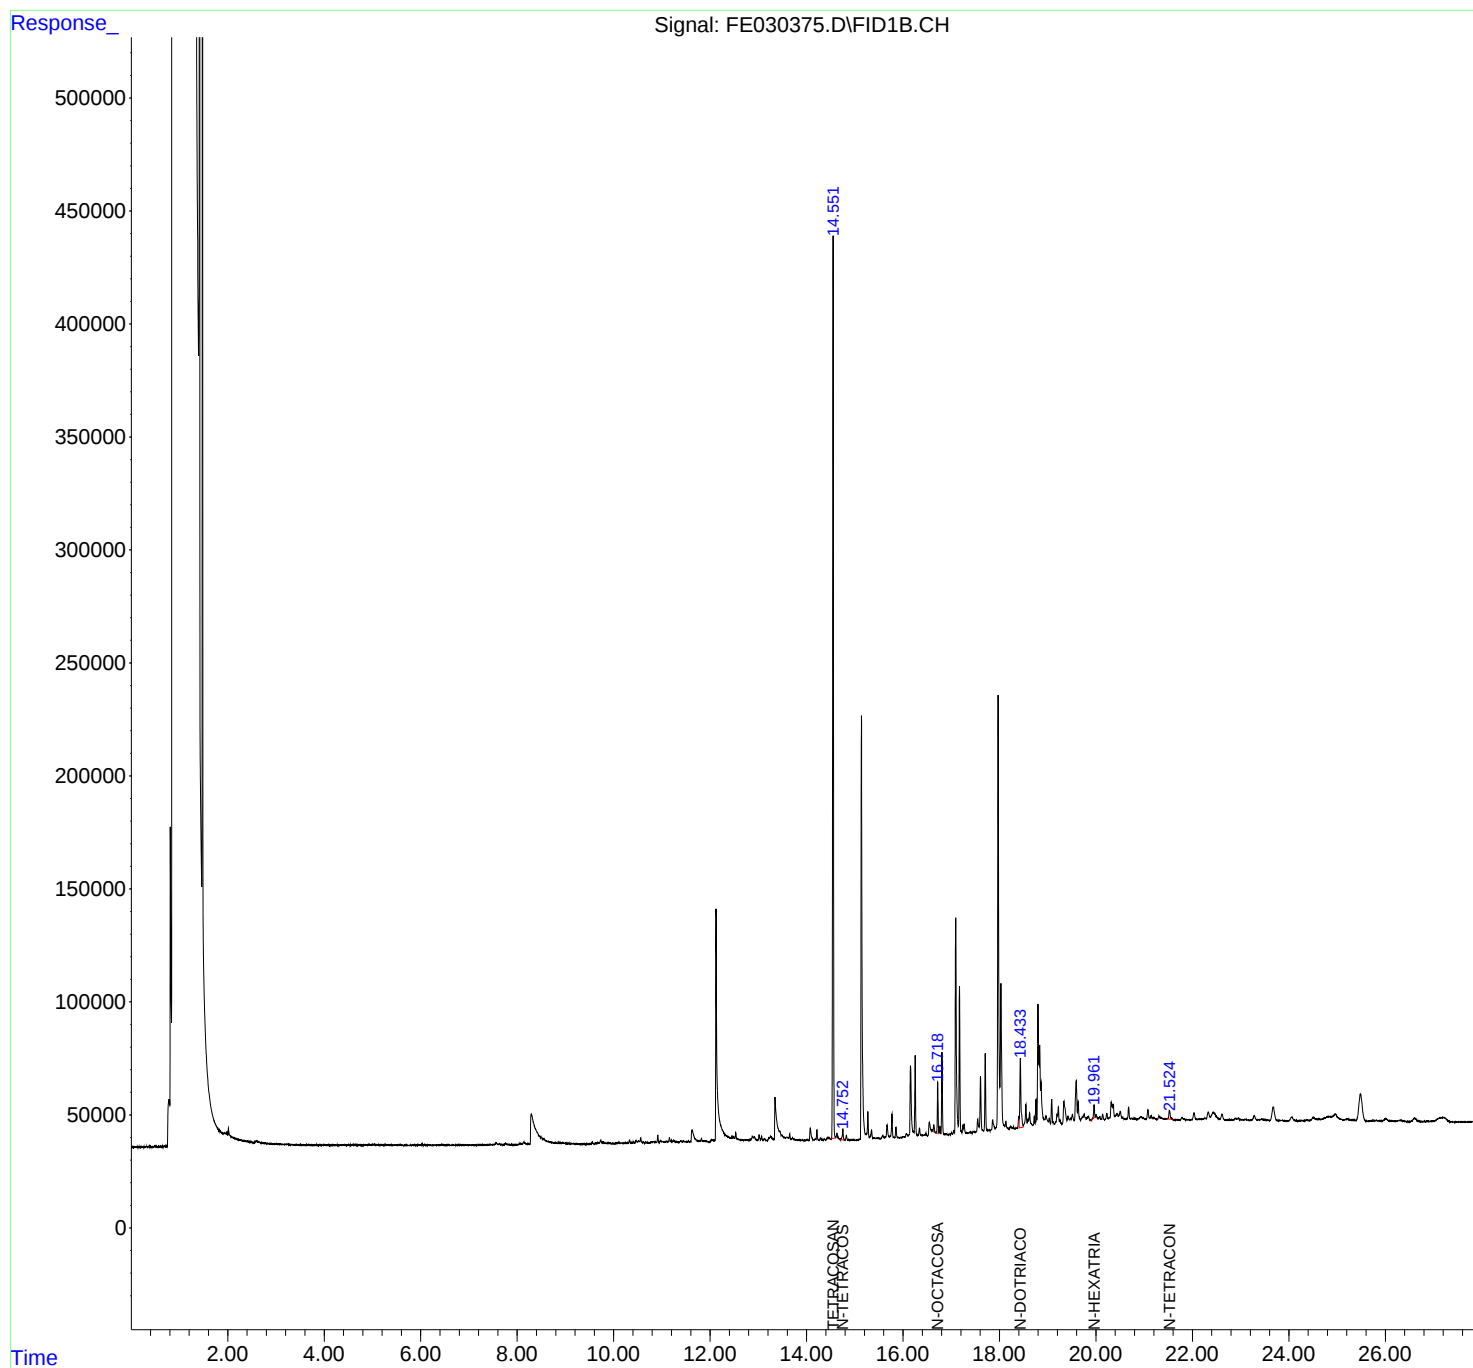


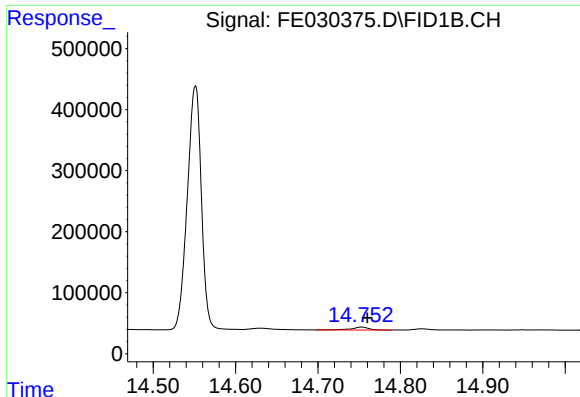

#10 N-TETRACOSANE


R.T.: 14.753 min
Delta R.T.: -0.007 min
Response: 67626
Conc: 0.35 ug/ml

Instrument :
FID_E
ClientSampleId :
A16

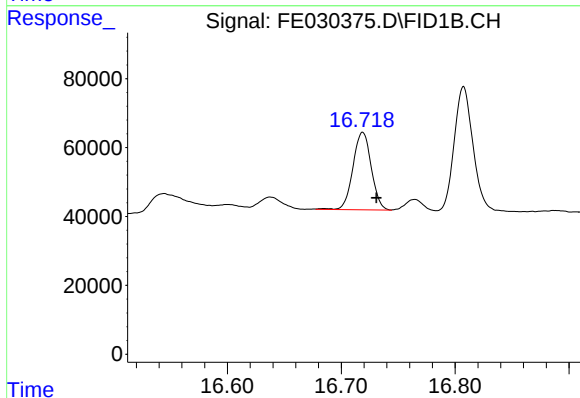


#11 N-OCTACOSANE

R.T.: 16.719 min
Delta R.T.: -0.012 min
Response: 251220
Conc: 1.33 ug/ml

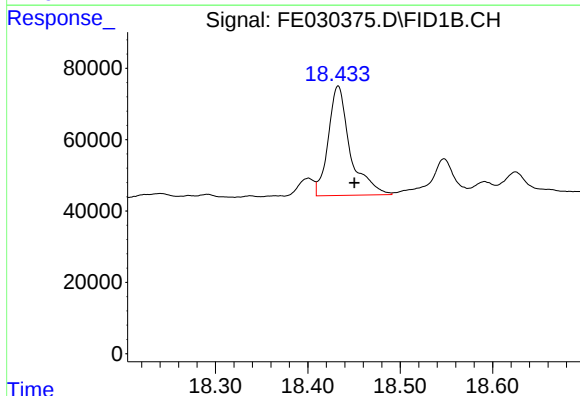


#12 N-DOTRIACONTANE

R.T.: 18.433 min
Delta R.T.: -0.018 min
Response: 506136
Conc: 2.85 ug/ml

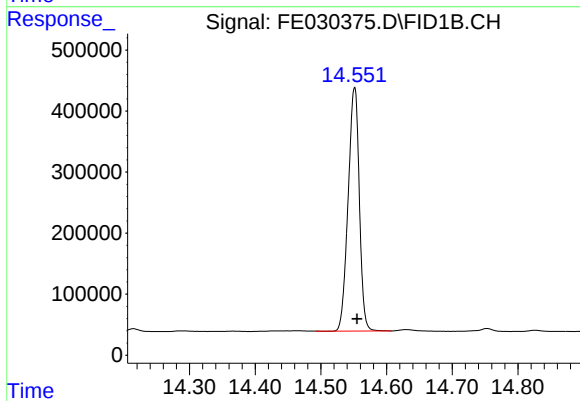

#13 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.551 min
Delta R.T.: -0.004 min
Response: 4726005
Conc: 23.75 ug/ml

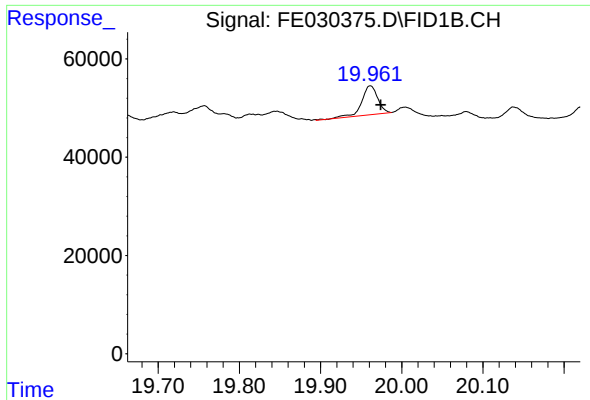

#14 N-HEXATRIACONTANE

R.T.: 19.961 min
Delta R.T.: -0.013 min
Response: 80513
Conc: 0.51 ug/ml

Instrument :
FID_E
ClientSampleId :
A16

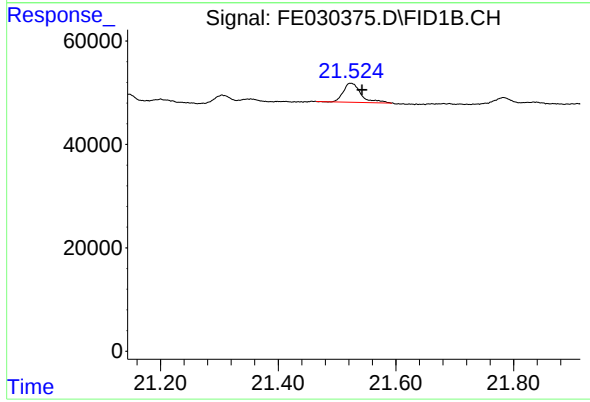

#15 N-TETRACONTANE

R.T.: 21.523 min
Delta R.T.: -0.019 min
Response: 76551
Conc: 0.55 ug/ml