

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030381.D
 Signal(s) : FID1B.CH
 Acq On : 10 Sep 2019 5:33
 Operator : DD\AJ
 Sample : K4758-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 B2

Integration File: autoint1.e
 Quant Time: Sep 10 08:46:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.549	4153312	20.870 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.751	192907	1.006 ug/ml
11)	N-OCTACOSANE	16.719	409989	2.178 ug/ml
12)	N-DOTRIACONTANE	18.435	288062	1.621 ug/ml
14)	N-HEXATRIACONTANE	19.962	54673	0.345 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030381.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 5:33
Operator : DD\AJ
Sample : K4758-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B2

Integration File: autoint1.e
Quant Time: Sep 10 08:46:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

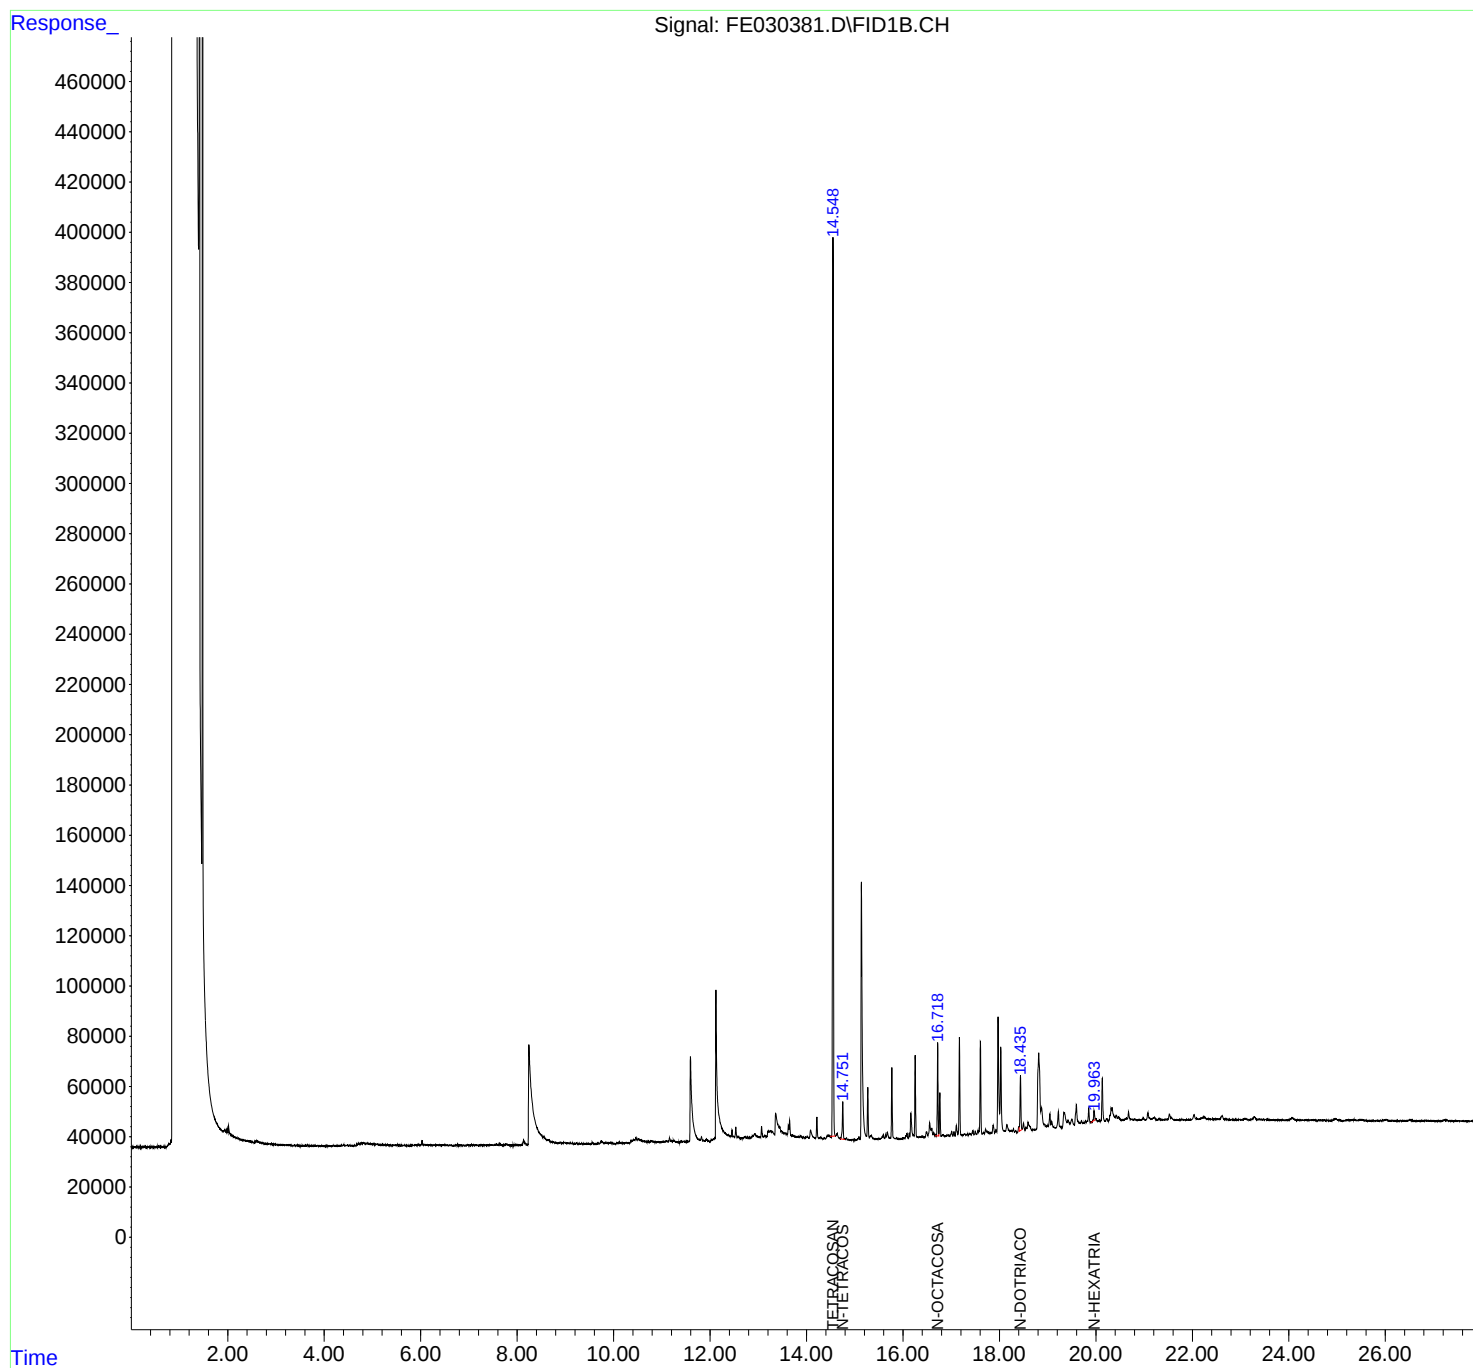


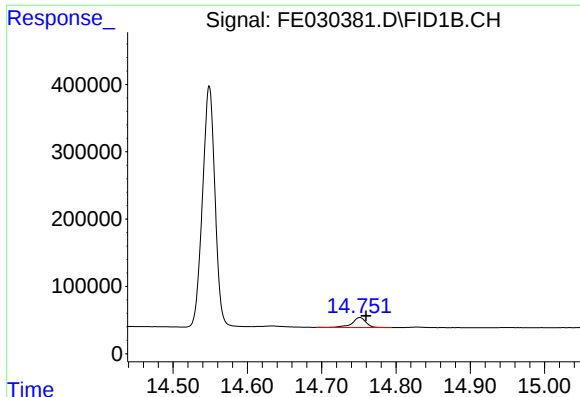

#10 N-TETRACOSANE


R.T.: 14.751 min
Delta R.T.: -0.009 min
Response: 192907
Conc: 1.01 ug/ml

Instrument :
FID_E
ClientSampleId :
B2

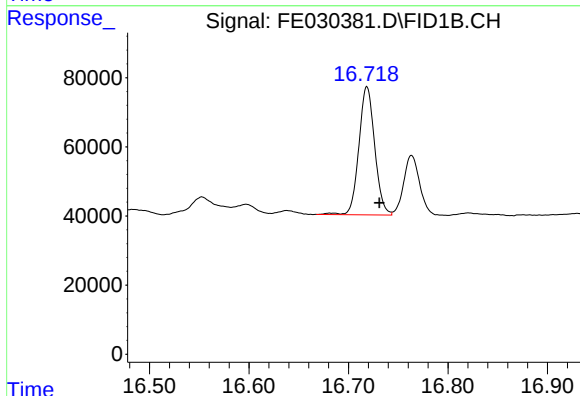


#11 N-OCTACOSANE

R.T.: 16.719 min
Delta R.T.: -0.012 min
Response: 409989
Conc: 2.18 ug/ml

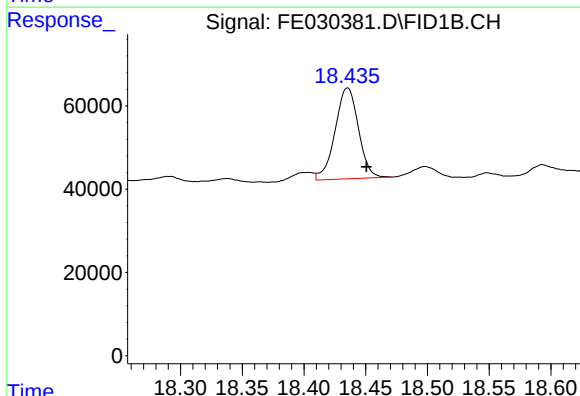


#12 N-DOTRIACONTANE

R.T.: 18.435 min
Delta R.T.: -0.015 min
Response: 288062
Conc: 1.62 ug/ml

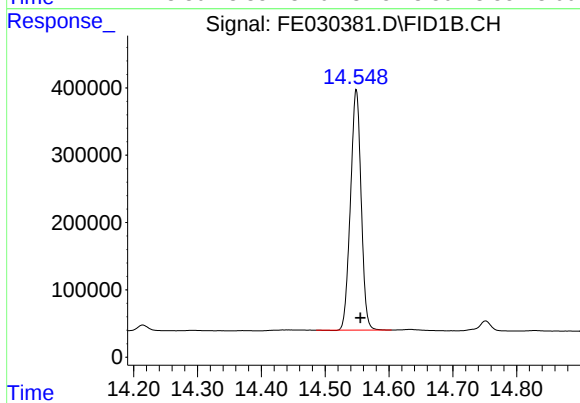

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.549 min
Delta R.T.: -0.006 min
Response: 4153312
Conc: 20.87 ug/ml

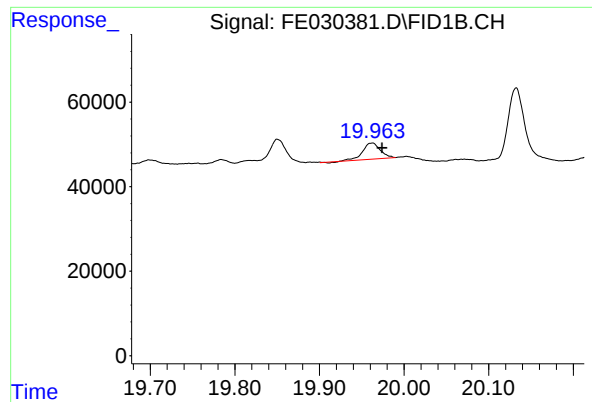

#14 N-HEXATRIACONTANE

R.T.: 19.962 min
Delta R.T.: -0.011 min
Response: 54673
Conc: 0.35 ug/ml

Instrument :
FID_E
ClientSampleId :
B2