

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030383.D
 Signal(s) : FID1B.CH
 Acq On : 10 Sep 2019 6:47
 Operator : DD\AJ
 Sample : K4758-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 B4

Integration File: autoint1.e
 Quant Time: Sep 10 08:46:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.552	5430439	27.288 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.750	335090	1.748 ug/ml
11)	N-OCTACOSANE	16.719	810058	4.303 ug/ml
12)	N-DOTRIACONTANE	18.435	547647	3.081 ug/ml
14)	N-HEXATRIACONTANE	19.960	114337	0.722 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030383.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 6:47
Operator : DD\AJ
Sample : K4758-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B4

Integration File: autoint1.e
Quant Time: Sep 10 08:46:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

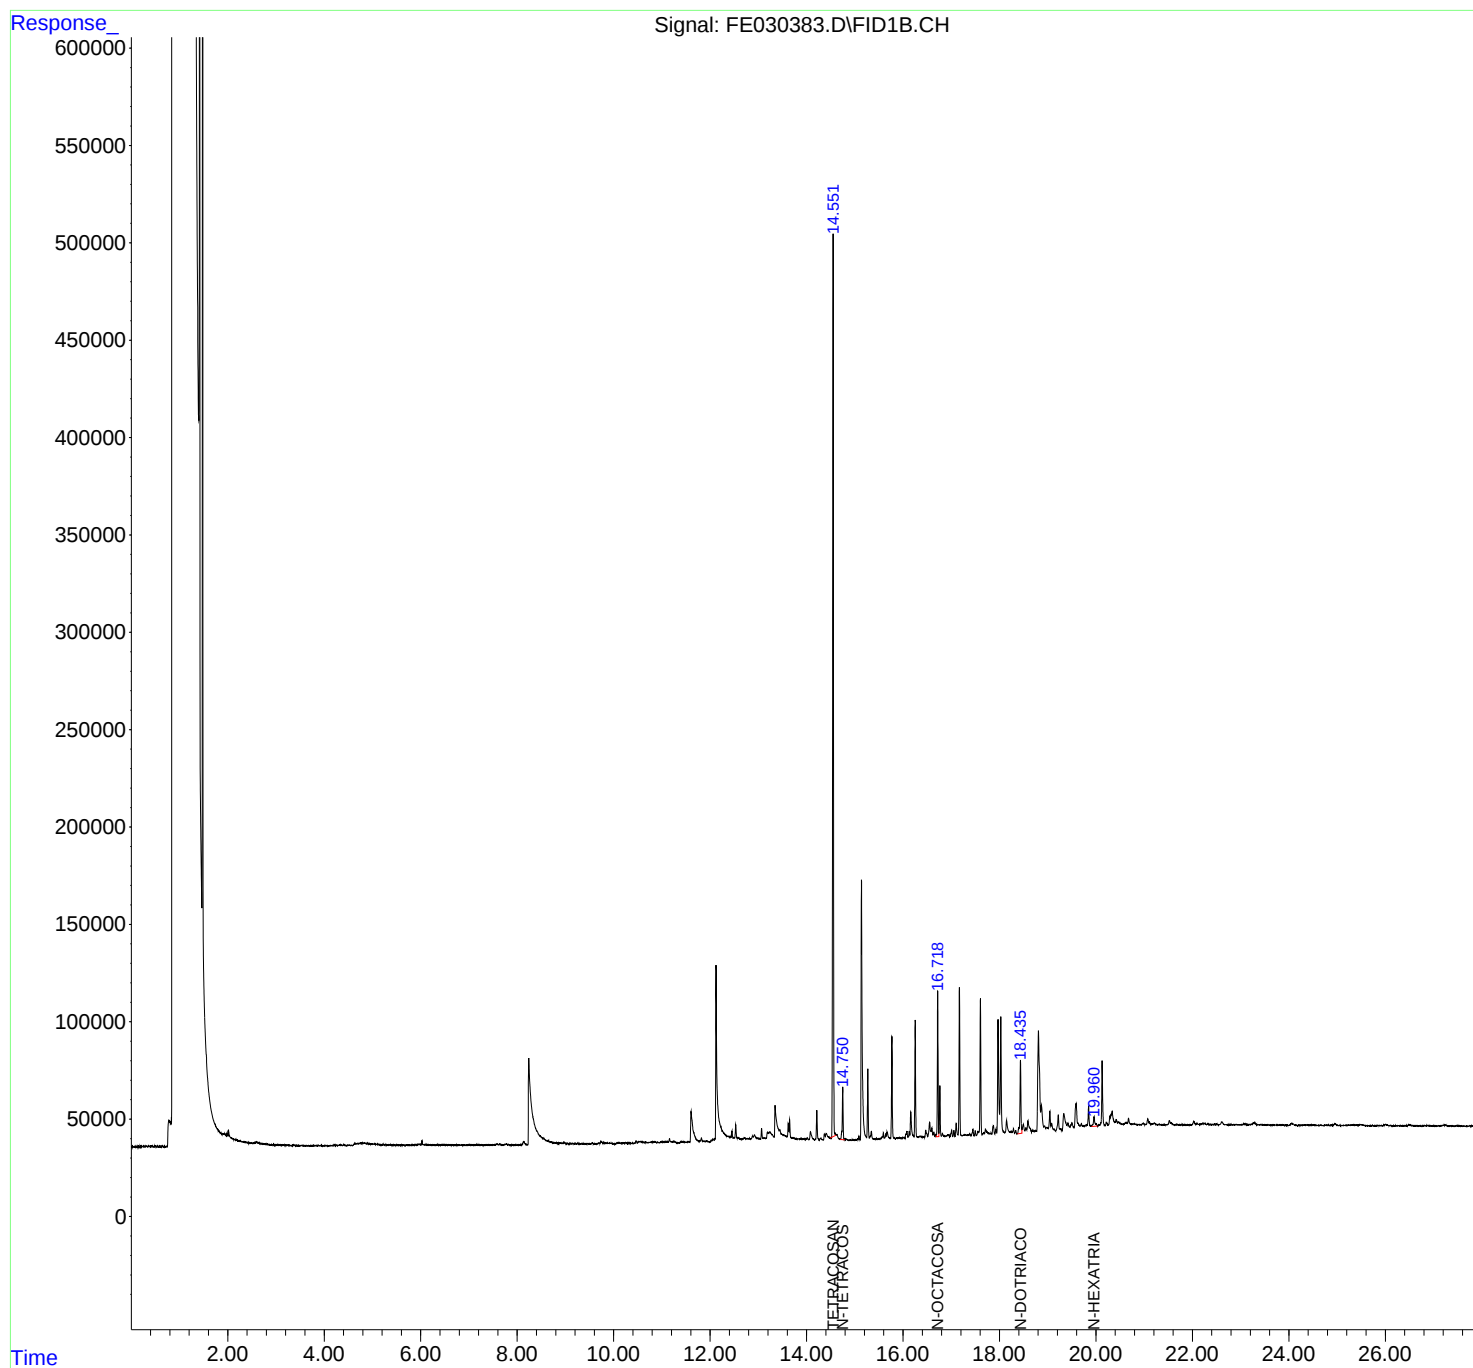


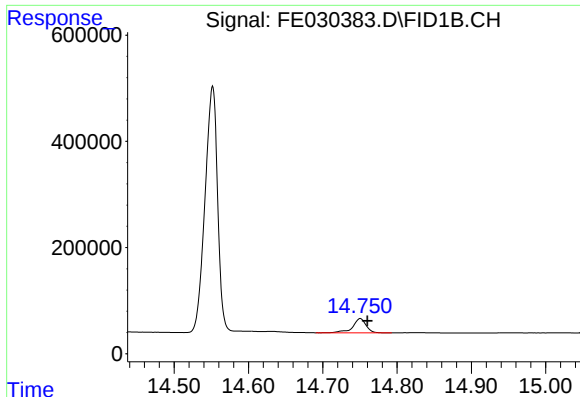

#10 N-TETRACOSANE


R.T.: 14.750 min
Delta R.T.: -0.010 min
Response: 335090
Conc: 1.75 ug/ml

Instrument :
FID_E
ClientSampleId :
B4

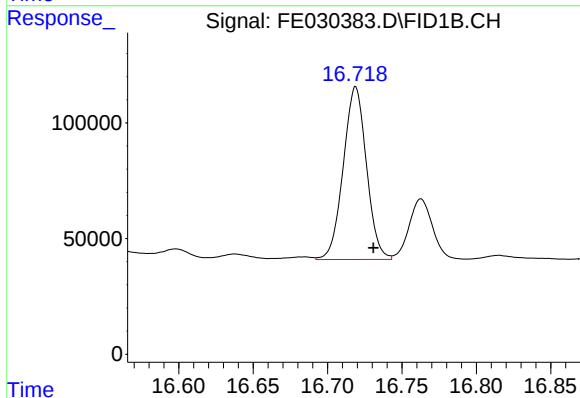


#11 N-OCTACOSANE

R.T.: 16.719 min
Delta R.T.: -0.012 min
Response: 810058
Conc: 4.30 ug/ml

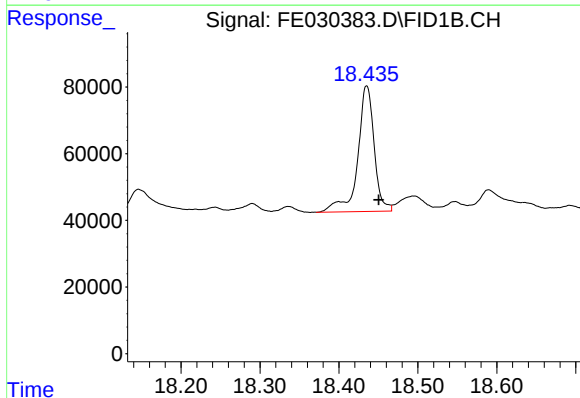


#12 N-DOTRIACONTANE

R.T.: 18.435 min
Delta R.T.: -0.015 min
Response: 547647
Conc: 3.08 ug/ml

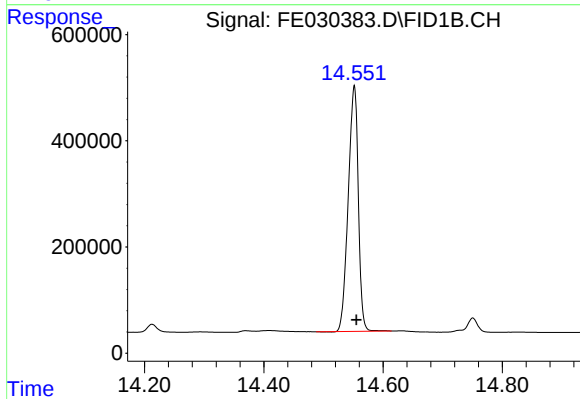

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.552 min
Delta R.T.: -0.003 min
Response: 5430439
Conc: 27.29 ug/ml

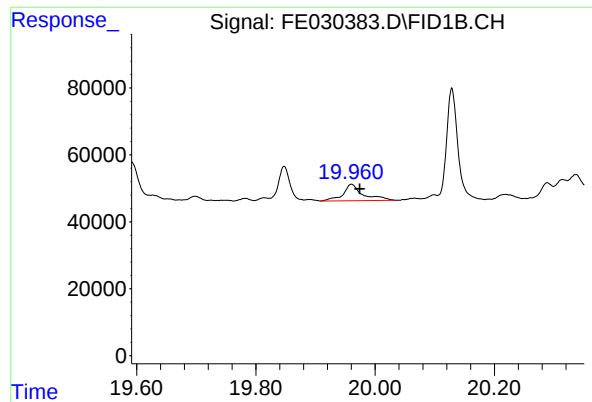

#14 N-HEXATRIACONTANE

R.T.: 19.960 min
Delta R.T.: -0.014 min
Response: 114337
Conc: 0.72 ug/ml

Instrument :
FID_E
ClientSampleId :
B4