

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030392.D
 Signal(s) : FID1B.CH
 Acq On : 10 Sep 2019 12:24
 Operator : DD\AJ
 Sample : K4758-15
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 B11

Integration File: autoint1.e
 Quant Time: Sep 11 00:46:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.547	3316349	16.664 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.750	347345	1.812 ug/ml
11)	N-OCTACOSANE	16.719	1118587	5.942 ug/ml
12)	N-DOTRIACONTANE	18.436	690273	3.883 ug/ml
14)	N-HEXATRIACONTANE	19.962	102648	0.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030392.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 12:24
Operator : DD\AJ
Sample : K4758-15
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B11

Integration File: autoint1.e
Quant Time: Sep 11 00:46:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

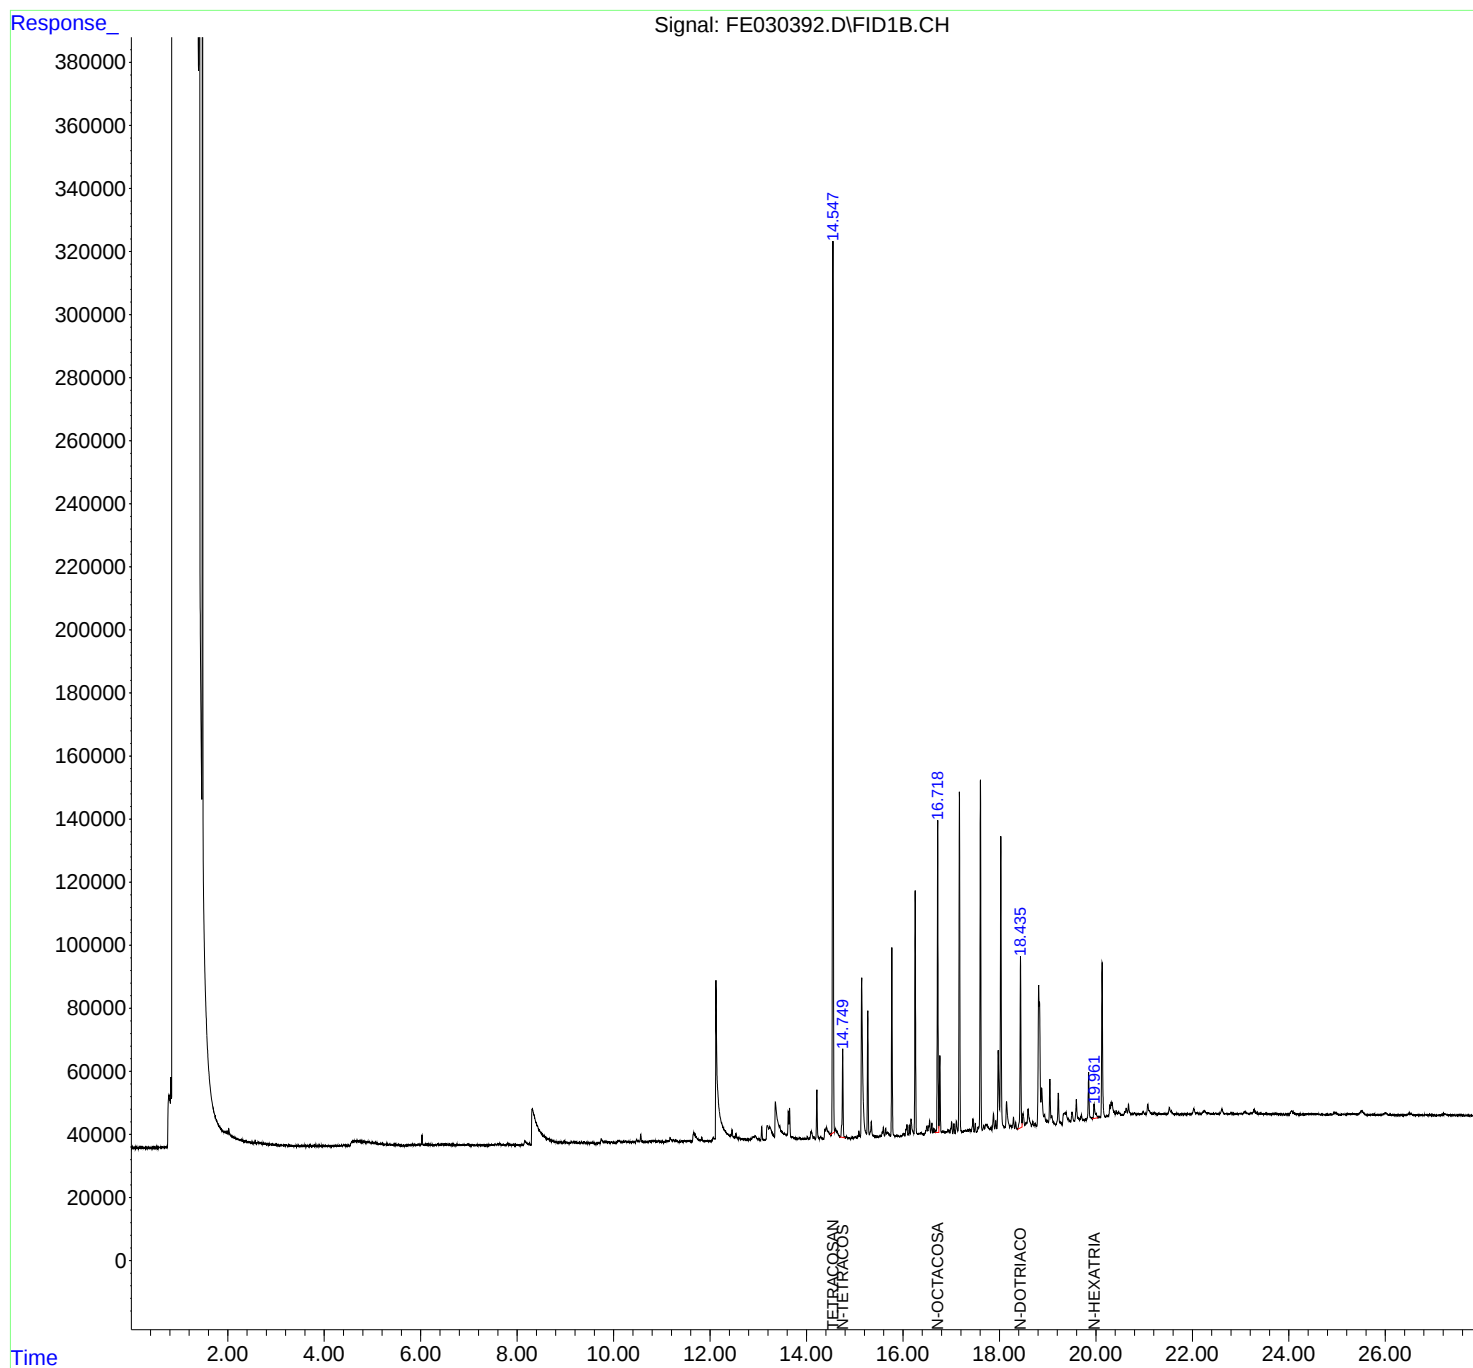


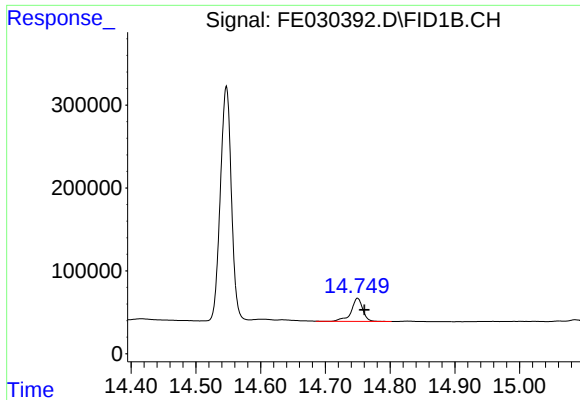

#10 N-TETRACOSANE


R.T.: 14.750 min
Delta R.T.: -0.010 min
Response: 347345
Conc: 1.81 ug/ml

Instrument :
FID_E
ClientSampleId :
B11

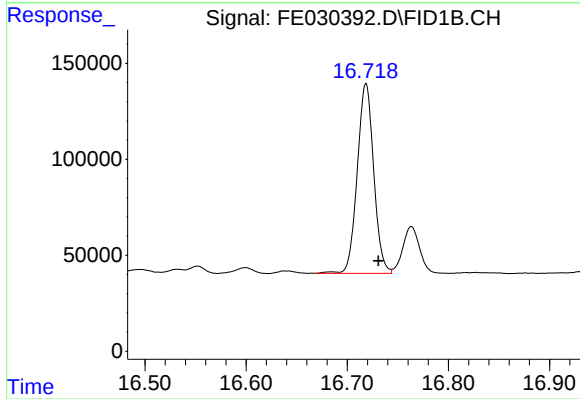


#11 N-OCTACOSANE

R.T.: 16.719 min
Delta R.T.: -0.012 min
Response: 1118587
Conc: 5.94 ug/ml

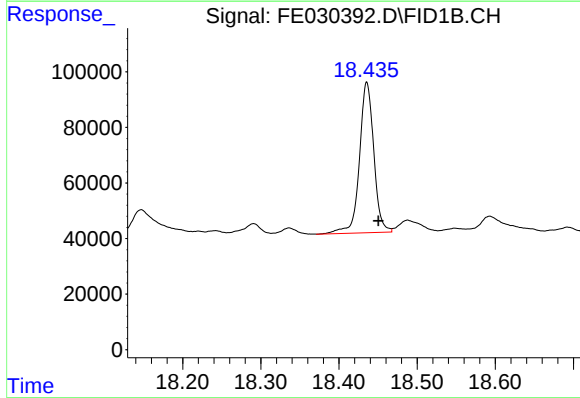


#12 N-DOTRIACONTANE

R.T.: 18.436 min
Delta R.T.: -0.015 min
Response: 690273
Conc: 3.88 ug/ml

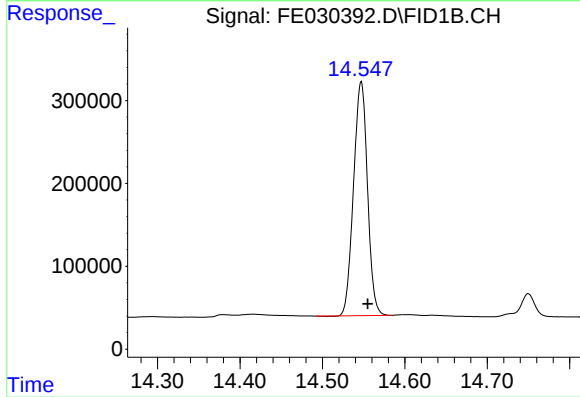

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.547 min
Delta R.T.: -0.008 min
Response: 3316349
Conc: 16.66 ug/ml

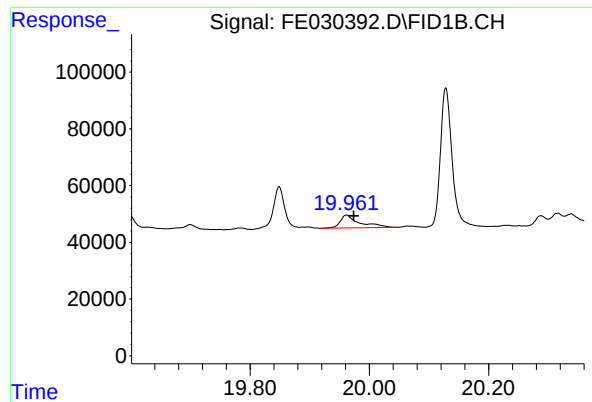

#14 N-HEXATRIACONTANE

R.T.: 19.962 min
Delta R.T.: -0.012 min
Response: 102648
Conc: 0.65 ug/ml

Instrument :
FID_E
ClientSampleId :
B11