

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030394.D
 Signal(s) : FID1B.CH
 Acq On : 10 Sep 2019 13:38
 Operator : DD\AJ
 Sample : K4758-17
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 B13

Integration File: autoint1.e
 Quant Time: Sep 11 00:47:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.547	4249767	21.355 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.749	313352	1.634 ug/ml
11)	N-OCTACOSANE	16.717	595006	3.161 ug/ml
12)	N-DOTRIACONTANE	18.433	495853	2.790 ug/ml
14)	N-HEXATRIACONTANE	19.959	100996	0.637 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030394.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 13:38
Operator : DD\AJ
Sample : K4758-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B13

Integration File: autoint1.e
Quant Time: Sep 11 00:47:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

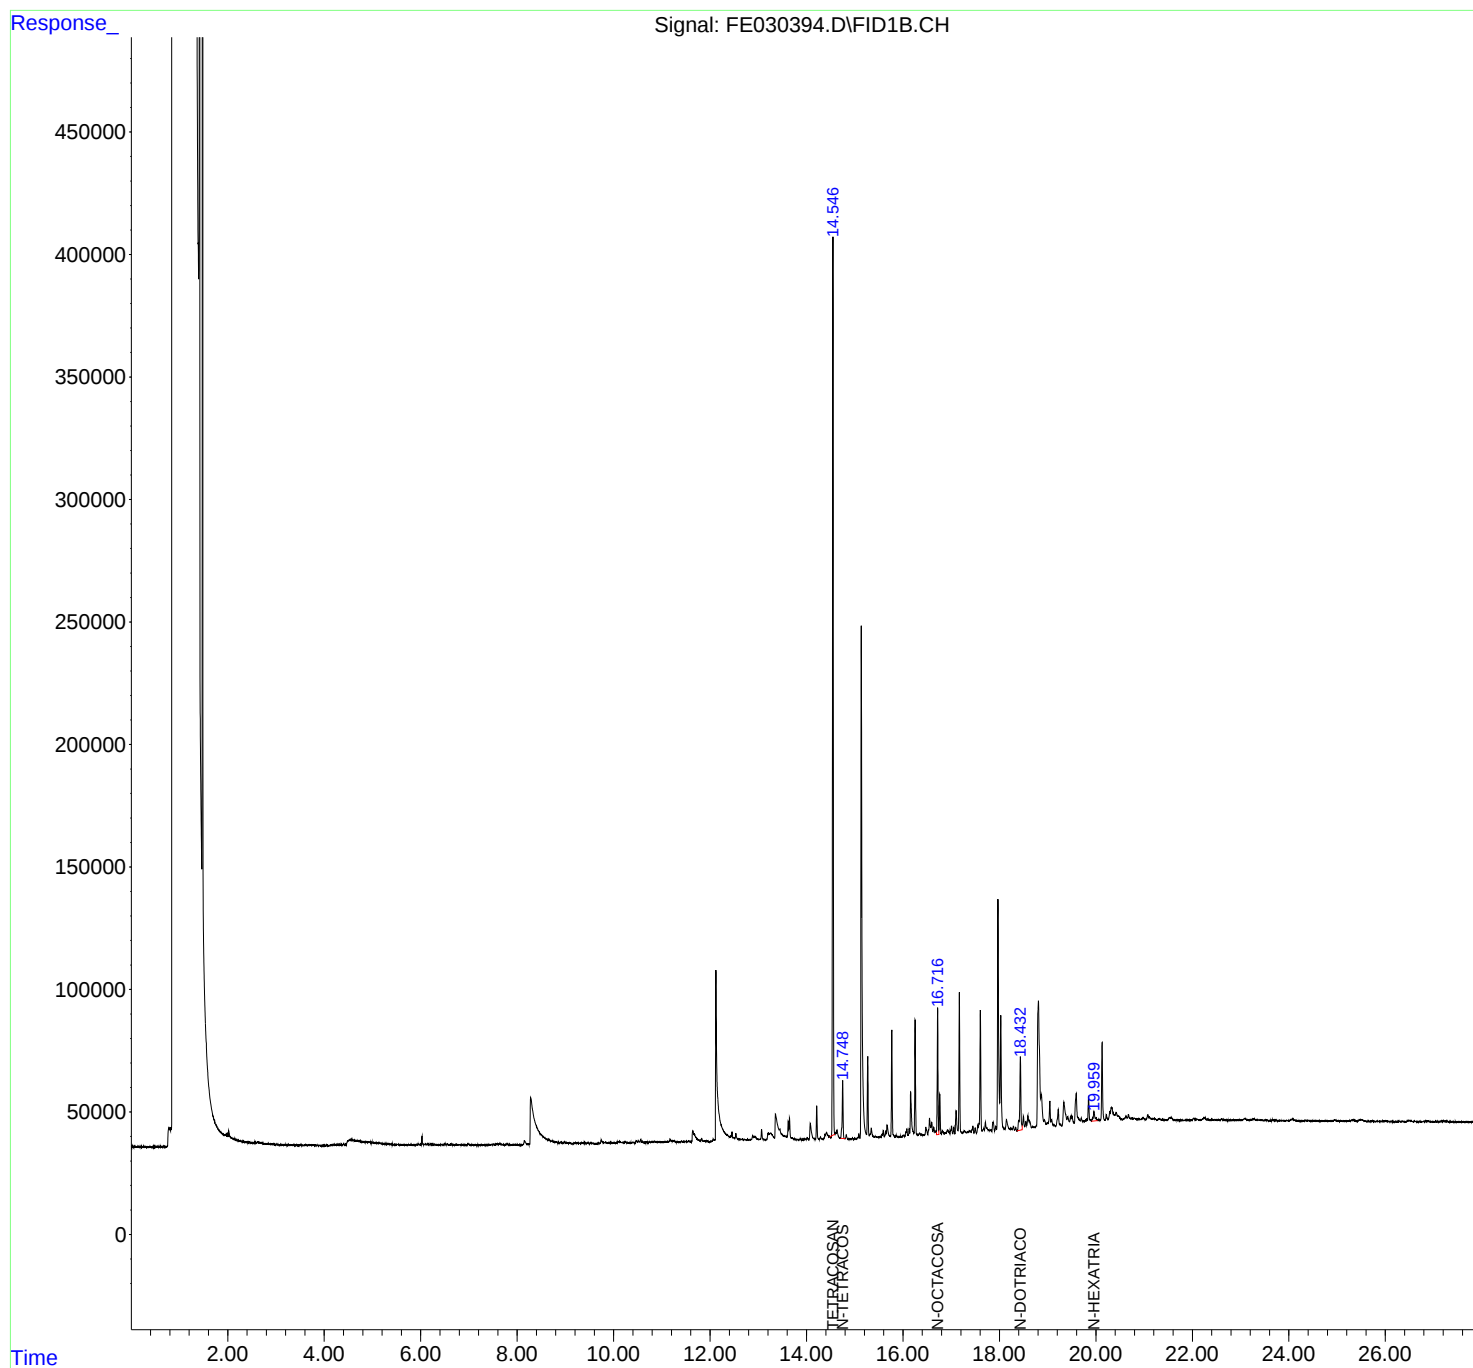


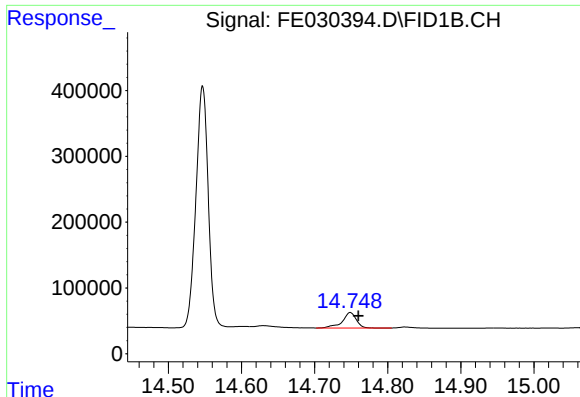

#10 N-TETRACOSANE


R.T.: 14.749 min
Delta R.T.: -0.011 min
Response: 313352
Conc: 1.63 ug/ml

Instrument :
FID_E
ClientSampleId :
B13

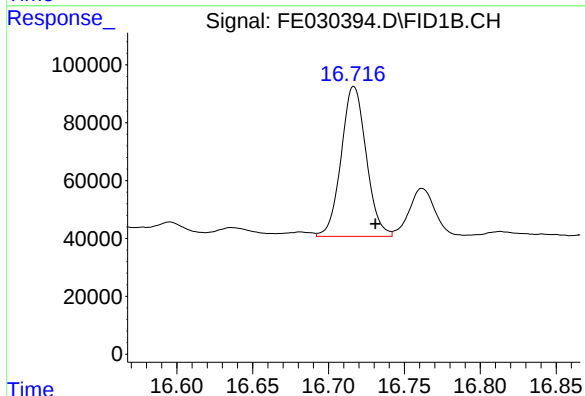


#11 N-OCTACOSANE

R.T.: 16.717 min
Delta R.T.: -0.014 min
Response: 595006
Conc: 3.16 ug/ml

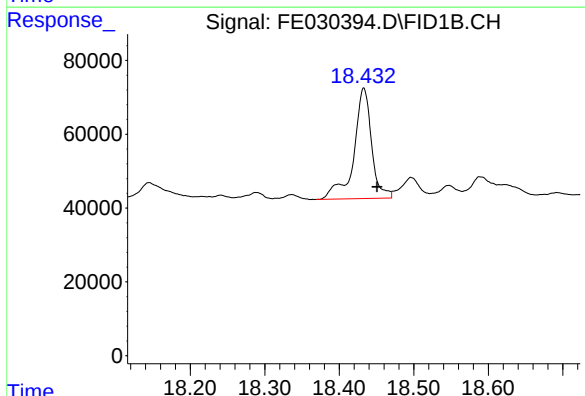


#12 N-DOTRIACONTANE

R.T.: 18.433 min
Delta R.T.: -0.018 min
Response: 495853
Conc: 2.79 ug/ml

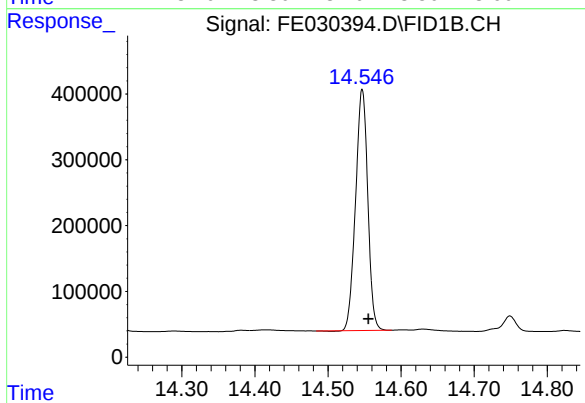

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.547 min
Delta R.T.: -0.008 min
Response: 4249767
Conc: 21.35 ug/ml

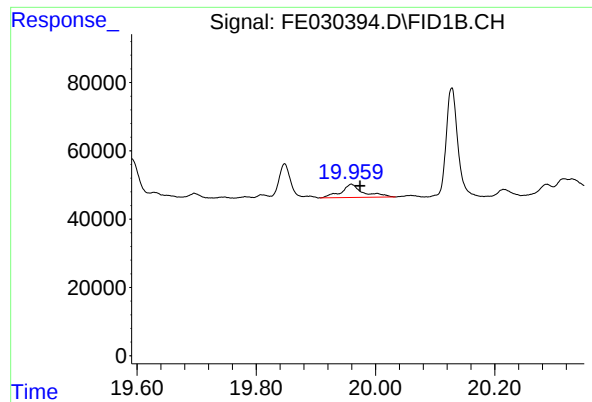

#14 N-HEXATRIACONTANE

R.T.: 19.959 min
Delta R.T.: -0.015 min
Response: 100996
Conc: 0.64 ug/ml

Instrument :
FID_E
ClientSampleId :
B13