

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030395.D
 Signal(s) : FID1B.CH
 Acq On : 10 Sep 2019 14:16
 Operator : DD\AJ
 Sample : K4758-18
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 B14

Integration File: autoint1.e
 Quant Time: Sep 11 00:47:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.548	3793163	19.060 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.751	111994	0.584 ug/ml
11)	N-OCTACOSANE	16.717	360003	1.913 ug/ml
12)	N-DOTRIACONTANE	18.434	327009	1.840 ug/ml
14)	N-HEXATRIACONTANE	19.962	75435	0.476 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030395.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 14:16
Operator : DD\AJ
Sample : K4758-18
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B14

Integration File: autoint1.e
Quant Time: Sep 11 00:47:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

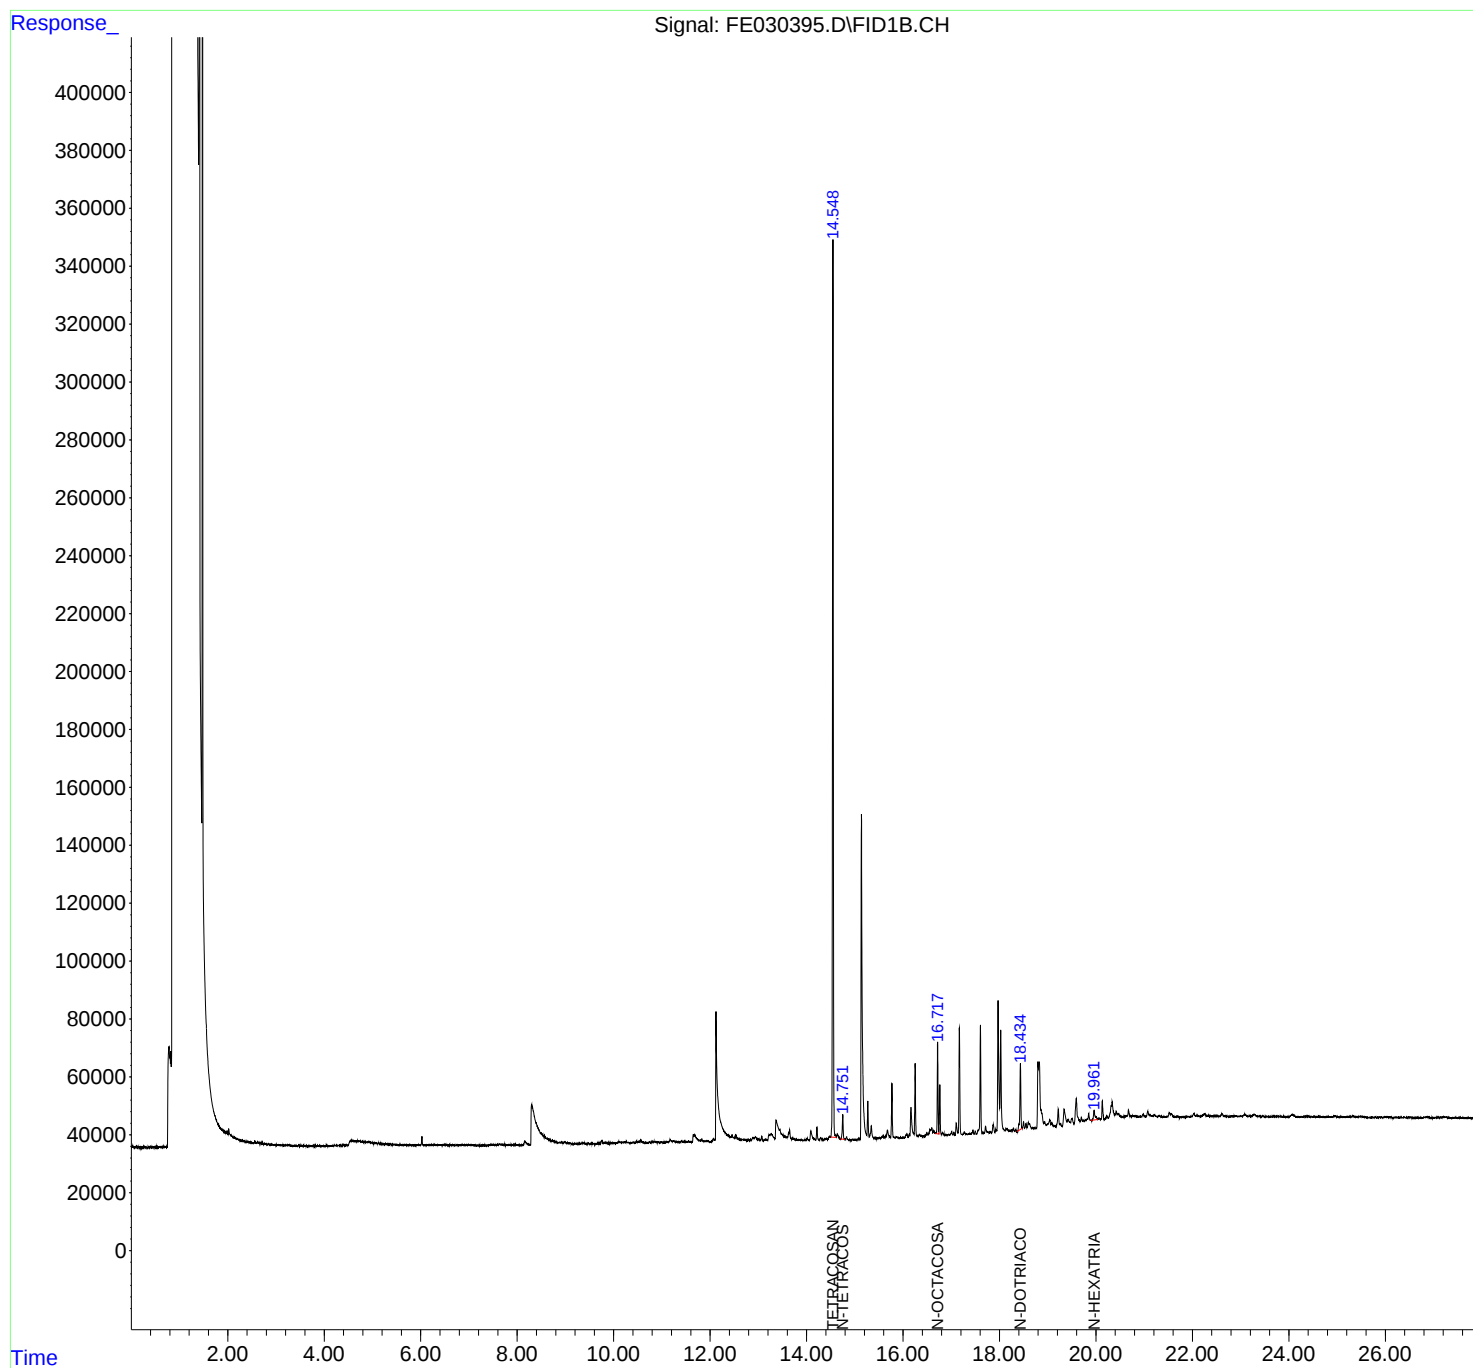


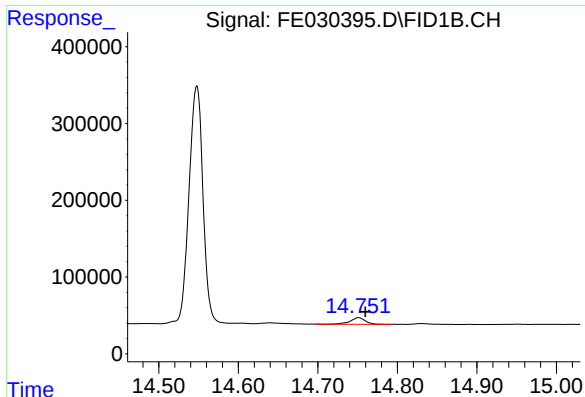

#10 N-TETRACOSANE


R.T.: 14.751 min
Delta R.T.: -0.009 min
Response: 111994
Conc: 0.58 ug/ml

Instrument :
FID_E
ClientSampleId :
B14

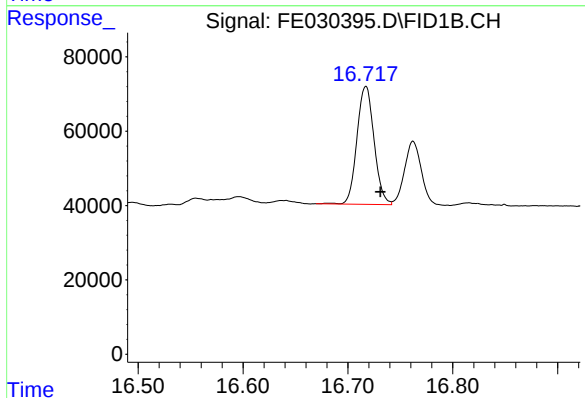


#11 N-OCTACOSANE

R.T.: 16.717 min
Delta R.T.: -0.014 min
Response: 360003
Conc: 1.91 ug/ml

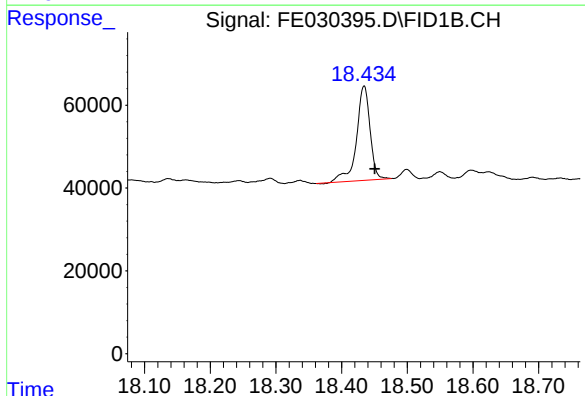


#12 N-DOTRIACONTANE

R.T.: 18.434 min
Delta R.T.: -0.016 min
Response: 327009
Conc: 1.84 ug/ml

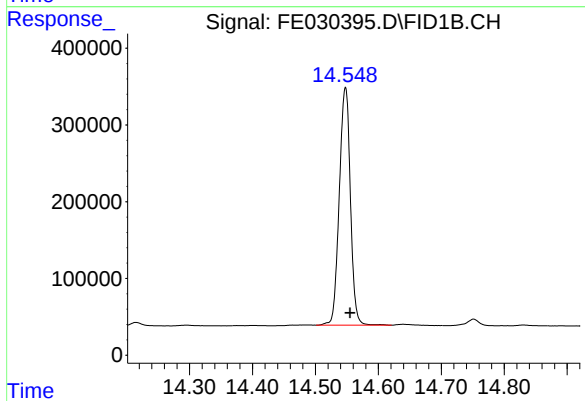

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.548 min
Delta R.T.: -0.007 min
Response: 3793163
Conc: 19.06 ug/ml

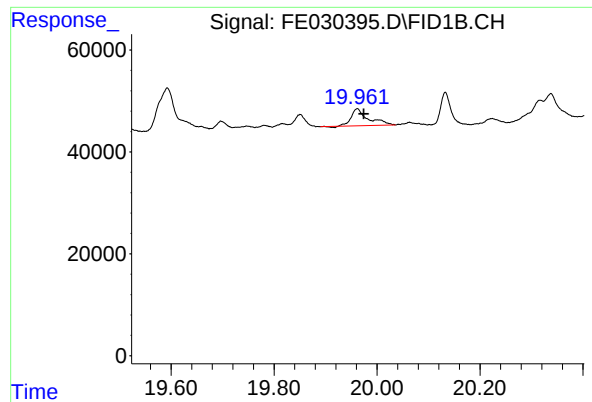

#14 N-HEXATRIACONTANE

R.T.: 19.962 min
Delta R.T.: -0.012 min
Response: 75435
Conc: 0.48 ug/ml

Instrument :
FID_E
ClientSampleId :
B14