

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
 Data File : FE030396.D
 Signal(s) : FID1B.CH
 Acq On : 10 Sep 2019 14:53
 Operator : DD\AJ
 Sample : K4758-19
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 B15

Integration File: autoint1.e
 Quant Time: Sep 11 00:47:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.548	4180226	21.005 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.752	127395	0.664 ug/ml
11)	N-OCTACOSANE	16.717	347551	1.846 ug/ml
12)	N-DOTRIACONTANE	18.433	363614	2.046 ug/ml
14)	N-HEXATRIACONTANE	19.963	30048	0.190 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090919\
Data File : FE030396.D
Signal(s) : FID1B.CH
Acq On : 10 Sep 2019 14:53
Operator : DD\AJ
Sample : K4758-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B15

Integration File: autoint1.e
Quant Time: Sep 11 00:47:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

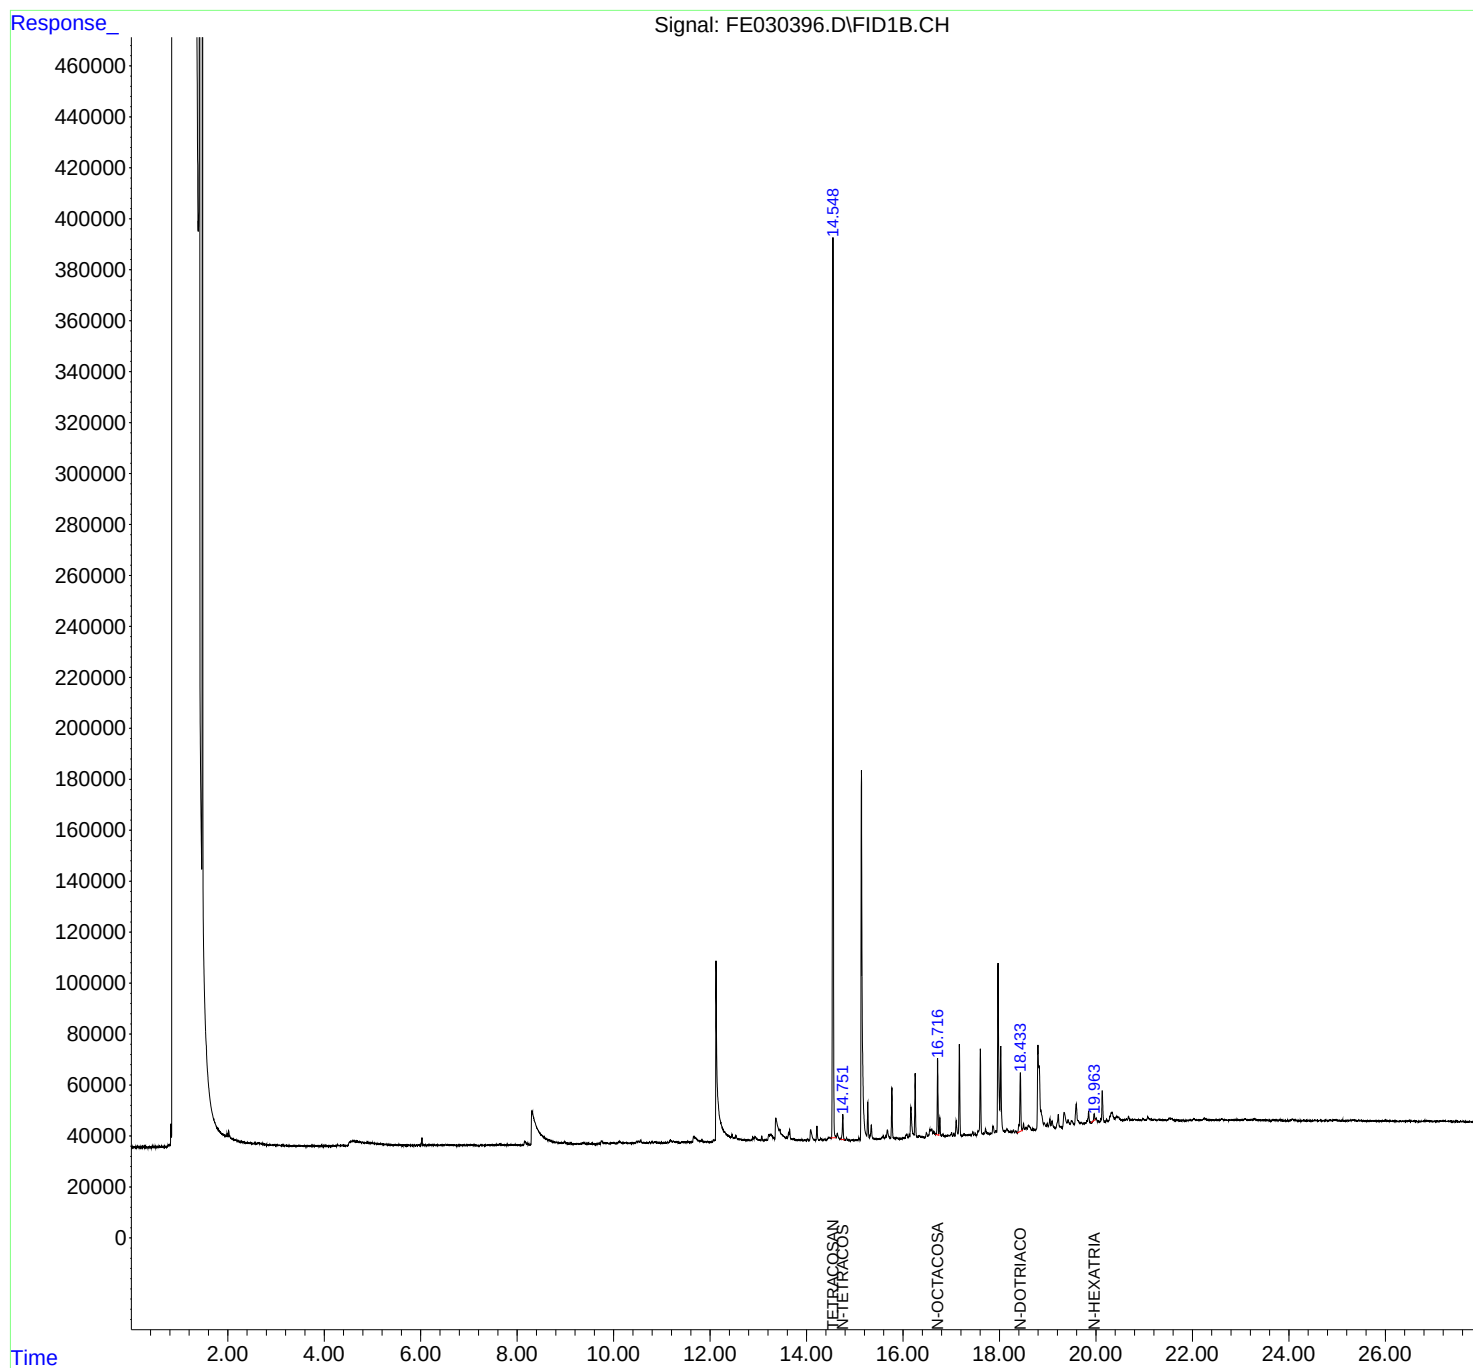


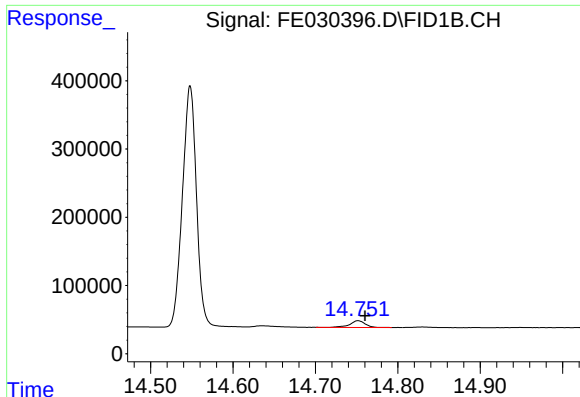

#10 N-TETRACOSANE


R.T.: 14.752 min
Delta R.T.: -0.008 min
Response: 127395
Conc: 0.66 ug/ml

Instrument :
FID_E
ClientSampleId :
B15

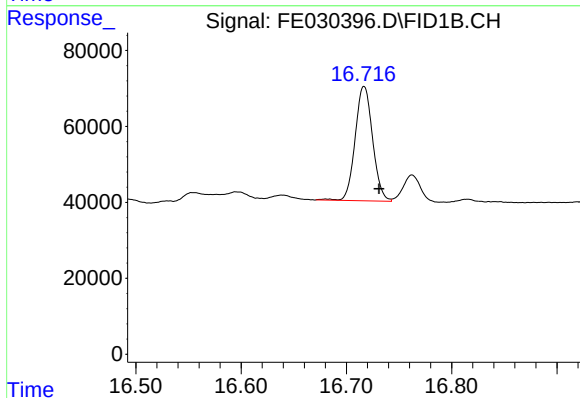


#11 N-OCTACOSANE

R.T.: 16.717 min
Delta R.T.: -0.014 min
Response: 347551
Conc: 1.85 ug/ml

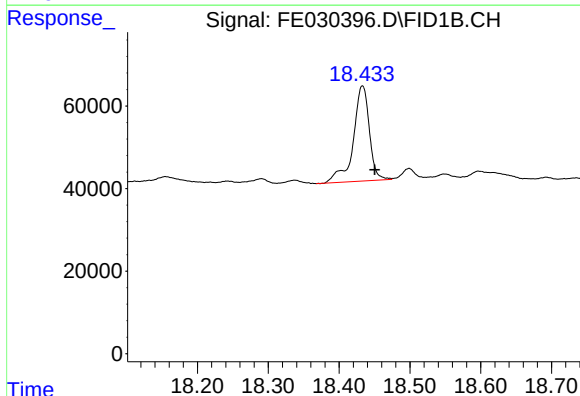


#12 N-DOTRIACONTANE

R.T.: 18.433 min
Delta R.T.: -0.018 min
Response: 363614
Conc: 2.05 ug/ml

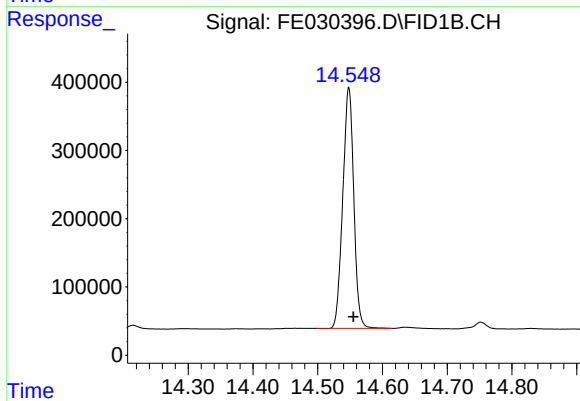

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.548 min
Delta R.T.: -0.007 min
Response: 4180226
Conc: 21.01 ug/ml

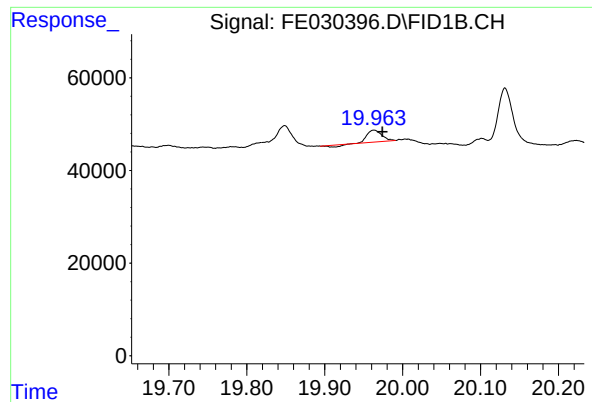

#14 N-HEXATRIACONTANE

R.T.: 19.963 min
Delta R.T.: -0.011 min
Response: 30048
Conc: 0.19 ug/ml

Instrument :
FID_E
ClientSampleId :
B15