

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090925AL\
Data File : FF016357.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2025 12:05
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 01:31:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 082825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 03:35:42 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	18.140	60123	0.483 ug/ml
18) T	n-Dotriacontane (C32)	18.973	104976	0.871 ug/ml
19) T	n-Tetratriacontane (C34)	19.759	87896	0.806 ug/ml
20) T	n-Hexatriacontane (C36)	20.504	54017	0.579 ug/ml
21) T	n-Octatriacontane (C38)	21.265	35940	0.427 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090925AL\
Data File : FF016357.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2025 12:05
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 01:31:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 082825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 03:35:42 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

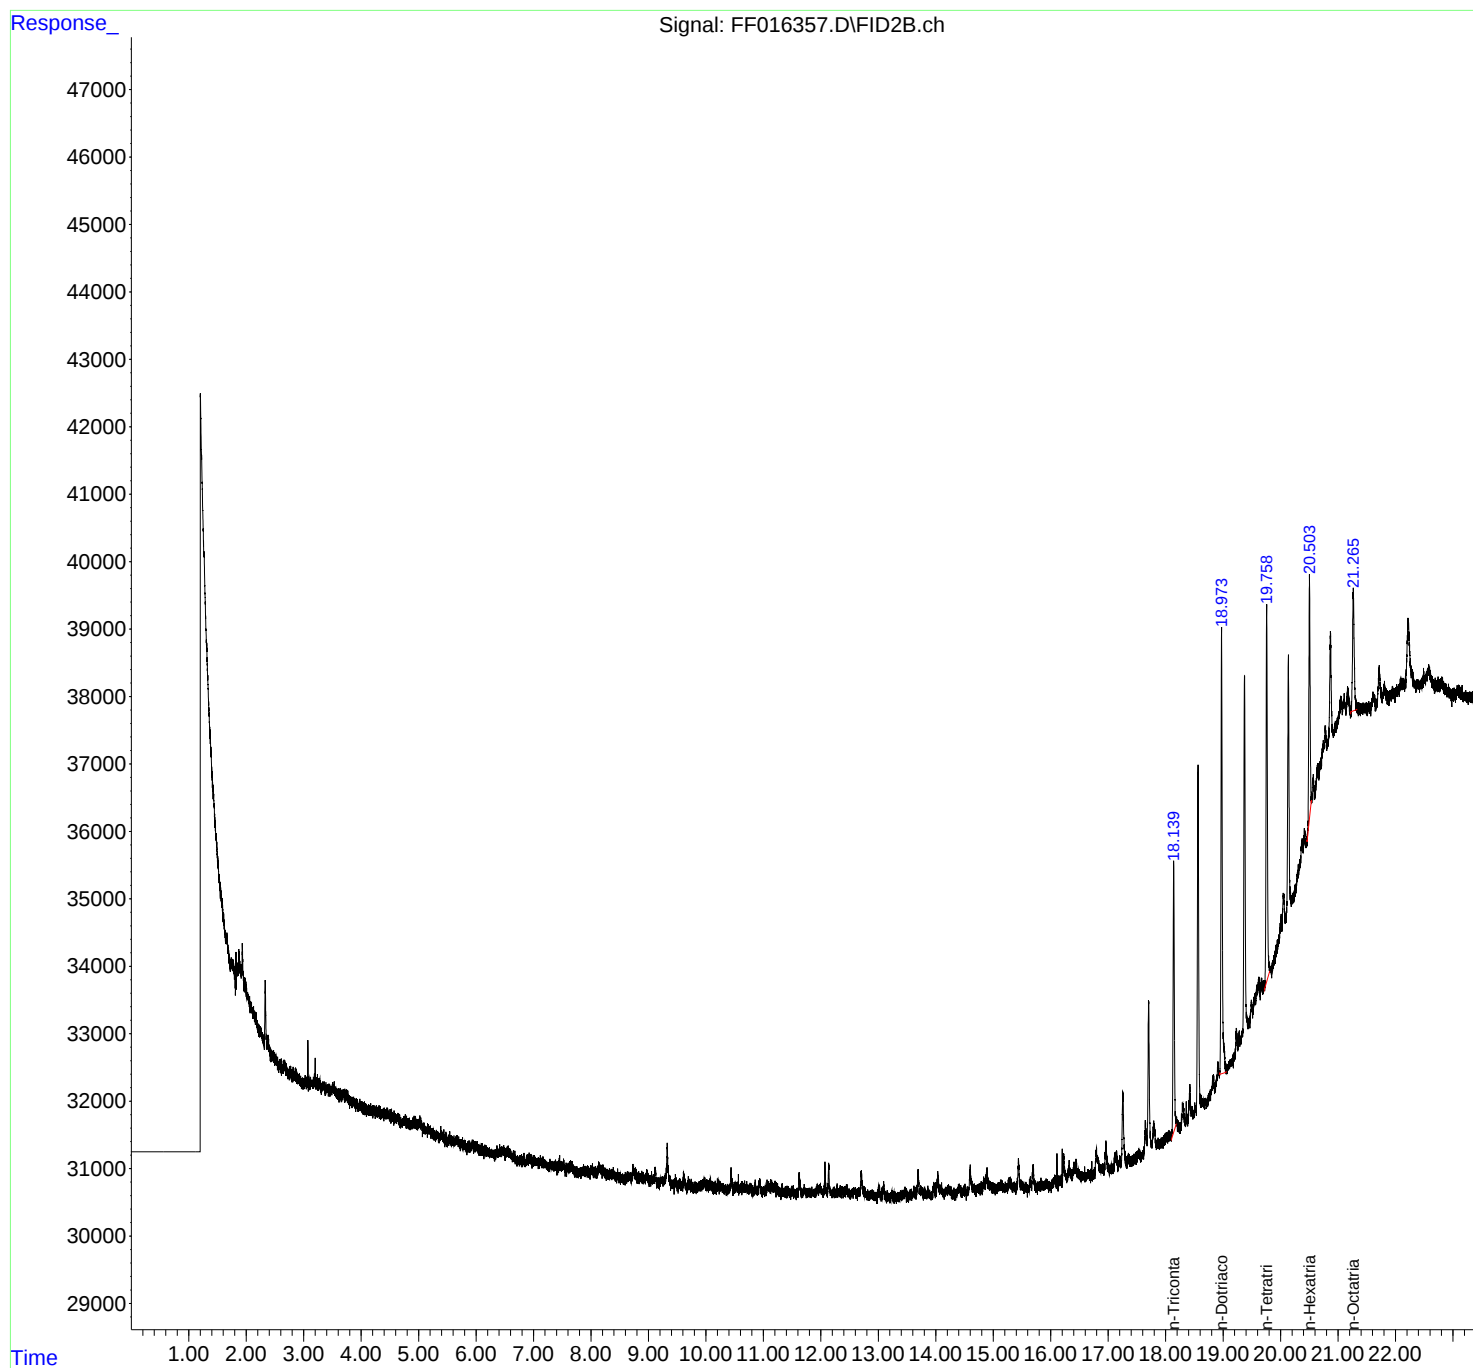


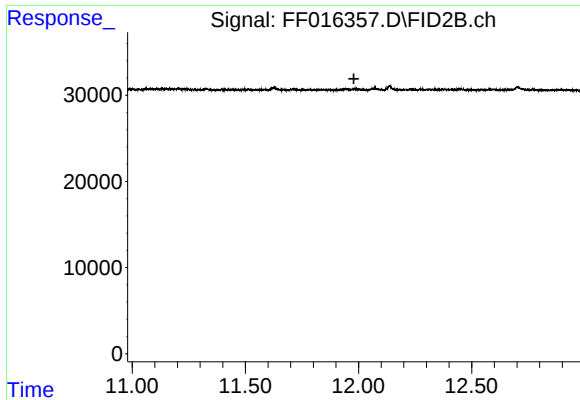

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.980 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

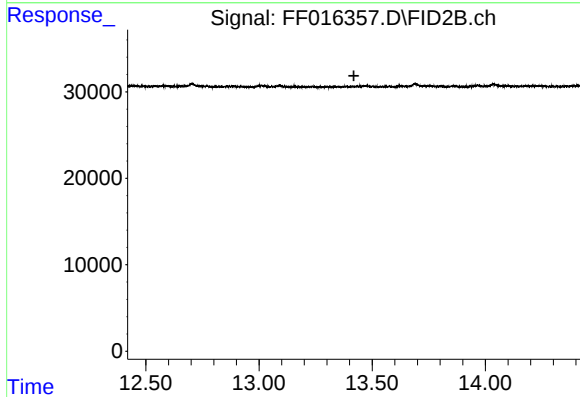


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.419 min
Response: 0
Conc: N.D.

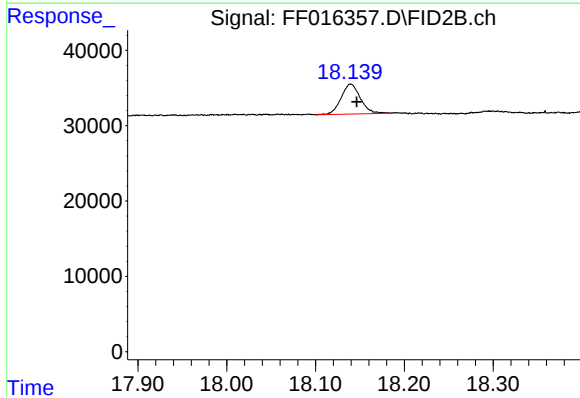


#17 n-Tricontane (C30)

R.T.: 18.140 min
Delta R.T.: -0.007 min
Response: 60123
Conc: 0.48 ug/ml

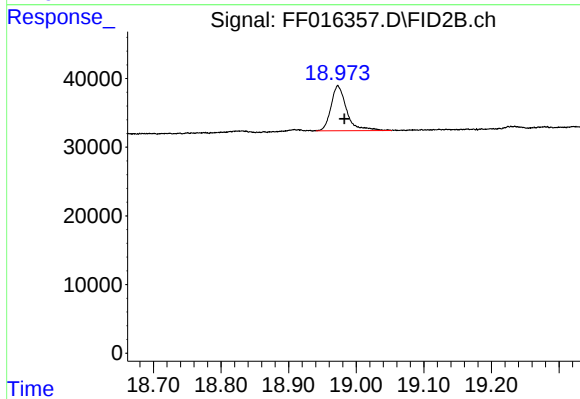

#18 n-Dotriacontane (C32)


R.T.: 18.973 min
Delta R.T.: -0.009 min
Response: 104976
Conc: 0.87 ug/ml

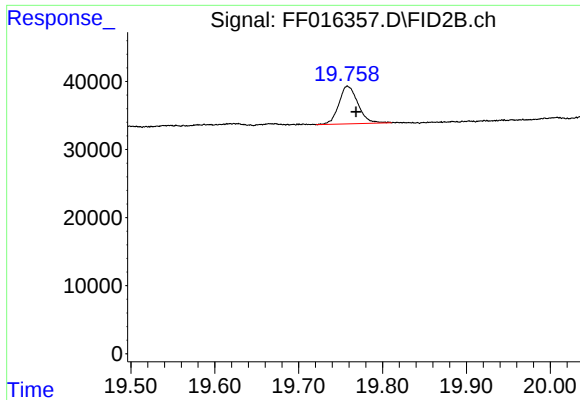

#19 n-Tetratriacontane (C34)


R.T.: 19.759 min
Delta R.T.: -0.010 min
Response: 87896
Conc: 0.81 ug/ml

Instrument :
FID_E
ClientSampleId :

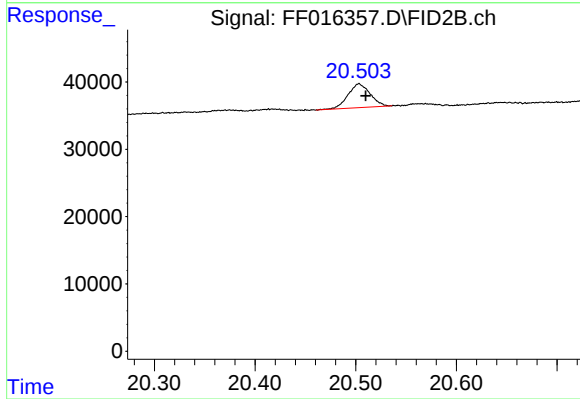

#20 n-Hexatriacontane (C36)

R.T.: 20.504 min
Delta R.T.: -0.007 min
Response: 54017
Conc: 0.58 ug/ml

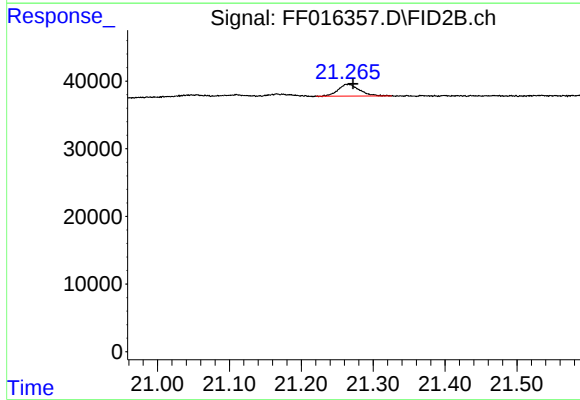

#21 n-Octatriacontane (C38)

R.T.: 21.265 min
Delta R.T.: -0.007 min
Response: 35940
Conc: 0.43 ug/ml