

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091019\
 Data File : FE030424.D
 Signal(s) : FID1B.CH
 Acq On : 11 Sep 2019 8:16
 Operator : DD\AJ
 Sample : K4759-20
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 11 13:55:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.544	3573416	17.956 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.744	398997	2.081 ug/ml
11)	N-OCTACOSANE	16.714	838460	4.454 ug/ml
12)	N-DOTRIACONTANE	18.432	547395	3.080 ug/ml
14)	N-HEXATRIACONTANE	19.957	56384	0.356 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091019\
Data File : FE030424.D
Signal(s) : FID1B.CH
Acq On : 11 Sep 2019 8:16
Operator : DD\AJ
Sample : K4759-20
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 11 13:55:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

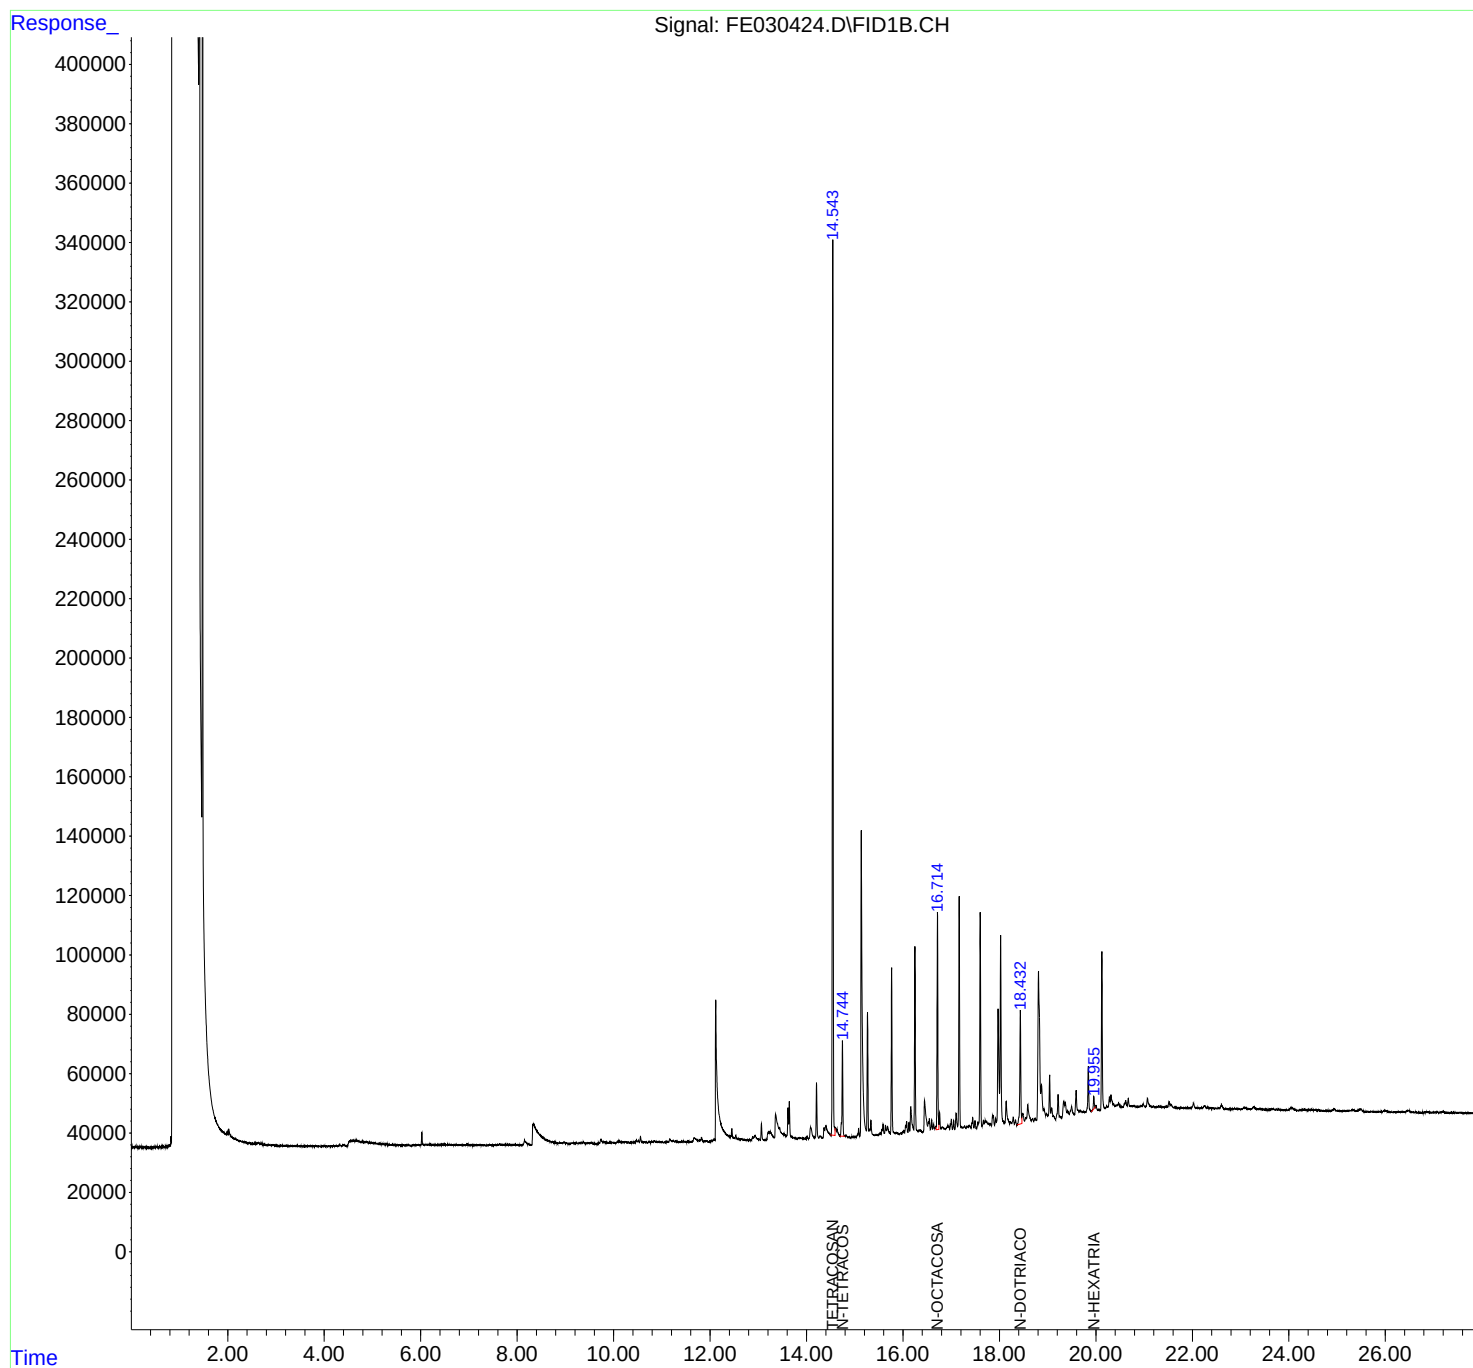

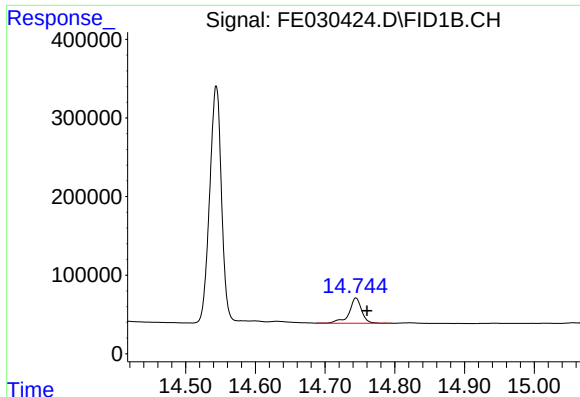


#10 N-TETRACOSANE

R.T.: 14.744 min
Delta R.T.: -0.016 min
Response: 398997
Conc: 2.08 ug/ml

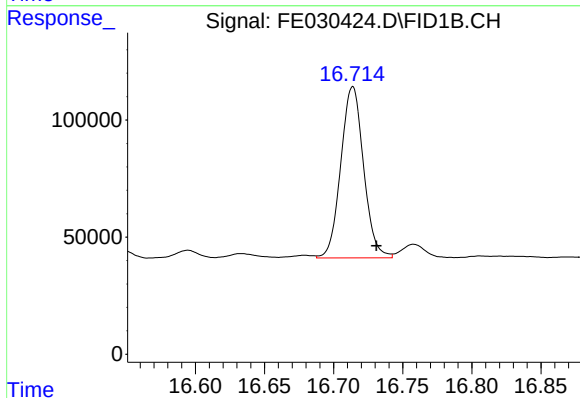


#11 N-OCTACOSANE

R.T.: 16.714 min
Delta R.T.: -0.017 min
Response: 838460
Conc: 4.45 ug/ml

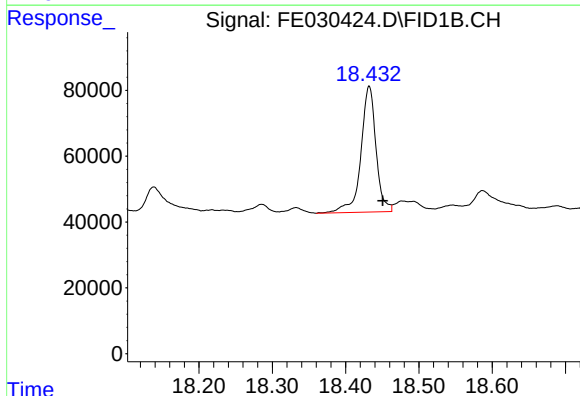


#12 N-DOTRIACONTANE

R.T.: 18.432 min
Delta R.T.: -0.018 min
Response: 547395
Conc: 3.08 ug/ml

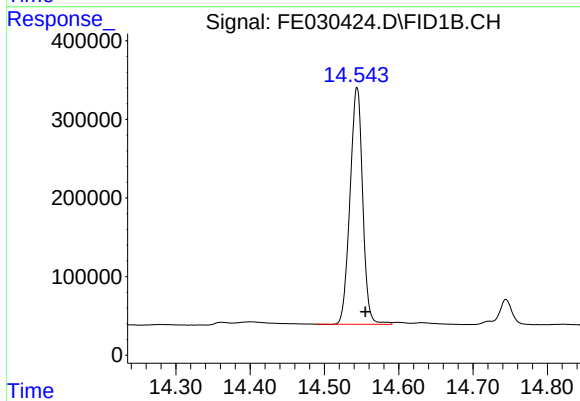

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.544 min
Delta R.T.: -0.011 min
Response: 3573416
Conc: 17.96 ug/ml

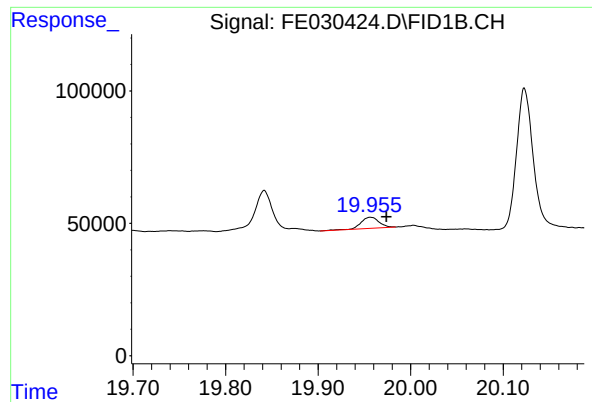

#14 N-HEXATRIACONTANE

R.T.: 19.957 min
Delta R.T.: -0.017 min
Response: 56384
Conc: 0.36 ug/ml