

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091021\
Data File : FE034322.D
Signal(s) : FID1B.CH
Acq On : 11 Sep 2021 00:37
Operator : DD\AJ
Sample : M3700-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 02:12:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE090821.M
Quant Title :
QLast Update : Thu Sep 09 02:48:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	6672334	20.025 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091021\
Data File : FE034322.D
Signal(s) : FID1B.CH
Acq On : 11 Sep 2021 00:37
Operator : DD\AJ
Sample : M3700-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 02:12:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE090821.M
Quant Title :
QLast Update : Thu Sep 09 02:48:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

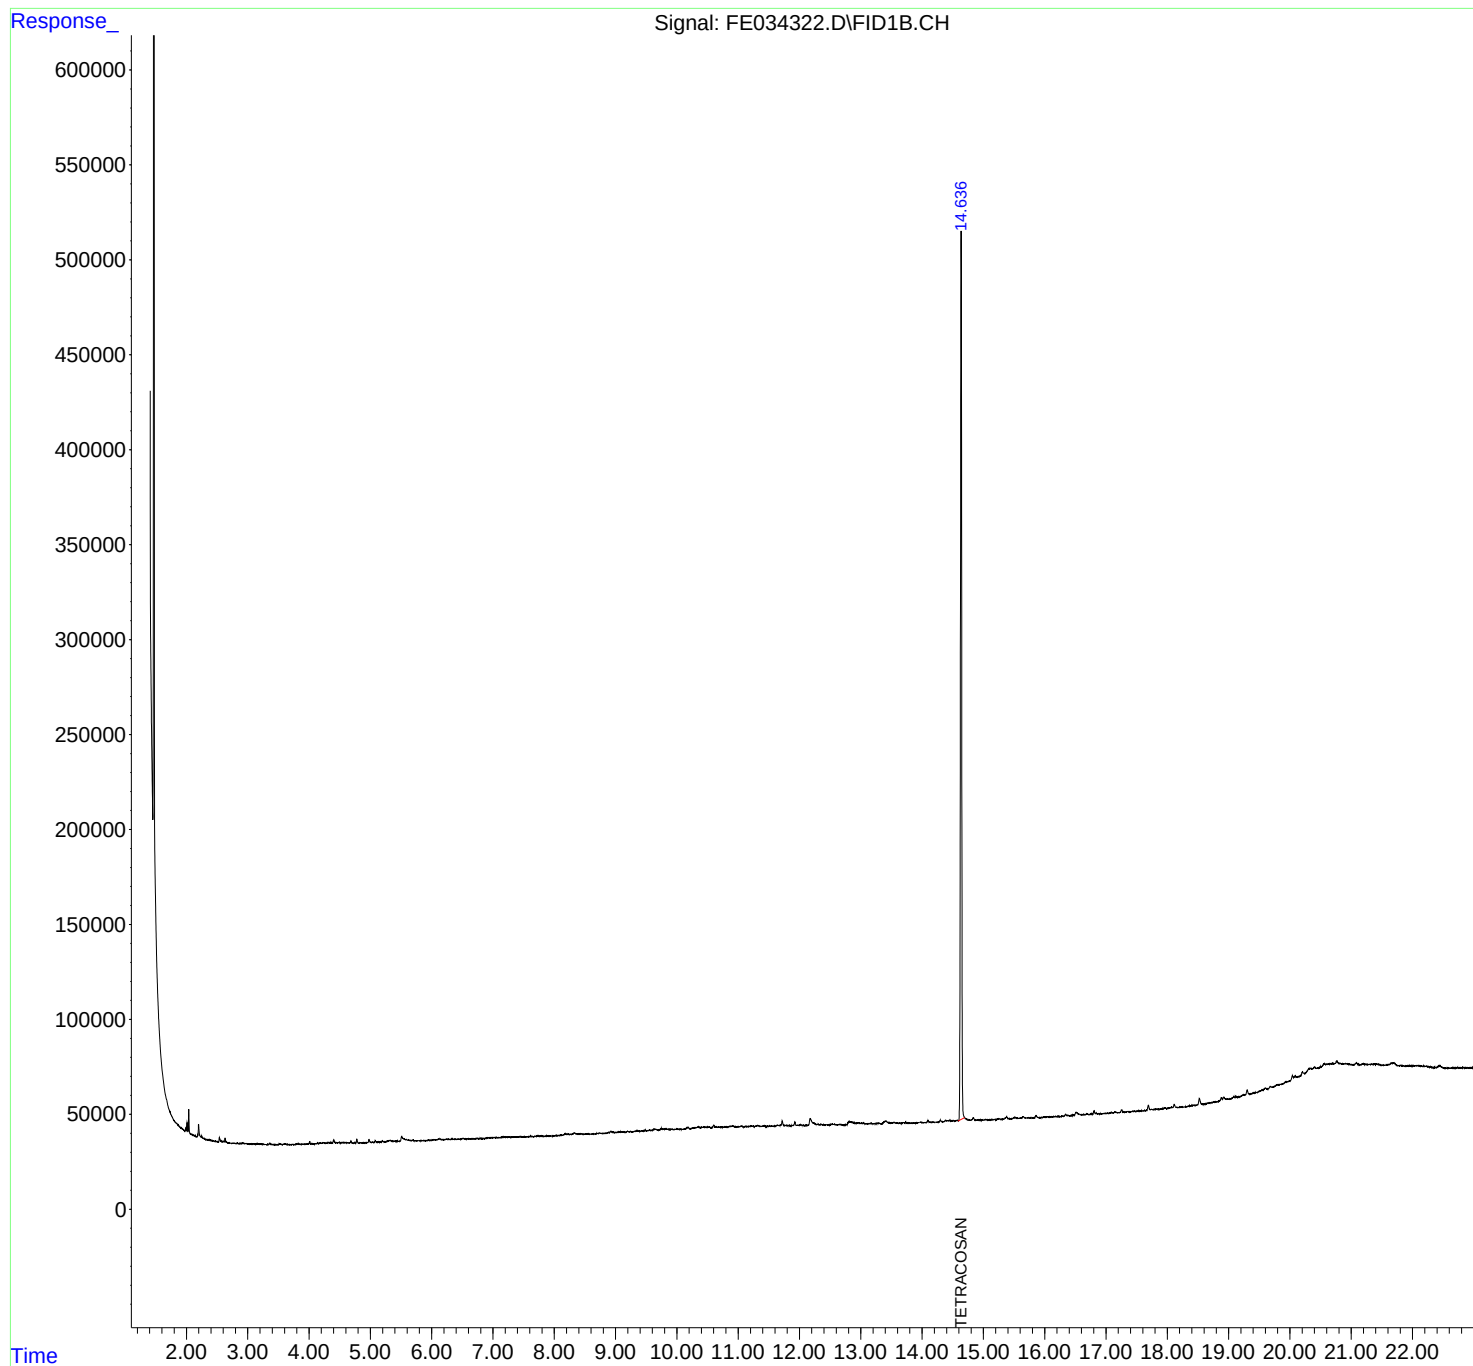

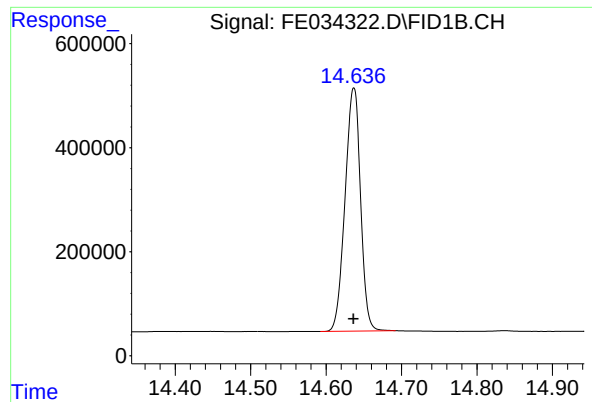

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.637 min
Delta R.T.: 0.000 min
Response: 6672334
Conc: 20.02 ug/ml

Instrument :
FID_E
ClientSampleId :