

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091025AL\
Data File : FE055740.D
Signal(s) : FID1B.ch
Acq On : 10 Sep 2025 09:49
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Sep 11 00:24:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082925.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 08:12:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.239	105750	0.715 ug/ml
18) T	n-Dotriacontane (C32)	19.075	136649	0.931 ug/ml
19) T	n-Tetratriacontane (C34)	19.860	99092	0.701 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091025AL\
Data File : FE055740.D
Signal(s) : FID1B.ch
Acq On : 10 Sep 2025 09:49
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Sep 11 00:24:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082925.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 08:12:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

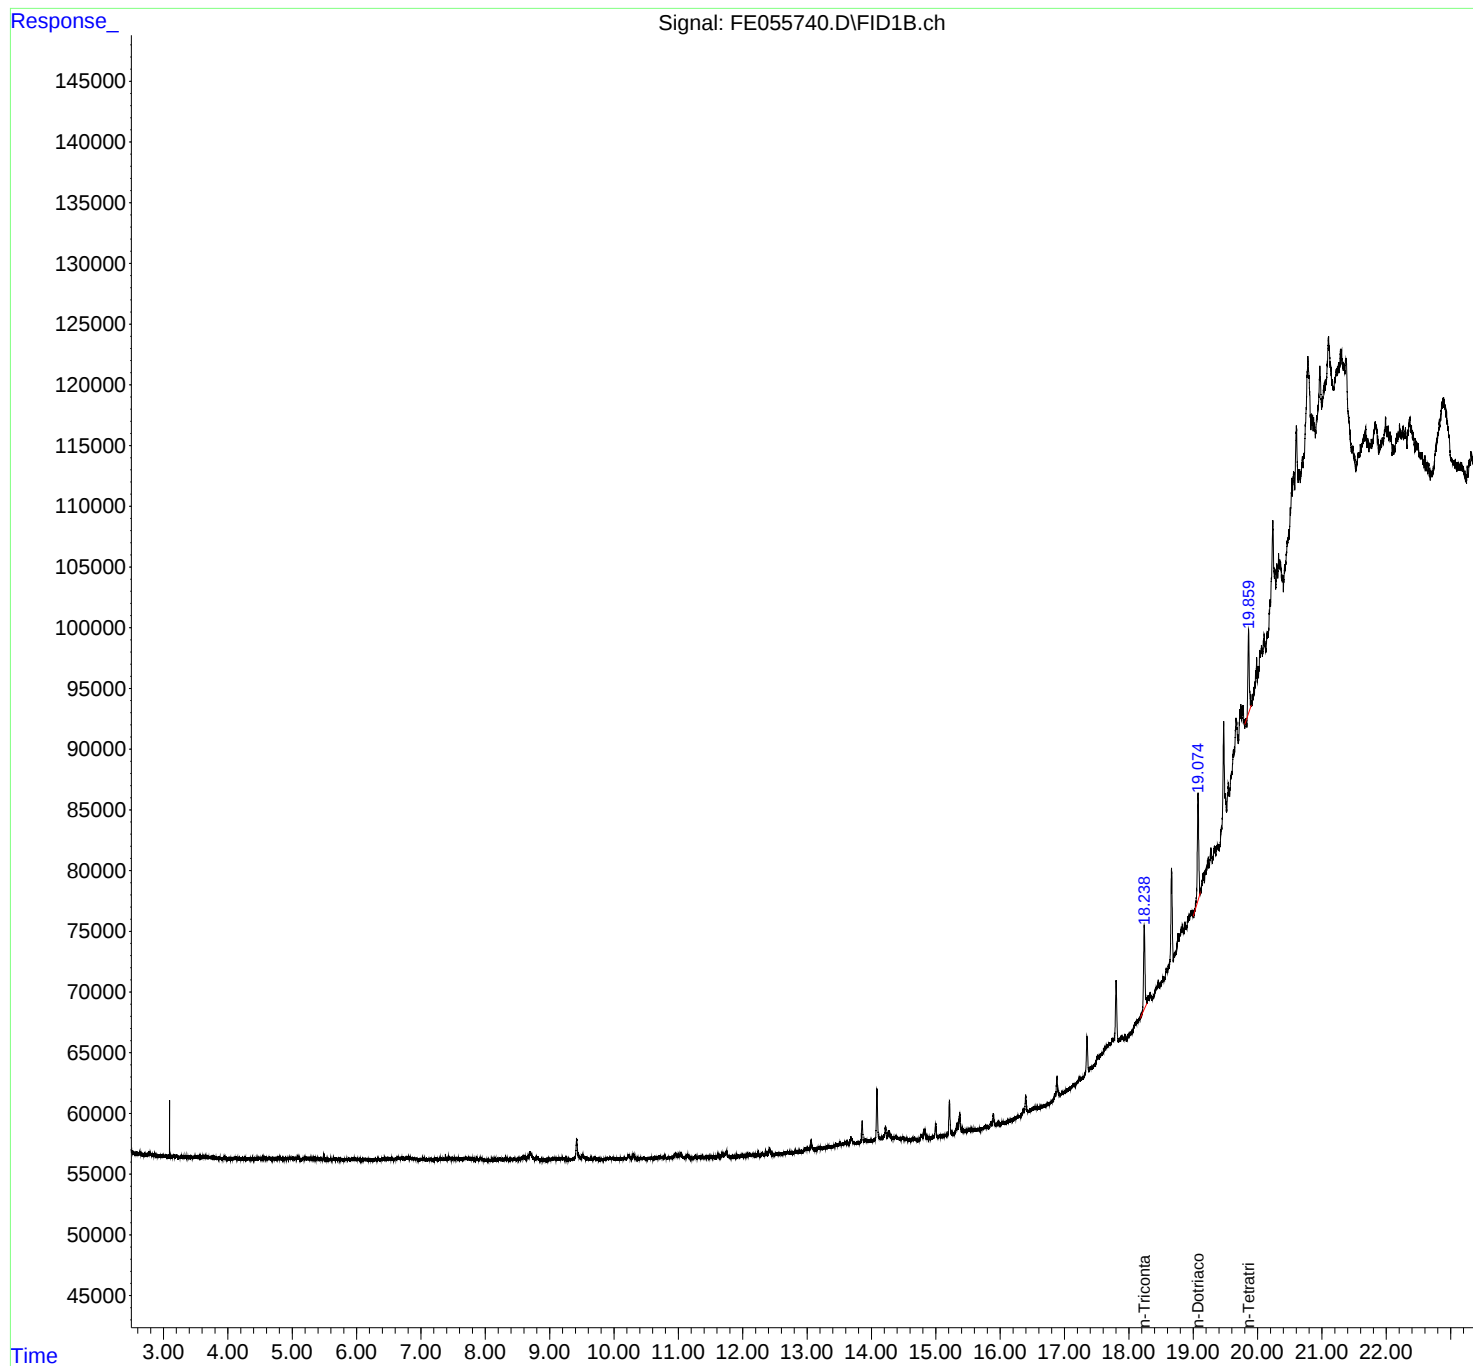


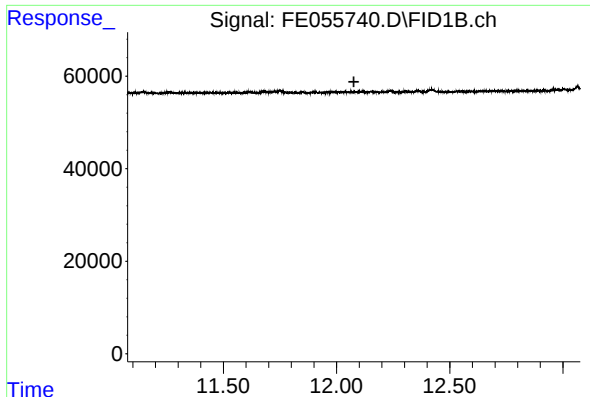

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 12.077 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

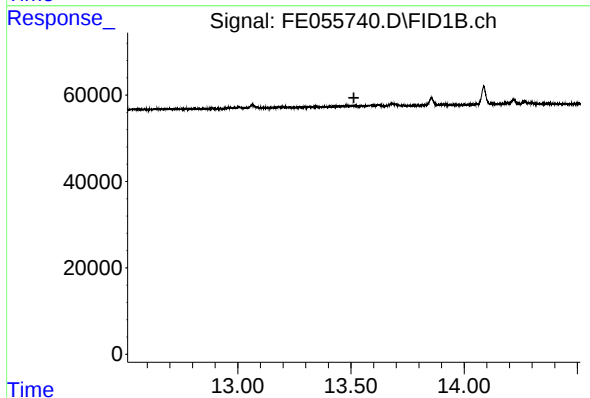


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.513 min
Response: 0
Conc: N.D.

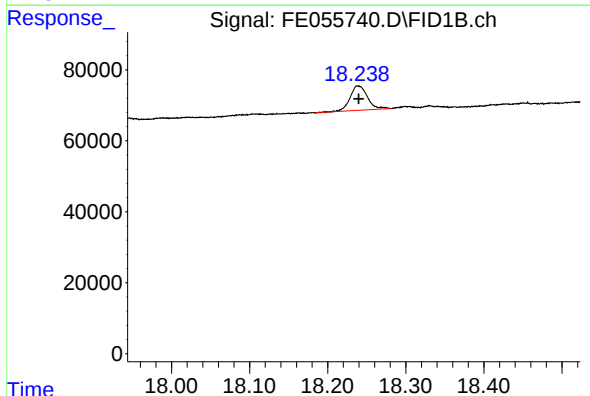


#17 n-Tricontane (C30)

R.T.: 18.239 min
Delta R.T.: 0.000 min
Response: 105750
Conc: 0.72 ug/ml

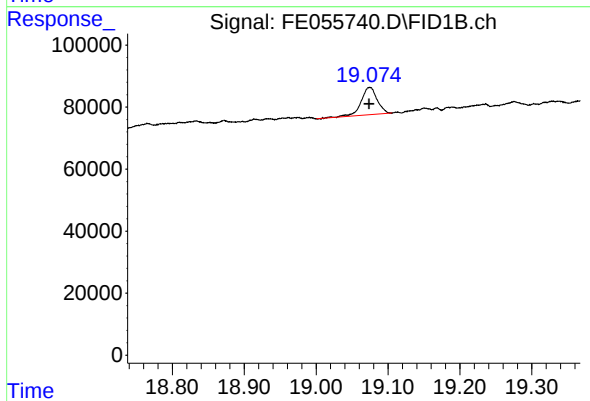

#18 n-Dotriacontane (C32)

R.T.: 19.075 min
Delta R.T.: 0.000 min
Response: 136649
Conc: 0.93 ug/ml

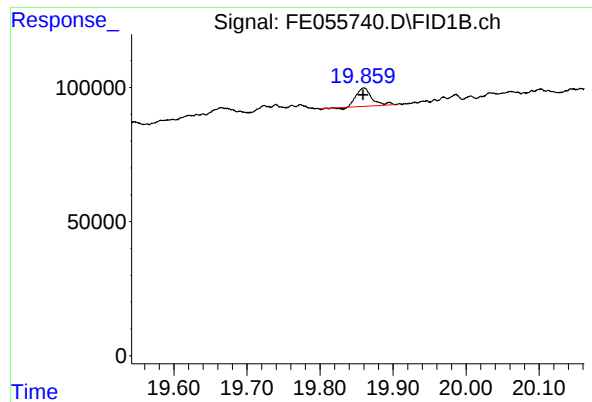

#19 n-Tetratriacontane (C34)

R.T.: 19.860 min
Delta R.T.: 0.000 min
Response: 99092
Conc: 0.70 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2