

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG091025AL\  
 Data File : FG016587.D  
 Signal(s) : FID1A.ch  
 Acq On : 10 Sep 2025 10:58  
 Operator : YP\AJ  
 Sample : PB169439BL  
 Misc :  
 ALS Vial : 71 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Sep 11 04:50:36 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\Aliphatic EPH 082825.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Aug 28 12:01:28 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.512 | 3350185    | 33.283 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 66.57%       |
| Target Compounds               |        |            |              |
| 17) T n-Tricontane (C30)       | 18.258 | 78132      | 0.715 ug/ml  |
| 18) T n-Dotriacontane (C32)    | 19.095 | 108034     | 1.028 ug/ml  |
| 19) T n-Tetratriacontane (C34) | 19.883 | 86987      | 0.906 ug/ml  |
| 20) T n-Hexatriacontane (C36)  | 20.629 | 54859      | 0.656 ug/ml  |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG091025AL\  
Data File : FG016587.D  
Signal(s) : FID1A.ch  
Acq On : 10 Sep 2025 10:58  
Operator : YP\AJ  
Sample : PB169439BL  
Misc :  
ALS Vial : 71 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 11 04:50:36 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\Aliphatic EPH 082825.M  
Quant Title : GC Extractables  
QLast Update : Thu Aug 28 12:01:28 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

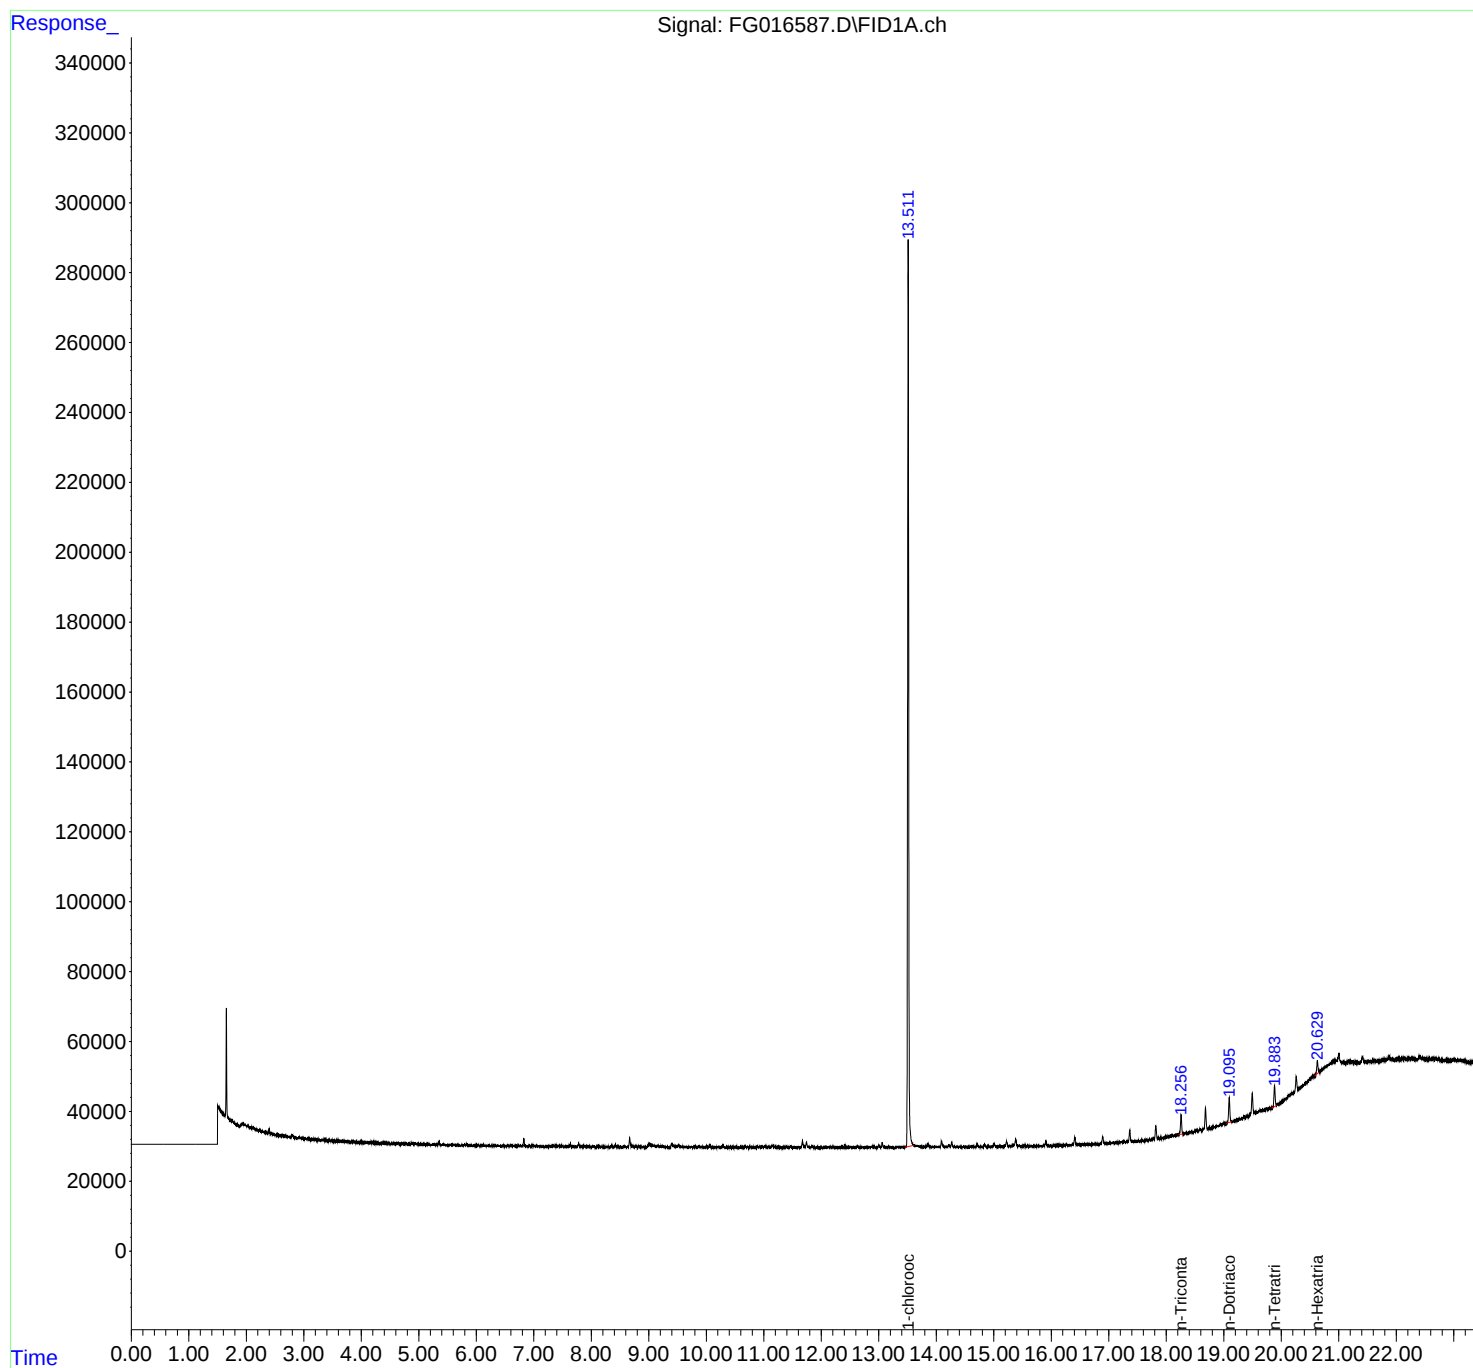


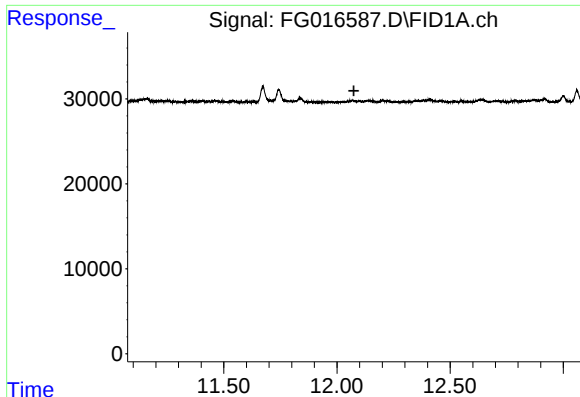

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T.: 12.075 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

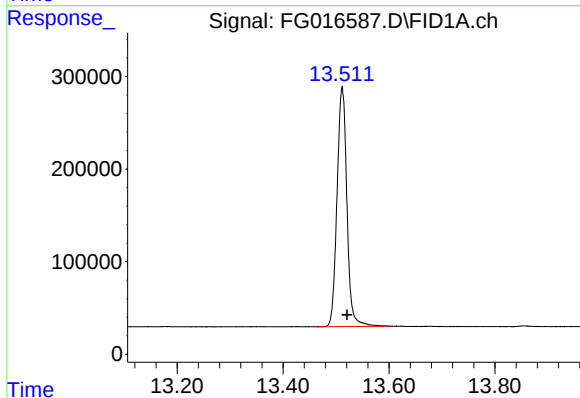


#12 1-chlorooctadecane (SURR)

R.T.: 13.512 min  
Delta R.T.: -0.009 min  
Response: 3350185  
Conc: 33.28 ug/ml

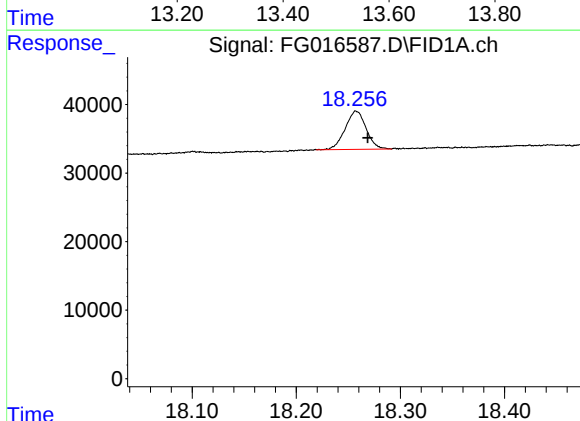


#17 n-Tricontane (C30)

R.T.: 18.258 min  
Delta R.T.: -0.011 min  
Response: 78132  
Conc: 0.72 ug/ml

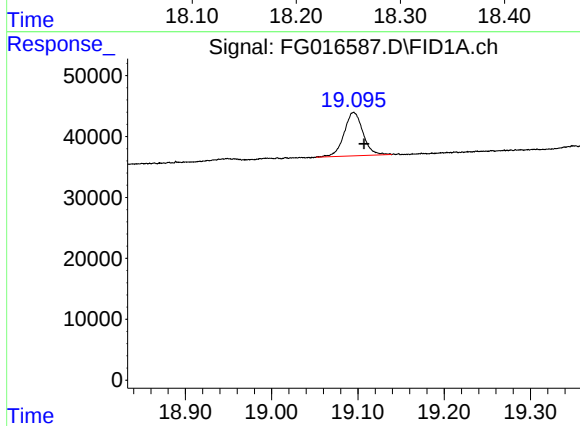

#18 n-Dotriacontane (C32)


R.T.: 19.095 min  
Delta R.T.: -0.012 min  
Response: 108034  
Conc: 1.03 ug/ml

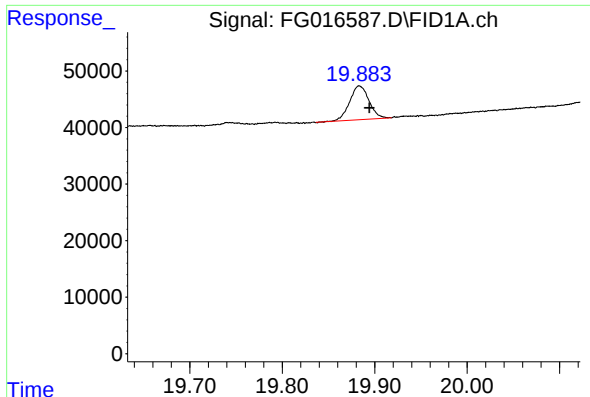

#19 n-Tetratriacontane (C34)

R.T.: 19.883 min  
Delta R.T.: -0.011 min  
Response: 86987  
Conc: 0.91 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

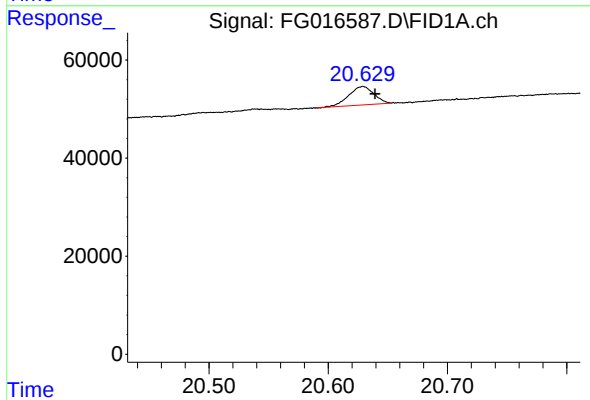

#20 n-Hexatriacontane (C36)

R.T.: 20.629 min  
Delta R.T.: -0.010 min  
Response: 54859  
Conc: 0.66 ug/ml