

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091119\
 Data File : FE030436.D
 Signal(s) : FID1B.CH
 Acq On : 11 Sep 2019 16:36
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Sep 12 05:46:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
 Quant Title :
 QLast Update : Mon Sep 09 04:07:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
5) N-DODECANE	6.319	14252727	75.106	ug/ml
11) N-OCTACOSANE	16.734	14462424	76.831	ug/ml
12) N-DOTRIACONTANE	18.433	761393	4.284	ug/ml
14) N-HEXATRIACONTANE	19.958	328243	2.071	ug/ml
15) N-TETRACONTANE	21.520	69581	0.498	ug/ml
16) N-TETRTETRACOCANE	24.052	241215	1.969	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091119\
Data File : FE030436.D
Signal(s) : FID1B.CH
Acq On : 11 Sep 2019 16:36
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 12 05:46:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

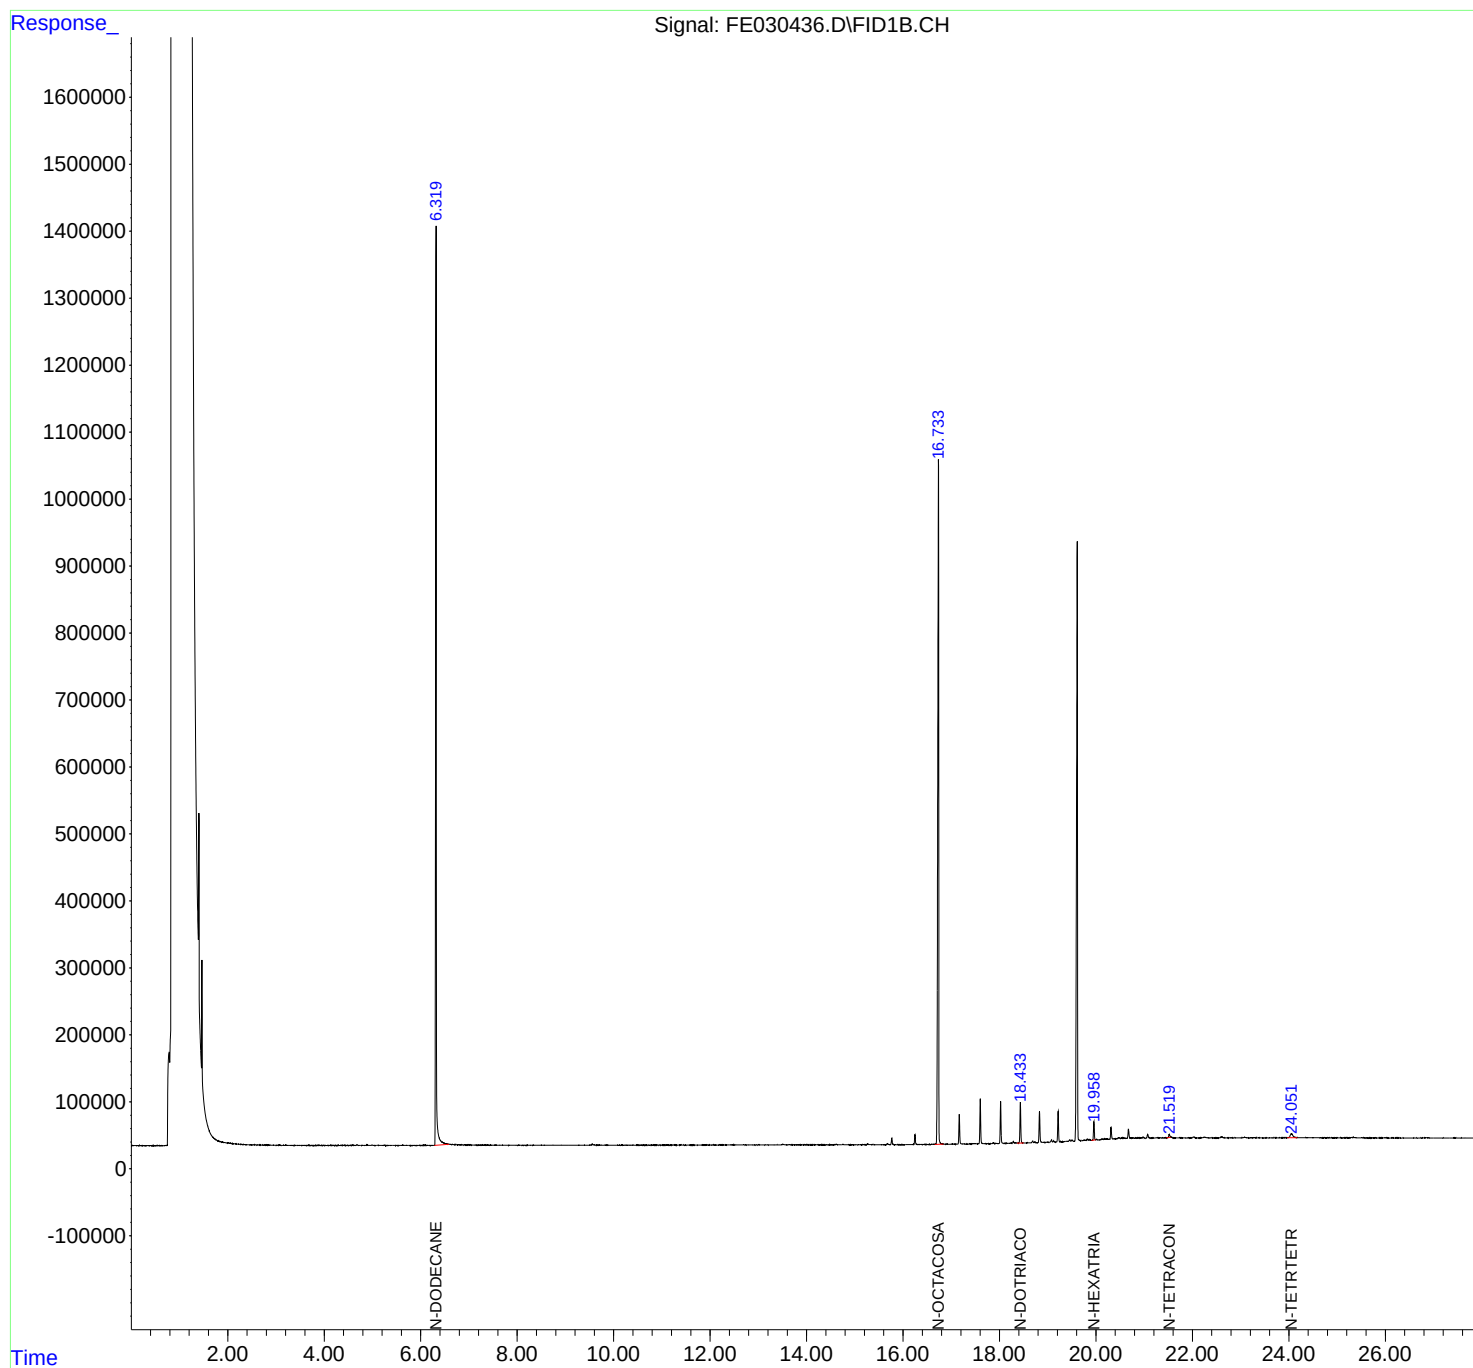


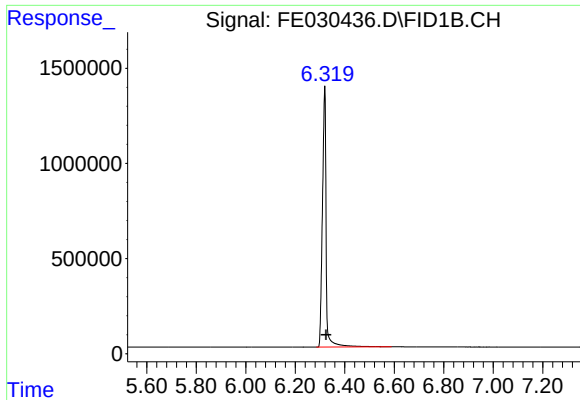

#5 N-DODECANE


R.T.: 6.319 min
Delta R.T.: -0.006 min
Response: 14252727
Conc: 75.11 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

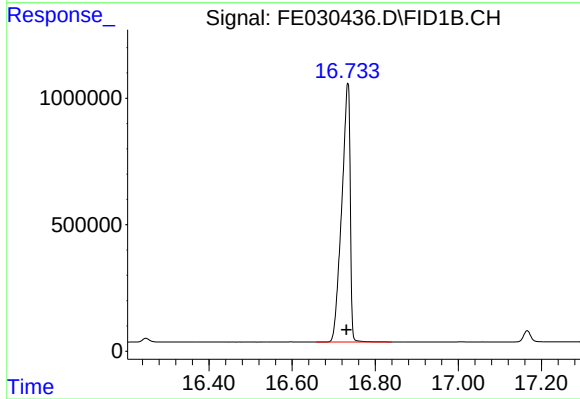


#11 N-OCTACOSANE

R.T.: 16.734 min
Delta R.T.: 0.003 min
Response: 14462424
Conc: 76.83 ug/ml

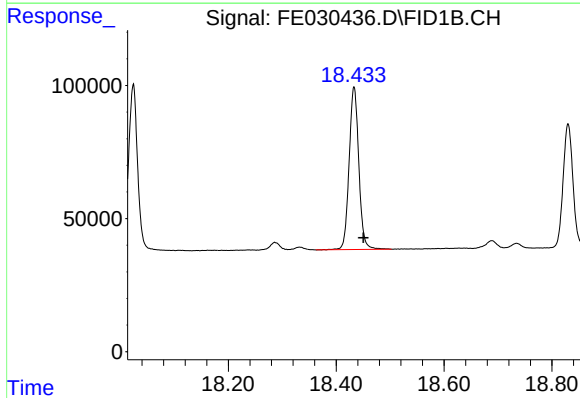


#12 N-DOTRIACONTANE

R.T.: 18.433 min
Delta R.T.: -0.017 min
Response: 761393
Conc: 4.28 ug/ml

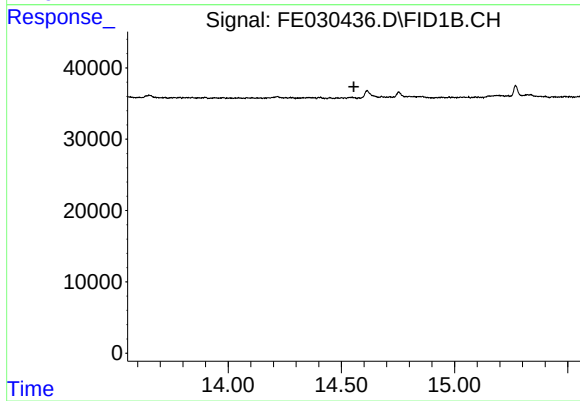

#13 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.555 min
Response: 0
Conc: N.D.

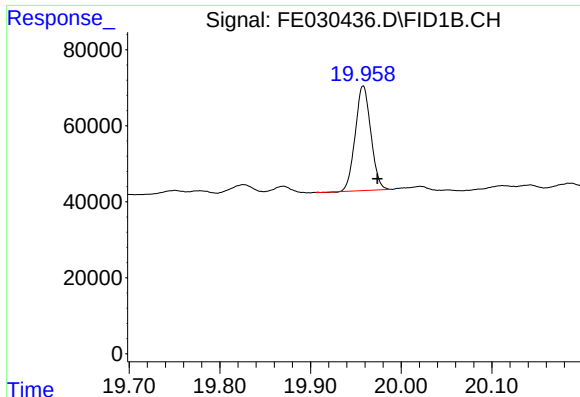

#14 N-HEXATRIACONTANE


R.T.: 19.958 min
Delta R.T.: -0.016 min
Response: 328243
Conc: 2.07 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

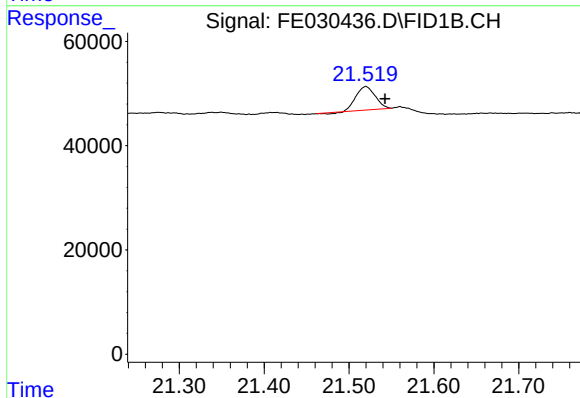

#15 N-TETRACONTANE

R.T.: 21.520 min
Delta R.T.: -0.023 min
Response: 69581
Conc: 0.50 ug/ml

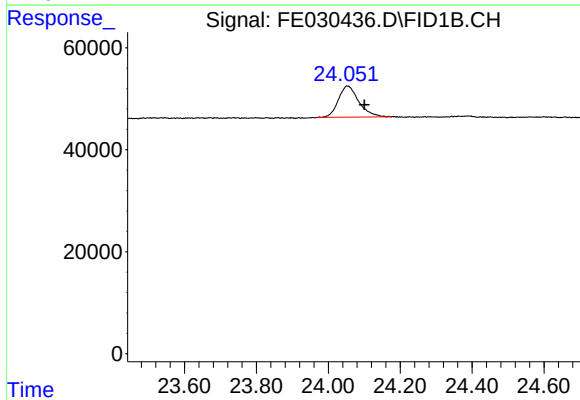

#16 N-TETRTETRACOTANE

R.T.: 24.052 min
Delta R.T.: -0.049 min
Response: 241215
Conc: 1.97 ug/ml