

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091125AL\
Data File : FE055768.D
Signal(s) : FID1B.ch
Acq On : 11 Sep 2025 11:30
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 12 01:19:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082925.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 08:12:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.237	100730	0.681 ug/ml
18) T	n-Dotriacontane (C32)	19.070	137639	0.938 ug/ml
19) T	n-Tetratriacontane (C34)	19.856	97931	0.693 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091125AL\
Data File : FE055768.D
Signal(s) : FID1B.ch
Acq On : 11 Sep 2025 11:30
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 12 01:19:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082925.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 08:12:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

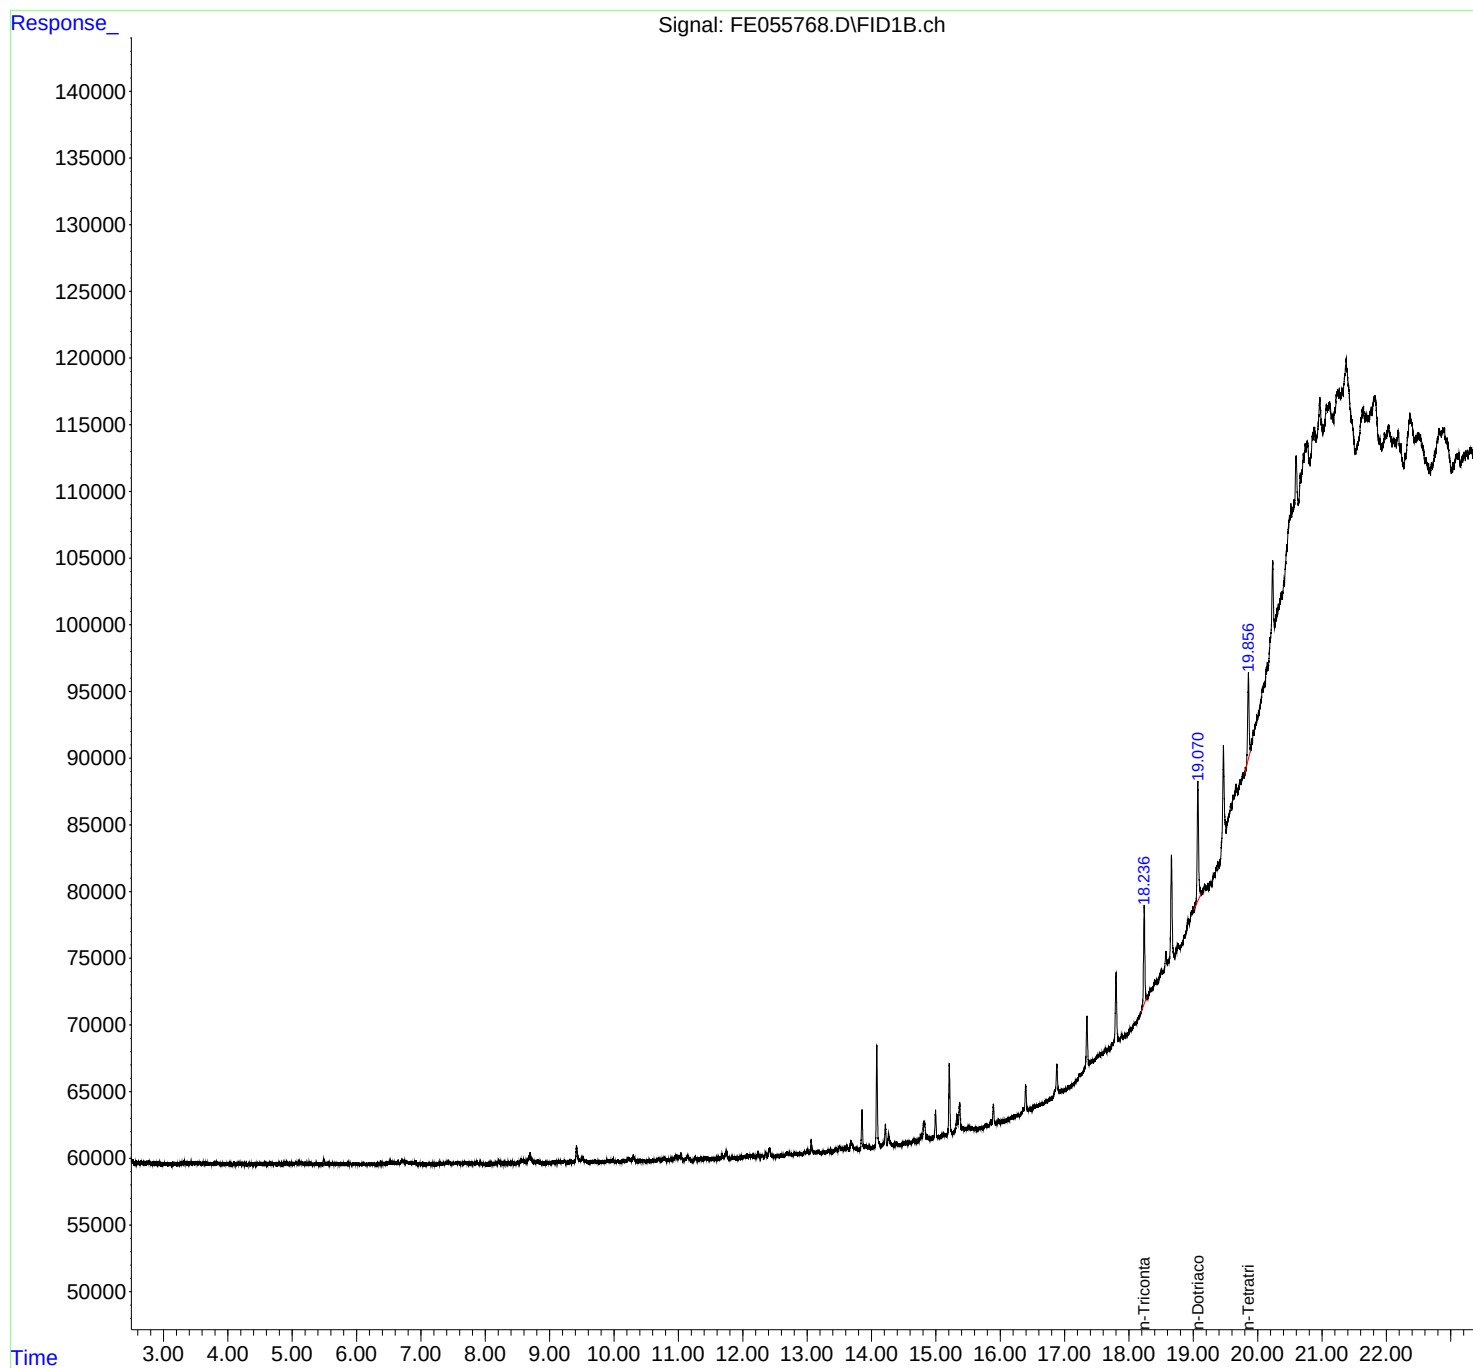


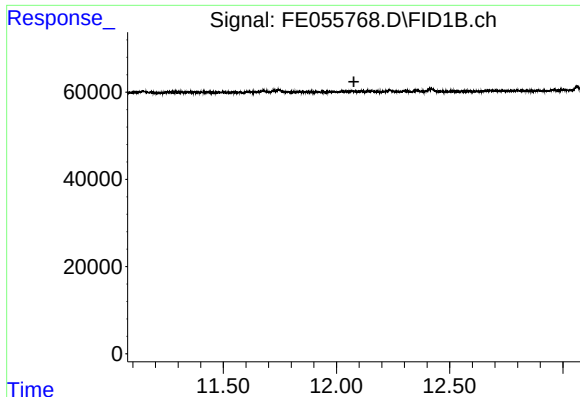

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 12.077 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
I.BLK

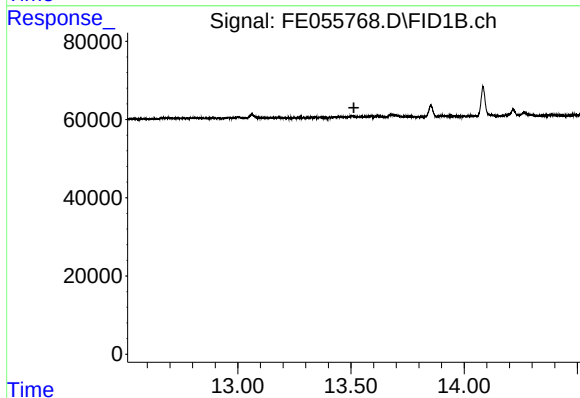


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.513 min
Response: 0
Conc: N.D.

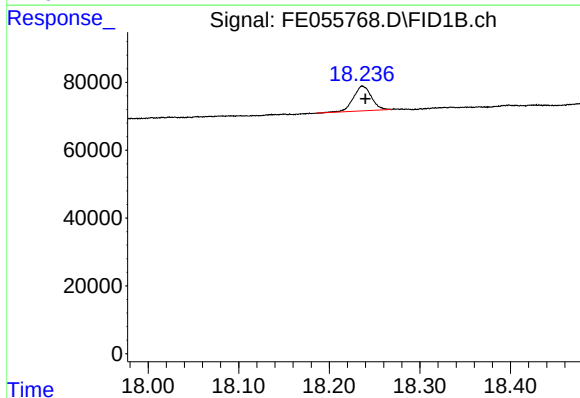


#17 n-Tricontane (C30)

R.T.: 18.237 min
Delta R.T.: -0.003 min
Response: 100730
Conc: 0.68 ug/ml

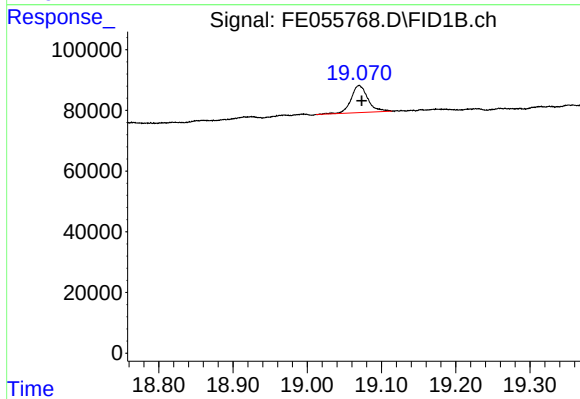

#18 n-Dotriacontane (C32)

R.T.: 19.070 min
Delta R.T.: -0.004 min
Response: 137639
Conc: 0.94 ug/ml

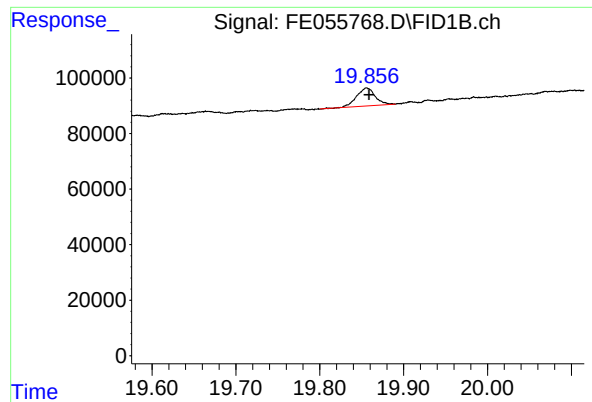

#19 n-Tetratriacontane (C34)

R.T.: 19.856 min
Delta R.T.: -0.003 min
Response: 97931
Conc: 0.69 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK