

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091222AL\
 Data File : FE037489.D
 Signal(s) : FID1B.ch
 Acq On : 12 Sep 2022 10:12
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 13 06:48:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T n-Tetratriacontane (C34)	19.368	22070	0.174 ug/ml
21) T n-Octatriacontane (C38)	20.798	150998	1.213 ug/ml
22) T n-Tetracontane (C40)	21.617	107716	0.836 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091222AL\
Data File : FE037489.D
Signal(s) : FID1B.ch
Acq On : 12 Sep 2022 10:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 06:48:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

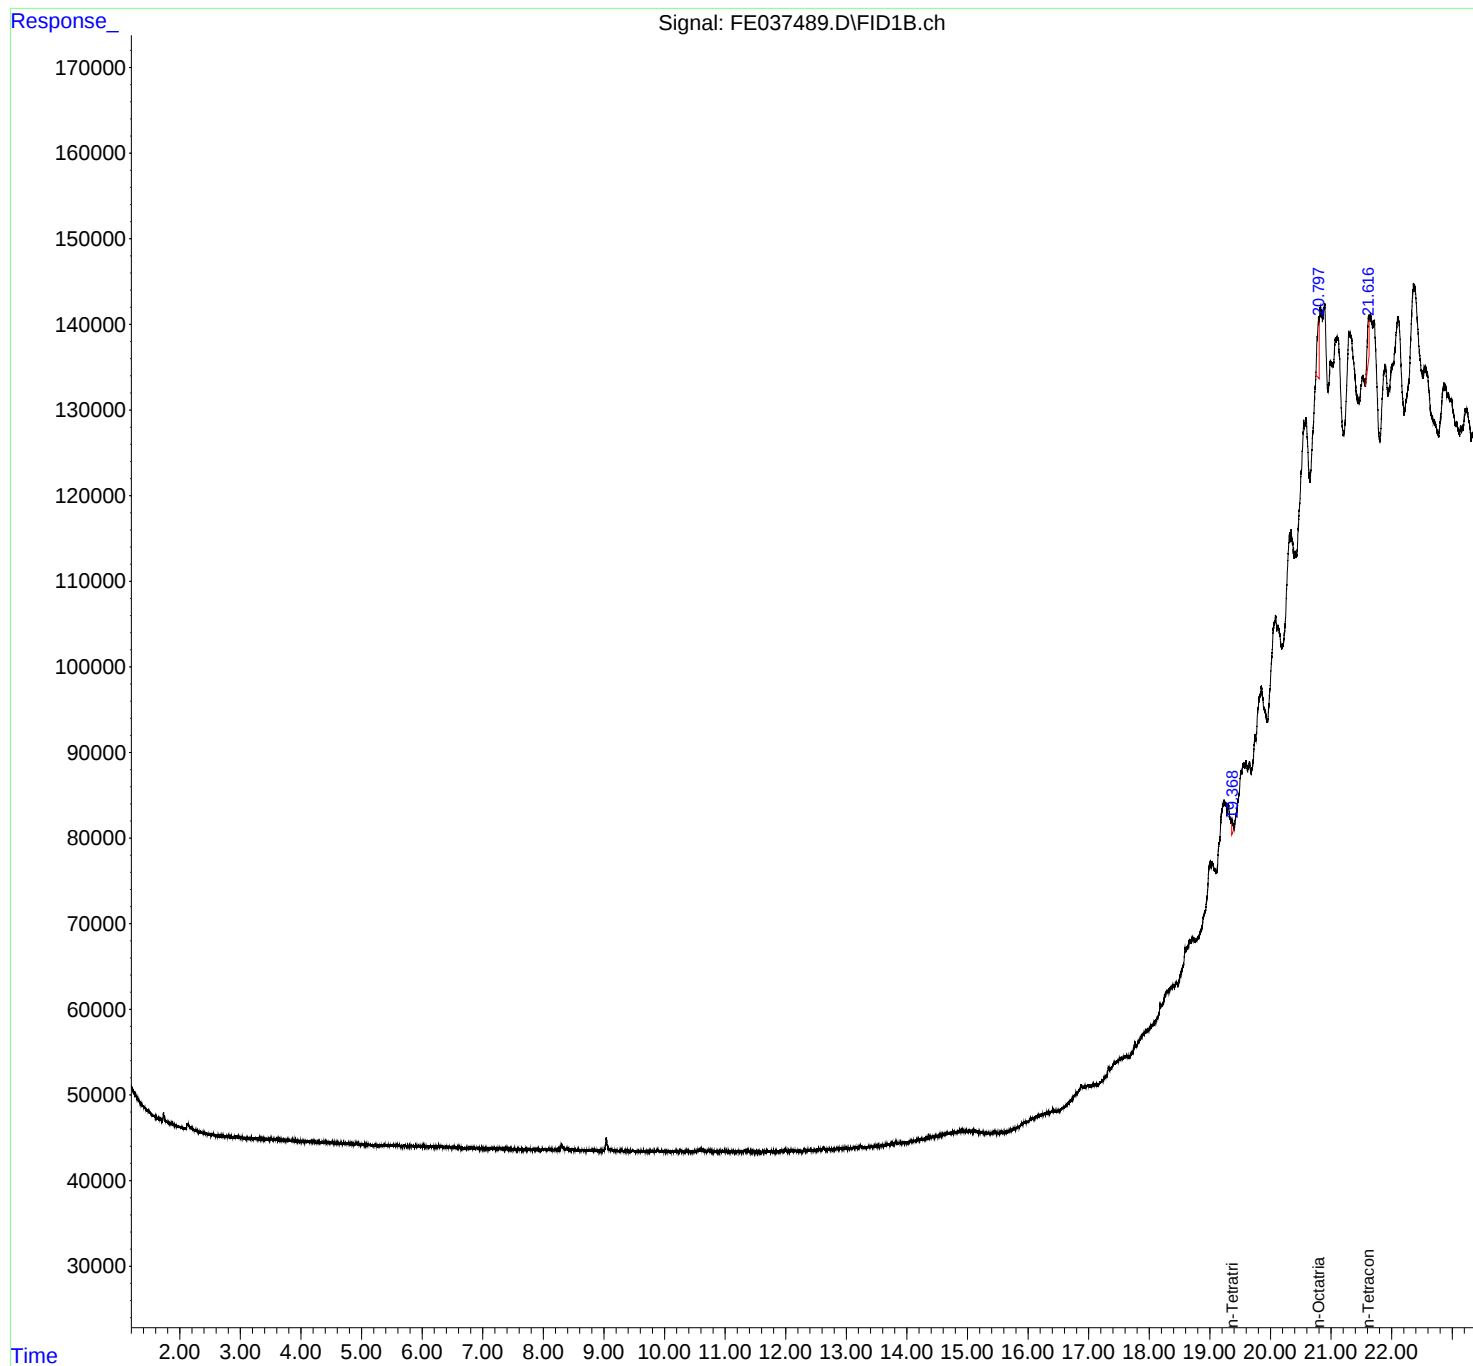


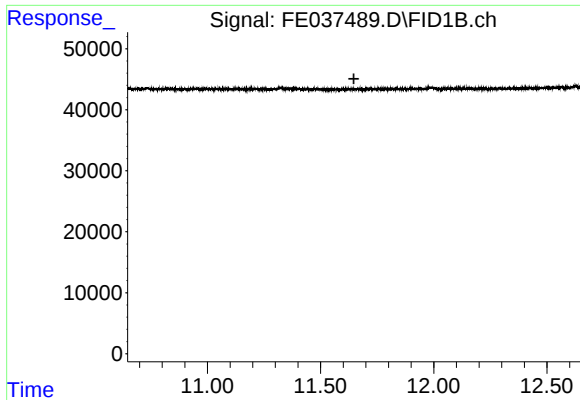

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.647 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

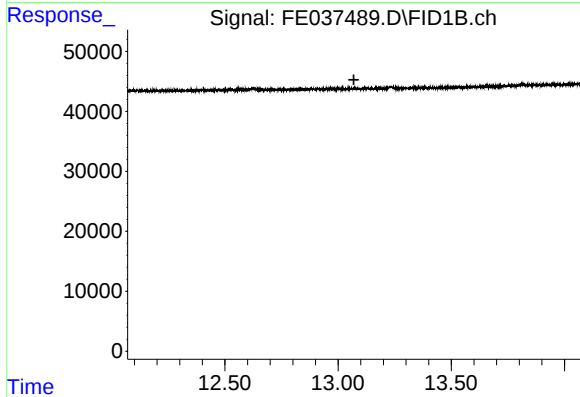


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.070 min
Response: 0
Conc: N.D.

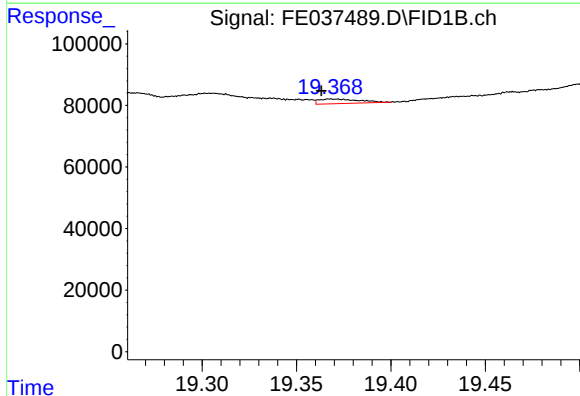


#19 n-Tetratriacontane (C34)

R.T.: 19.368 min
Delta R.T.: 0.005 min
Response: 22070
Conc: 0.17 ug/ml

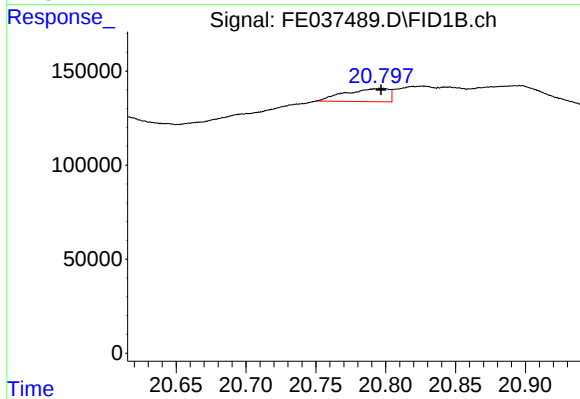

#21 n-Octatriacontane (C38)

R.T.: 20.798 min
Delta R.T.: 0.001 min
Response: 150998
Conc: 1.21 ug/ml

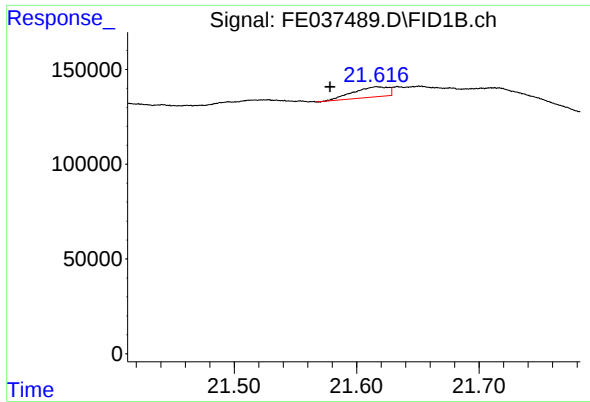

#22 n-Tetracontane (C40)

R.T.: 21.617 min
Delta R.T.: 0.038 min
Response: 107716
Conc: 0.84 ug/ml

Instrument :
FID_E
ClientSampleId :