

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091222AL\
 Data File : FE037494.D
 Signal(s) : FID1B.ch
 Acq On : 12 Sep 2022 20:27
 Operator : YP\AJ
 Sample : N4545-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 13 06:50:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.641	6624195	39.198 ug/ml
Spiked Amount 50.000		Recovery =	78.40%
12) S 1-chlorooctadecane (S...	13.065	4984417	38.729 ug/ml
Spiked Amount 50.000		Recovery =	77.46%
Target Compounds			
14) T n-Tetracosane (C24)	14.925	221651	1.474 ug/ml
16) T n-Octacosane (C28)	16.873	92802	0.670 ug/ml
17) T n-Tricontane (C30)	17.753	159691	1.174 ug/ml
18) T n-Dotriacontane (C32)	18.582	100467	0.752 ug/ml
19) T n-Tetratriacontane (C34)	19.365	76490	0.605 ug/ml
20) T n-Hexatriacontane (C36)	20.104	27030	0.210 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091222AL\
Data File : FE037494.D
Signal(s) : FID1B.ch
Acq On : 12 Sep 2022 20:27
Operator : YP\AJ
Sample : N4545-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 06:50:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

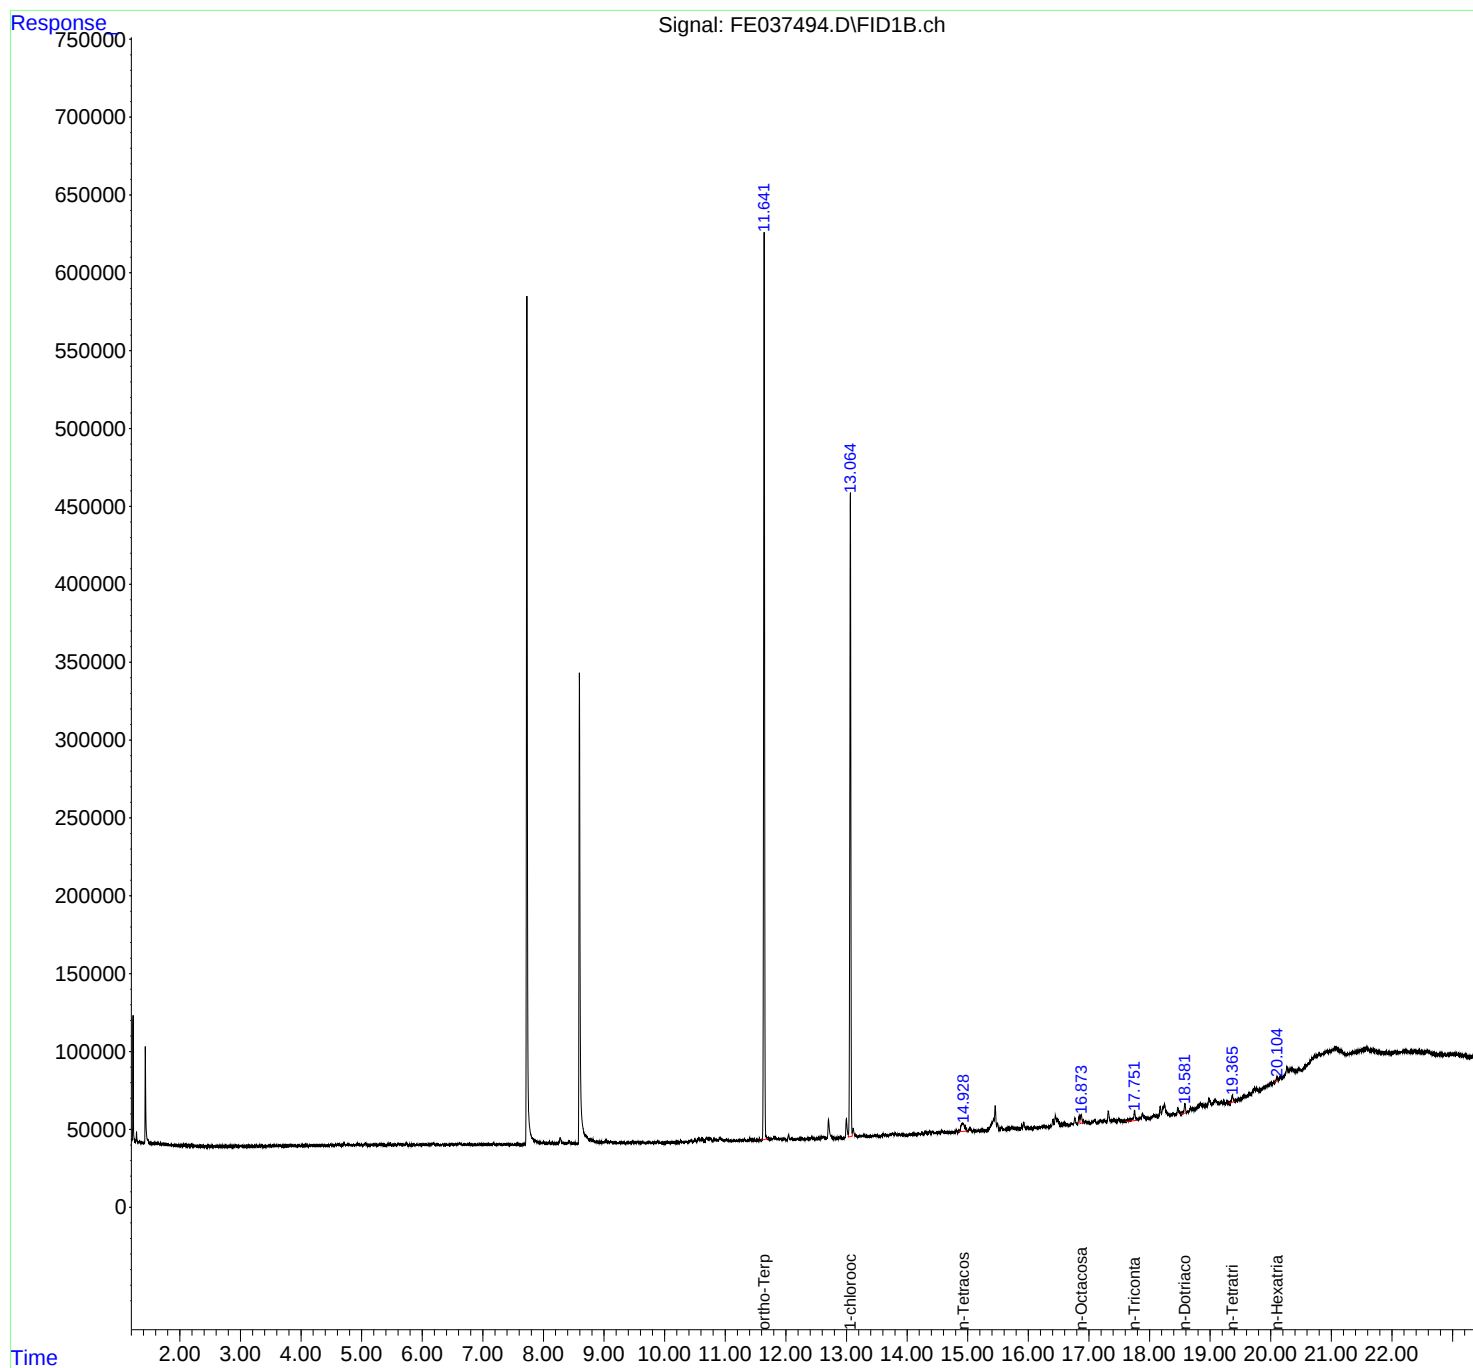


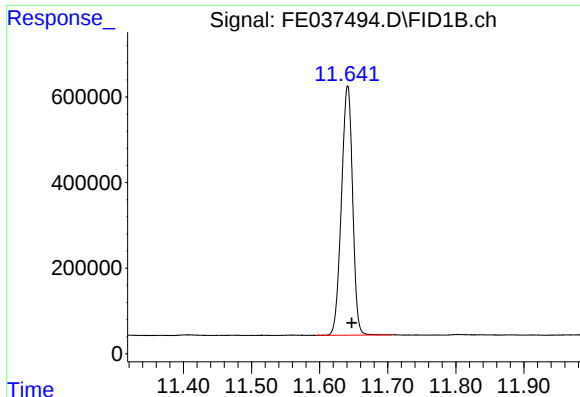

#9 ortho-Terphenyl (SURR)


R.T.: 11.641 min
Delta R.T.: -0.006 min
Response: 6624195
Conc: 39.20 ug/ml

Instrument :
FID_E
ClientSampleId :

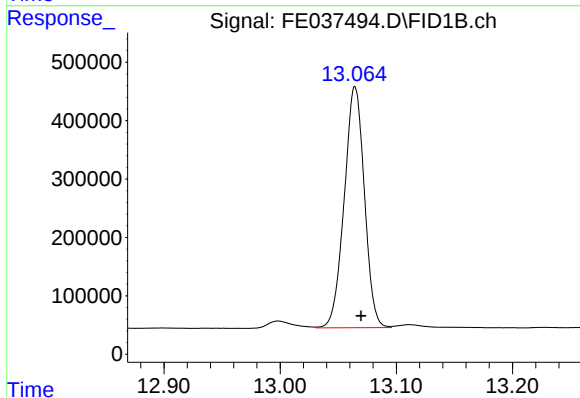


#12 1-chlorooctadecane (SURR)

R.T.: 13.065 min
Delta R.T.: -0.005 min
Response: 4984417
Conc: 38.73 ug/ml

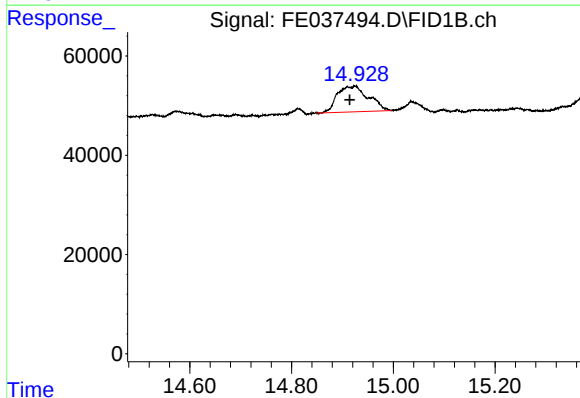


#14 n-Tetracosane (C24)

R.T.: 14.925 min
Delta R.T.: 0.010 min
Response: 221651
Conc: 1.47 ug/ml

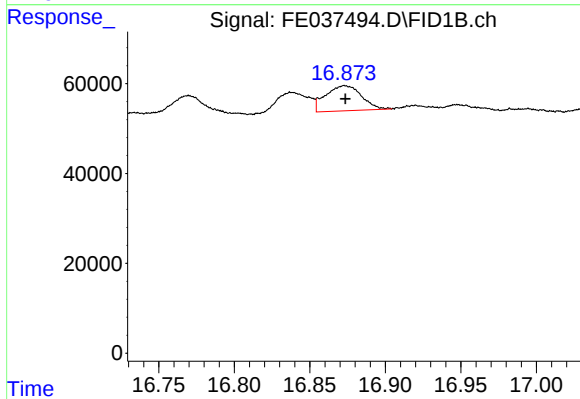

#16 n-Octacosane (C28)


R.T.: 16.873 min
Delta R.T.: 0.000 min
Response: 92802
Conc: 0.67 ug/ml

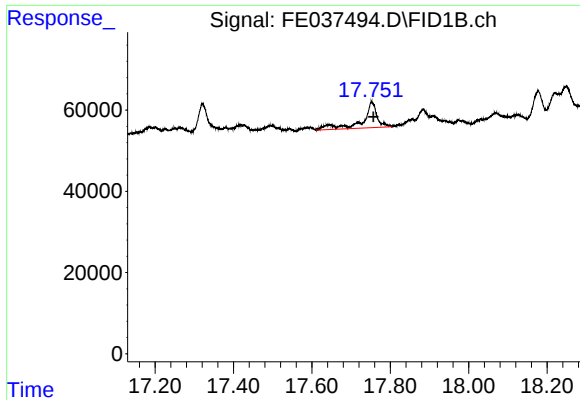

#17 n-Tricontane (C30)


R.T.: 17.753 min
Delta R.T.: -0.004 min
Response: 159691
Conc: 1.17 ug/ml

Instrument :
FID_E
ClientSampleId :

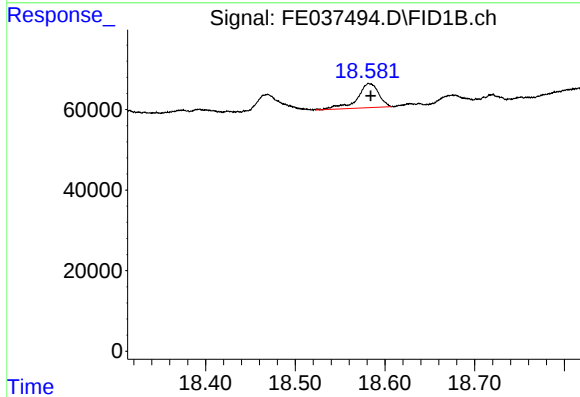


#18 n-Dotriacontane (C32)

R.T.: 18.582 min
Delta R.T.: -0.002 min
Response: 100467
Conc: 0.75 ug/ml

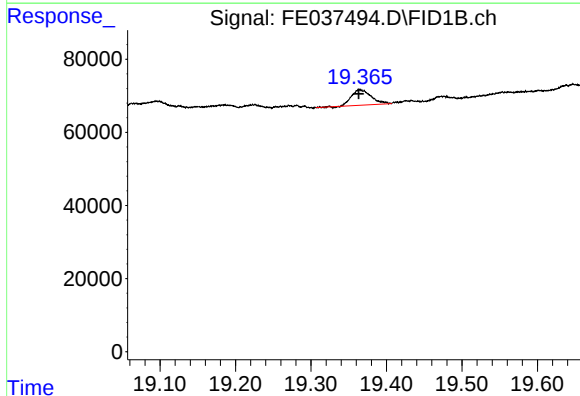

#19 n-Tetratriacontane (C34)

R.T.: 19.365 min
Delta R.T.: 0.001 min
Response: 76490
Conc: 0.60 ug/ml

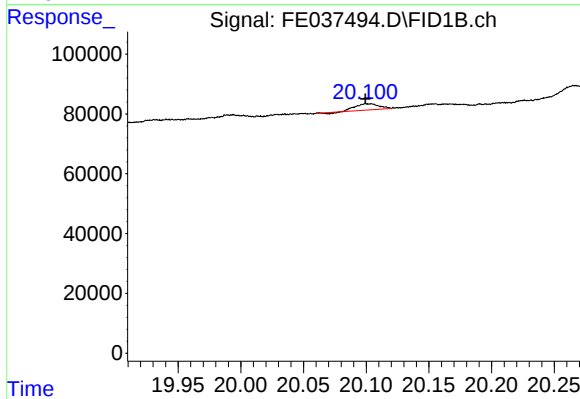

#20 n-Hexatriacontane (C36)

R.T.: 20.104 min
Delta R.T.: 0.004 min
Response: 27030
Conc: 0.21 ug/ml