

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091223AL\  
 Data File : FE044218.D  
 Signal(s) : FID1B.ch  
 Acq On : 12 Sep 2023 11:32  
 Operator : YP\AJ  
 Sample : 04363-06DL 10X  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 VNJ-222-E2DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 09/12/2023  
 Supervised By :Ankita Jodhani 09/13/2023

Integration File: autoint1.e  
 Quant Time: Sep 12 12:12:31 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 083023.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Aug 31 03:37:37 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units   |
|--------------------------------|--------|----------|--------------|
| -----                          |        |          |              |
| System Monitoring Compounds    |        |          |              |
| 9) S ortho-Terphenyl (SURR)    | 11.928 | 746606   | 3.941 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 7.88%      |
| 12) S 1-chlorooctadecane (S... | 13.368 | 570925   | 4.133 ug/ml  |
| Spiked Amount                  | 50.000 | Recovery | = 8.27%      |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091223AL\  
Data File : FE044218.D  
Signal(s) : FID1B.ch  
Acq On : 12 Sep 2023 11:32  
Operator : YP\AJ  
Sample : 04363-06DL 10X  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

**Instrument :**

FID\_E

**ClientSampleId :**

VNJ-222-E2DL

**Manual Integrations****APPROVED**

Reviewed By :Yogesh Patel 09/12/2023

Supervised By :Ankita Jodhani 09/13/2023

Integration File: autoint1.e

Quant Time: Sep 12 12:12:31 2023

Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 083023.

Quant Title : GC Extractables

QLast Update : Thu Aug 31 03:37:37 2023


Response via : Initial Calibration


Integrator: ChemStation

Volume Inj. : 1 ul

Signal Phase : Rxi-1ms

Signal Info : 20M x 0.18mm x 0.18um

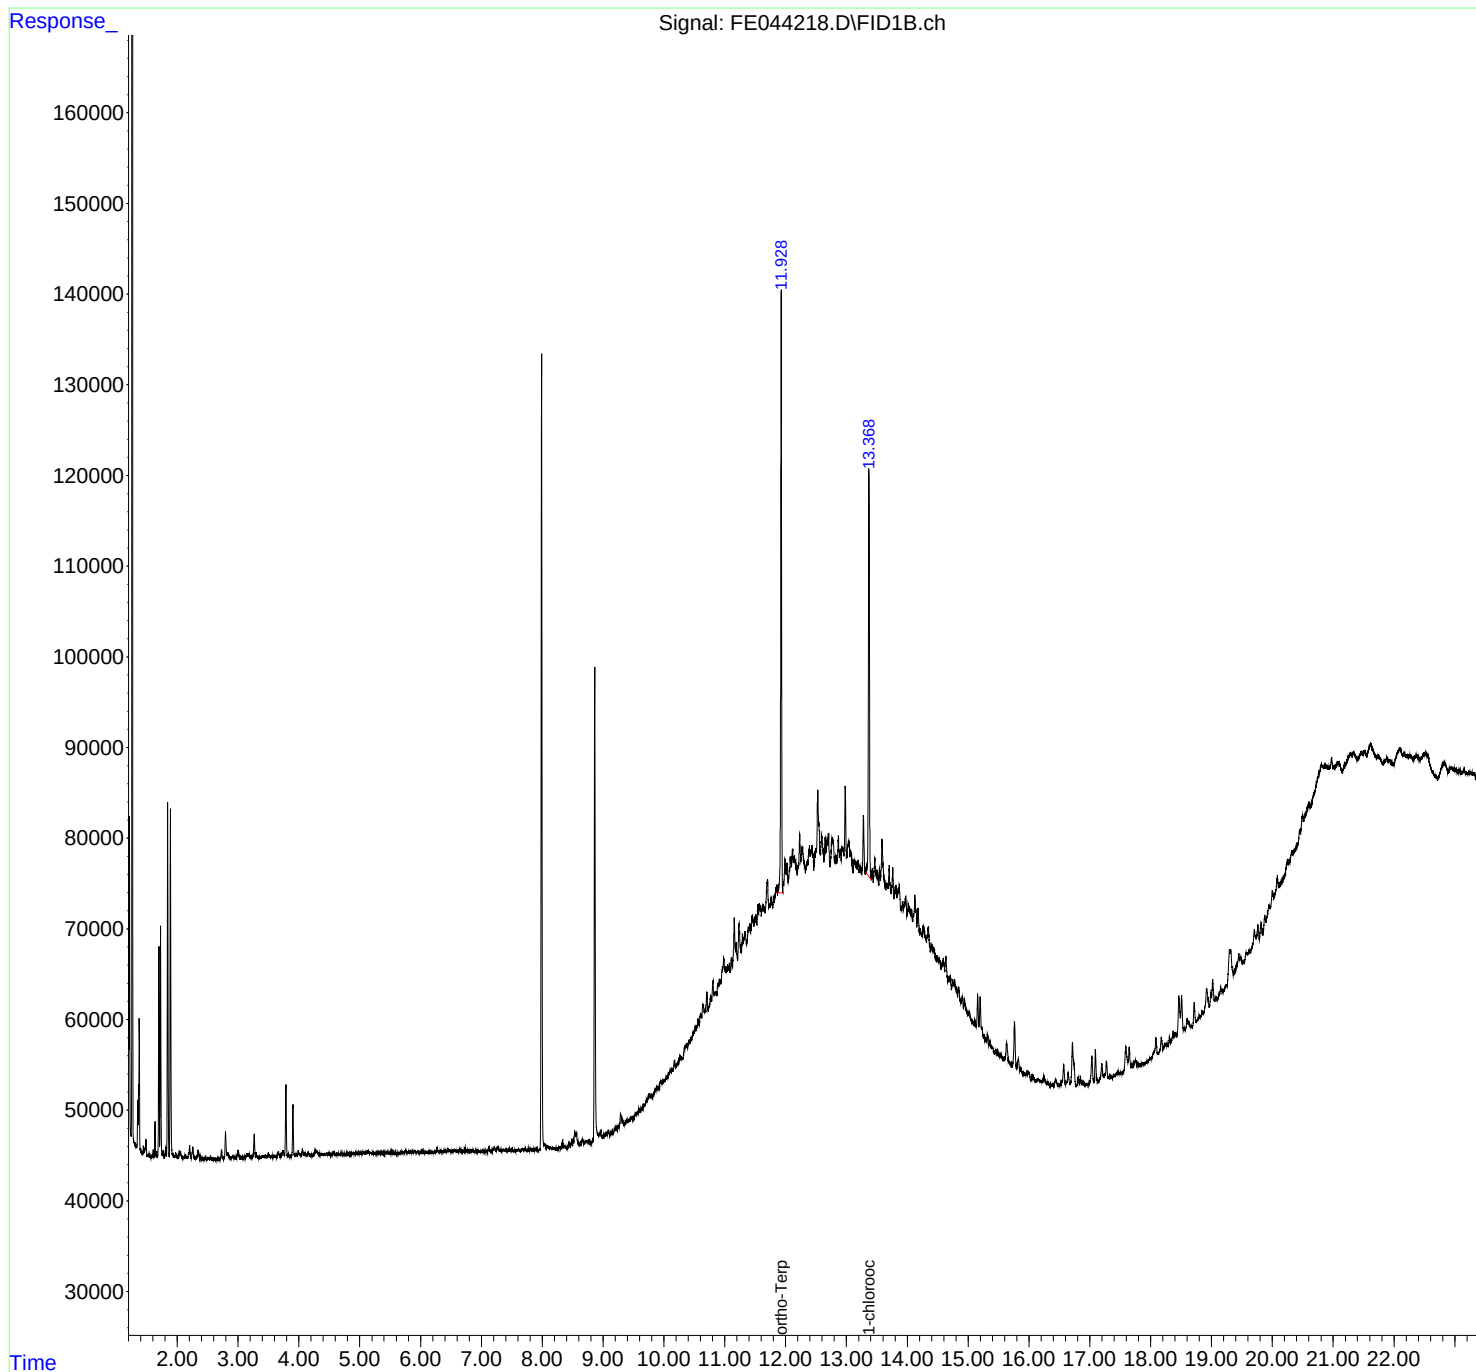

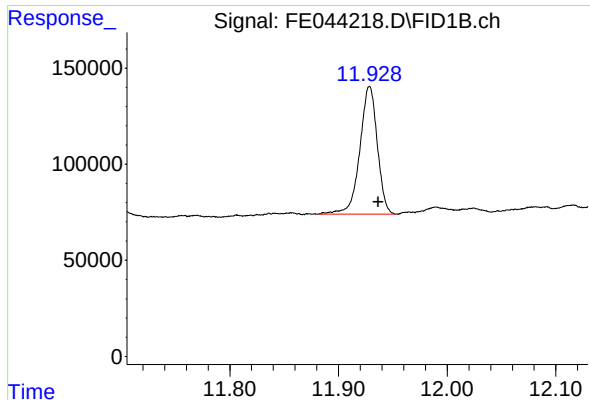


#9 ortho-Terphenyl (SURR)

R.T.: 11.928 min  
Delta R.T.: -0.008 min  
Response: 746606  
Conc: 3.94 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
VNJ-222-E2DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/12/2023  
Supervised By :Ankita Jodhani 09/13/2023

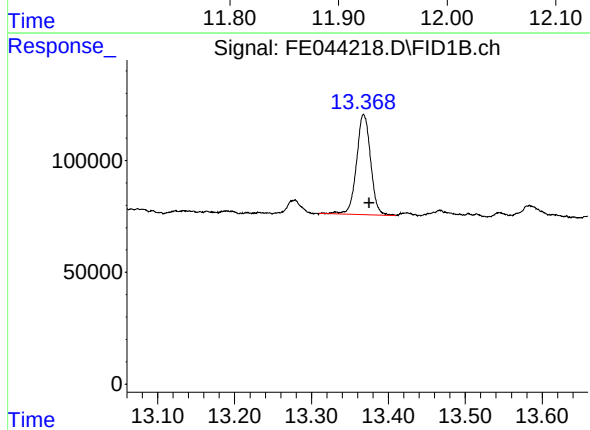

#12 1-chlorooctadecane (SURR)

R.T.: 13.368 min  
Delta R.T.: -0.007 min  
Response: 570925  
Conc: 4.13 ug/ml