

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091225AL\
Data File : FE055800.D
Signal(s) : FID1B.ch
Acq On : 12 Sep 2025 14:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 02:30:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082925.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 08:12:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.231	130108	0.880 ug/ml
18) T	n-Dotriacontane (C32)	19.065	162625	1.108 ug/ml
19) T	n-Tetratriacontane (C34)	19.850	109078	0.772 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091225AL\
Data File : FE055800.D
Signal(s) : FID1B.ch
Acq On : 12 Sep 2025 14:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 02:30:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082925.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 08:12:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

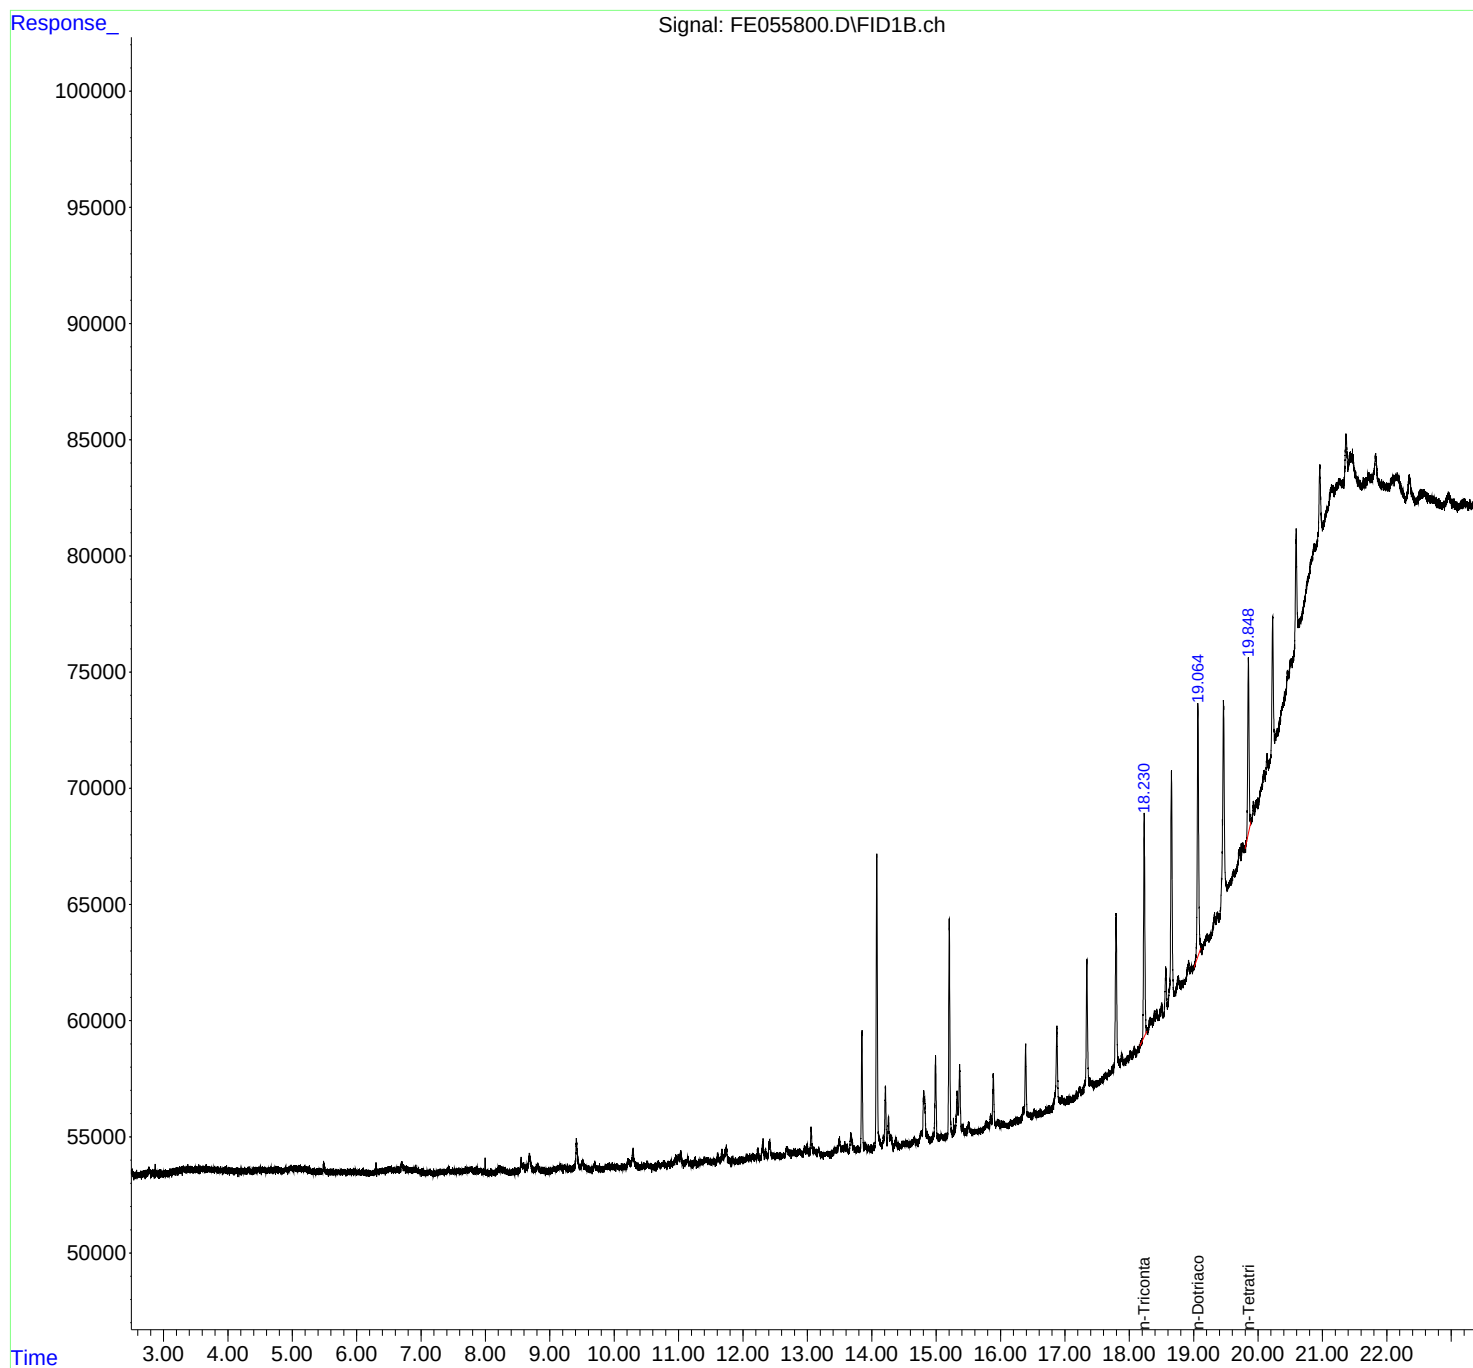


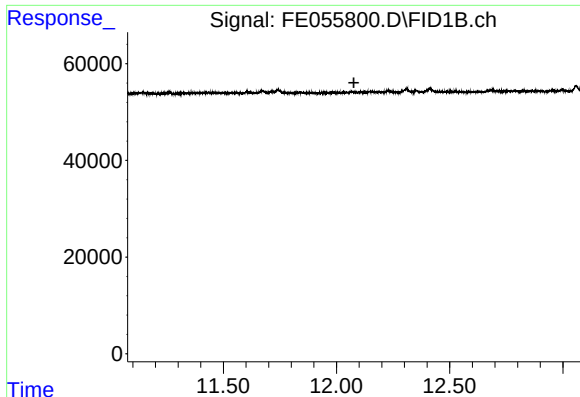

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 12.077 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

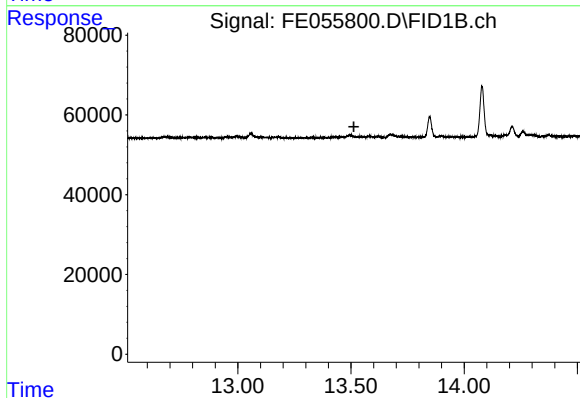


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.513 min
Response: 0
Conc: N.D.

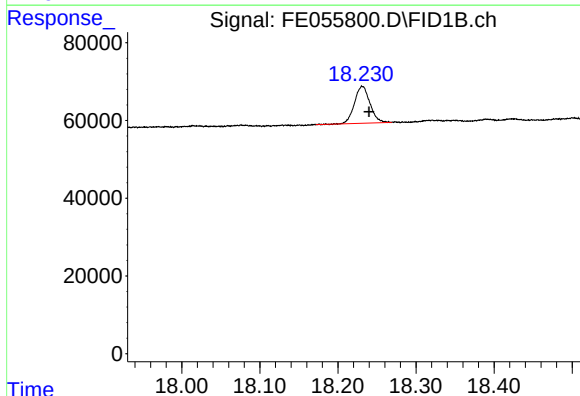


#17 n-Tricontane (C30)

R.T.: 18.231 min
Delta R.T.: -0.008 min
Response: 130108
Conc: 0.88 ug/ml

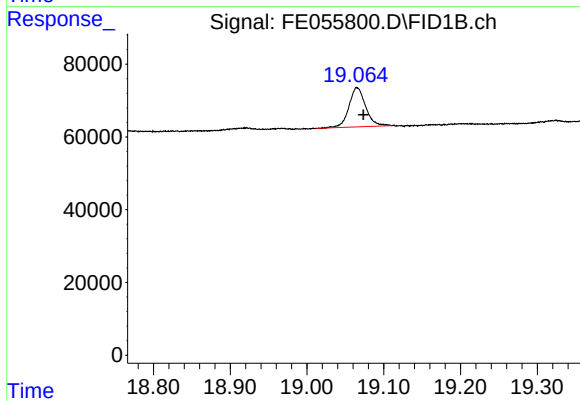

#18 n-Dotriacontane (C32)

R.T.: 19.065 min
Delta R.T.: -0.008 min
Response: 162625
Conc: 1.11 ug/ml

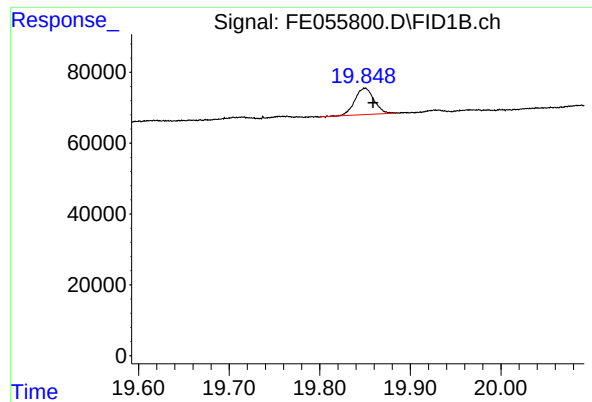

#19 n-Tetratriacontane (C34)

R.T.: 19.850 min
Delta R.T.: -0.009 min
Response: 109078
Conc: 0.77 ug/ml

Instrument :

FID_E

ClientSampleId :