

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091319\
Data File : FE030481.D
Signal(s) : FID1B.CH
Acq On : 13 Sep 2019 17:30
Operator : DD\AJ
Sample : K4857-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SLUDGE-COMP

Integration File: autoint1.e
Quant Time: Sep 14 05:02:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.541	3467878	17.426 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091319\
Data File : FE030481.D
Signal(s) : FID1B.CH
Acq On : 13 Sep 2019 17:30
Operator : DD\AJ
Sample : K4857-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SLUDGE-COMP

Integration File: autoint1.e
Quant Time: Sep 14 05:02:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rx1-1ms
Signal Info : 20m x 0.18mm x 0.18um

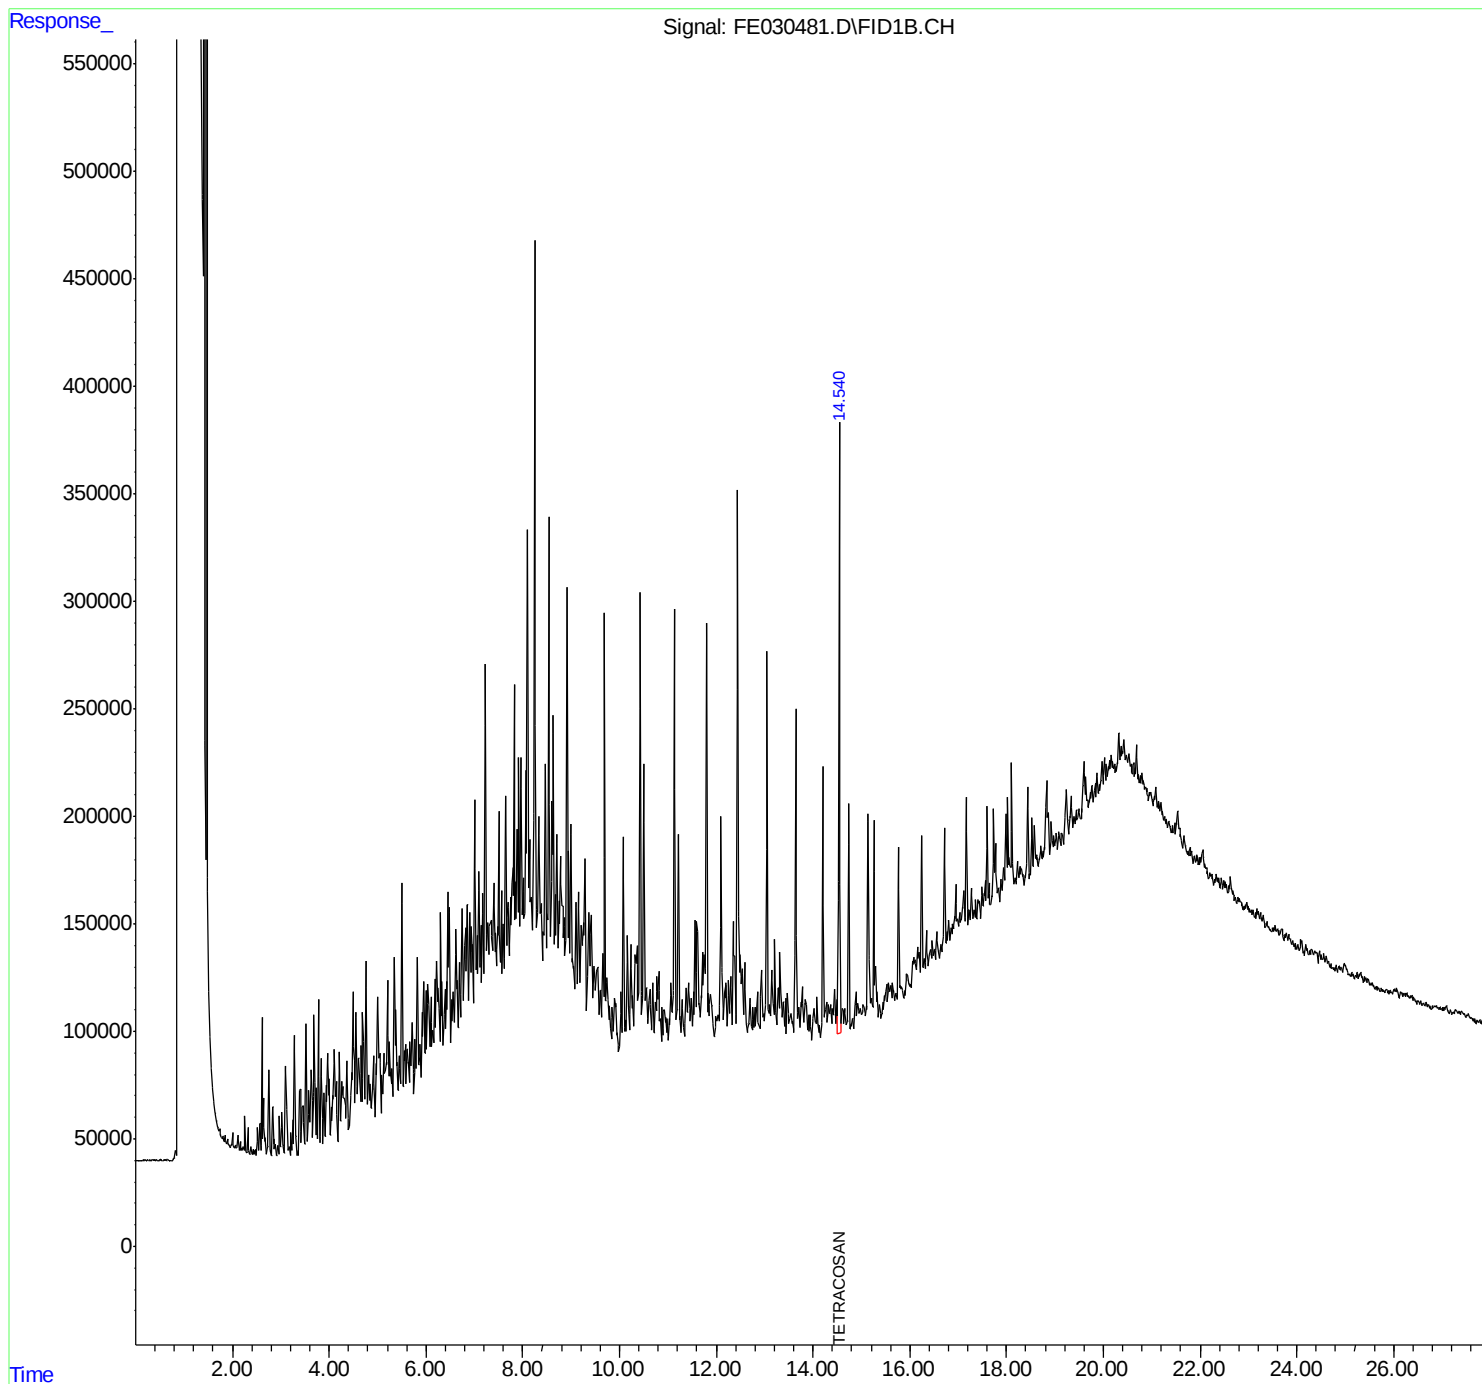

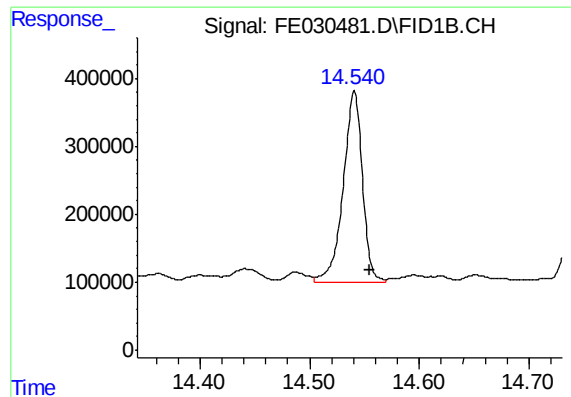

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.541 min
Delta R.T.: -0.014 min
Response: 3467878
Conc: 17.43 ug/ml

Instrument :
FID_E
ClientSampleId :
SLUDGE-COMP