

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091322AL\
 Data File : FE037508.D
 Signal(s) : FID1B.ch
 Acq On : 13 Sep 2022 09:55
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 14 08:08:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.608	80293	0.507 ug/ml
11) T	n-Heneicosane (C21)	13.221	84648	0.537 ug/ml
13) T	n-Docosane (C22)	13.805	61812	0.397 ug/ml
14) T	n-Tetracosane (C24)	14.901	83703	0.557 ug/ml
17) T	n-Tricontane (C30)	17.749	60323	0.443 ug/ml
18) T	n-Dotriacontane (C32)	18.585	133662	1.001 ug/ml
19) T	n-Tetratriacontane (C34)	19.413	49909	0.394 ug/ml
20) T	n-Hexatriacontane (C36)	20.137	148002	1.151 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091322AL\
Data File : FE037508.D
Signal(s) : FID1B.ch
Acq On : 13 Sep 2022 09:55
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 14 08:08:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

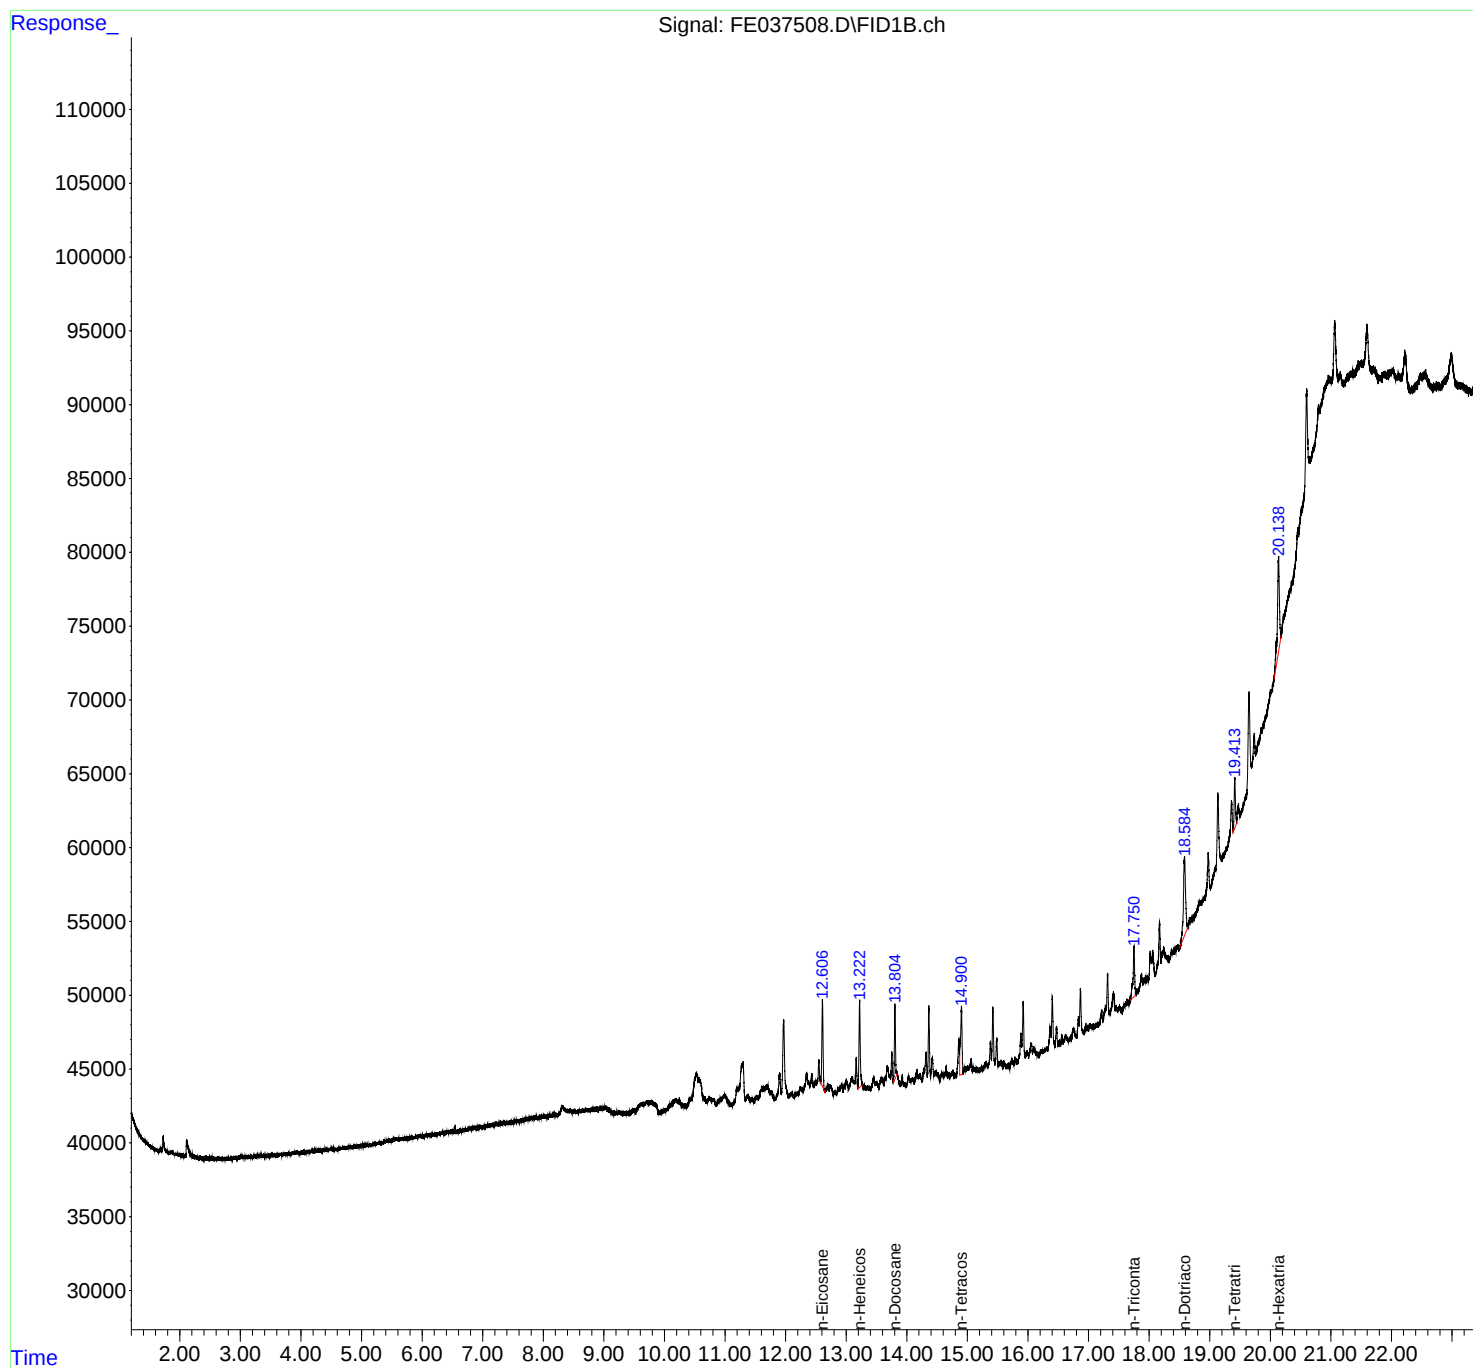


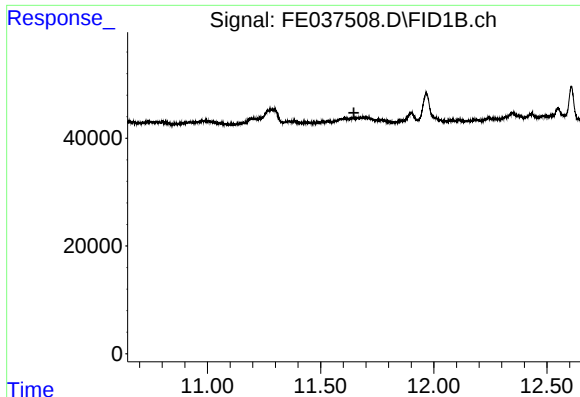

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.647 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

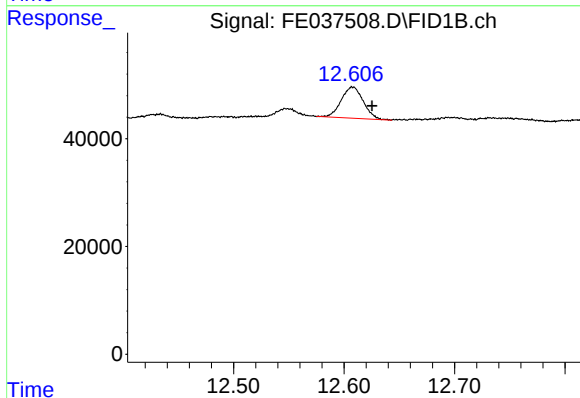


#10 n-Eicosane (C20)

R.T.: 12.608 min
Delta R.T.: -0.018 min
Response: 80293
Conc: 0.51 ug/ml

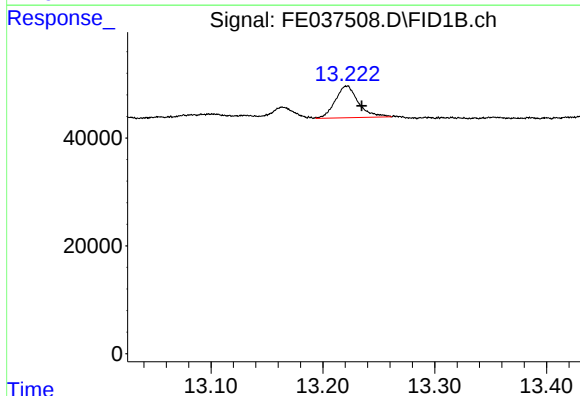


#11 n-Heneicosane (C21)

R.T.: 13.221 min
Delta R.T.: -0.013 min
Response: 84648
Conc: 0.54 ug/ml

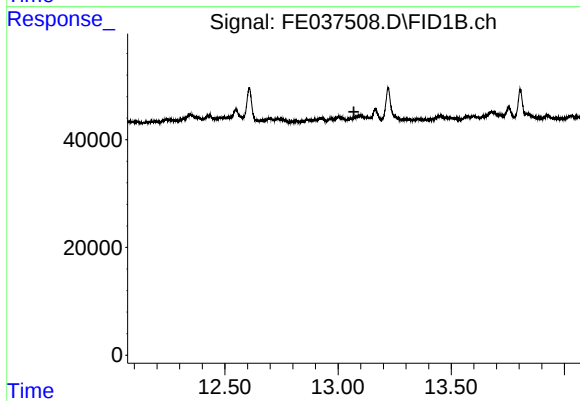

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.070 min
Response: 0
Conc: N.D.

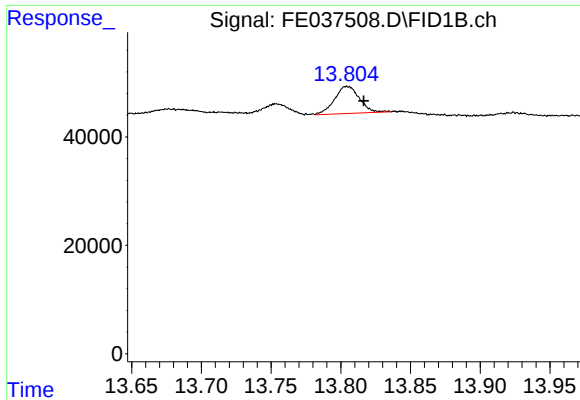

#13 n-Docosane (C22)


R.T.: 13.805 min
Delta R.T.: -0.012 min
Response: 61812
Conc: 0.40 ug/ml

Instrument :
FID_E
ClientSampleId :

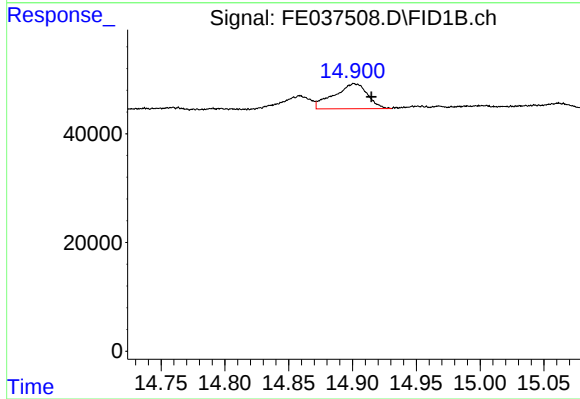


#14 n-Tetracosane (C24)

R.T.: 14.901 min
Delta R.T.: -0.013 min
Response: 83703
Conc: 0.56 ug/ml

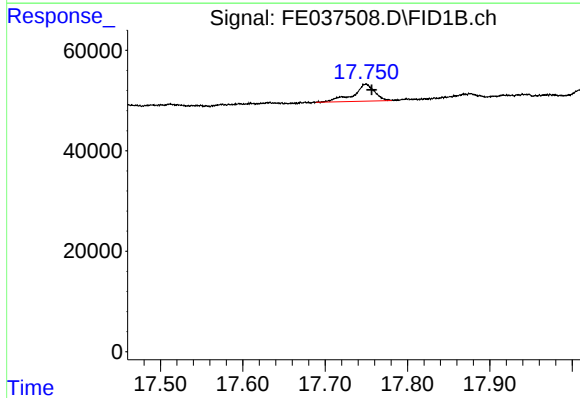


#17 n-Tricontane (C30)

R.T.: 17.749 min
Delta R.T.: -0.007 min
Response: 60323
Conc: 0.44 ug/ml

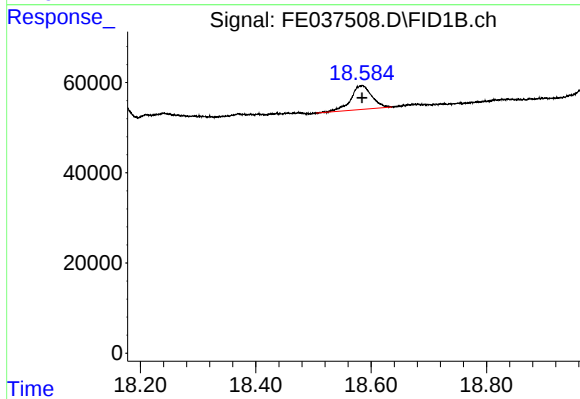

#18 n-Dotriacontane (C32)


R.T.: 18.585 min
Delta R.T.: 0.000 min
Response: 133662
Conc: 1.00 ug/ml

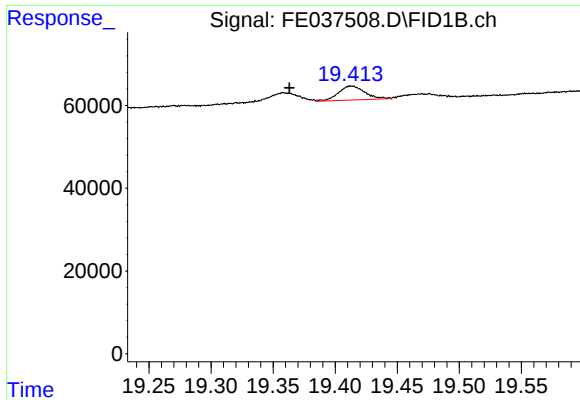

#19 n-Tetratriacontane (C34)

R.T.: 19.413 min
Delta R.T.: 0.050 min
Response: 49909
Conc: 0.39 ug/ml

Instrument :
FID_E
ClientSampleId :

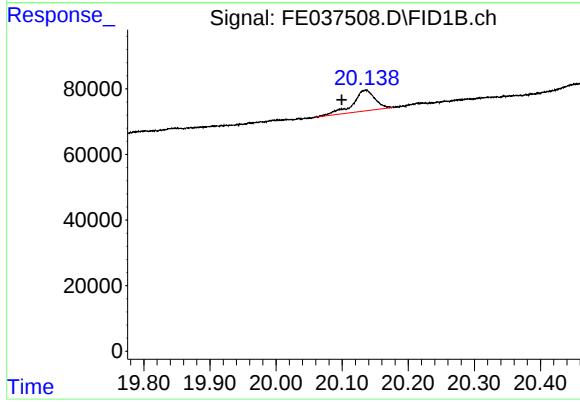

#20 n-Hexatriacontane (C36)

R.T.: 20.137 min
Delta R.T.: 0.037 min
Response: 148002
Conc: 1.15 ug/ml