

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091322AL\
 Data File : FE037538.D
 Signal(s) : FID1B.ch
 Acq On : 14 Sep 2022 01:56
 Operator : YP\AJ
 Sample : N4578-18
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 14 08:14:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.631	4981760	29.479 ug/ml
Spiked Amount 50.000		Recovery =	58.96%
12) S 1-chlorooctadecane (S...	13.055	4035364	31.355 ug/ml
Spiked Amount 50.000		Recovery =	62.71%
Target Compounds			
14) T n-Tetracosane (C24)	14.898	70509	0.469 ug/ml
15) T n-Hexacosane (C26)	15.914	78281	0.541 ug/ml
16) T n-Octacosane (C28)	16.860	54840	0.396 ug/ml
17) T n-Tricontane (C30)	17.741	63705	0.468 ug/ml
18) T n-Dotriacontane (C32)	18.568	53878	0.403 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091322AL\
Data File : FE037538.D
Signal(s) : FID1B.ch
Acq On : 14 Sep 2022 01:56
Operator : YP\AJ
Sample : N4578-18
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 14 08:14:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

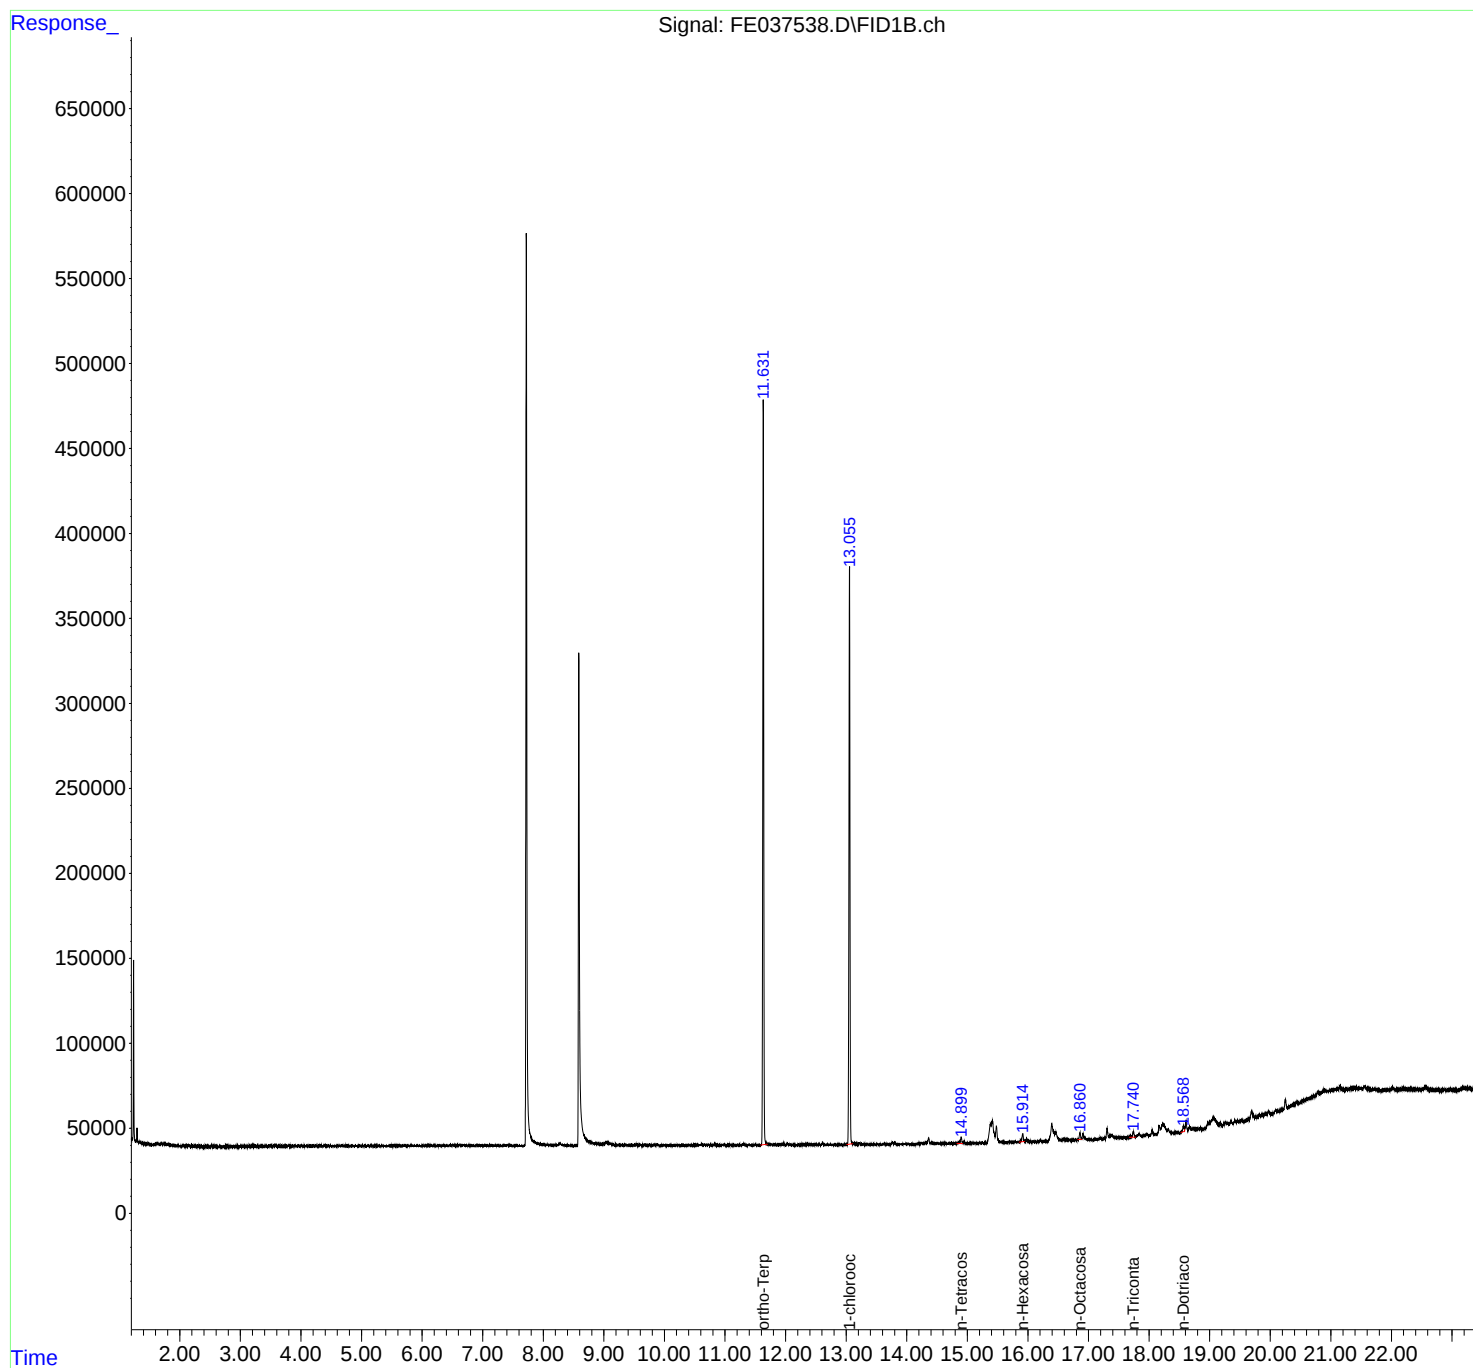


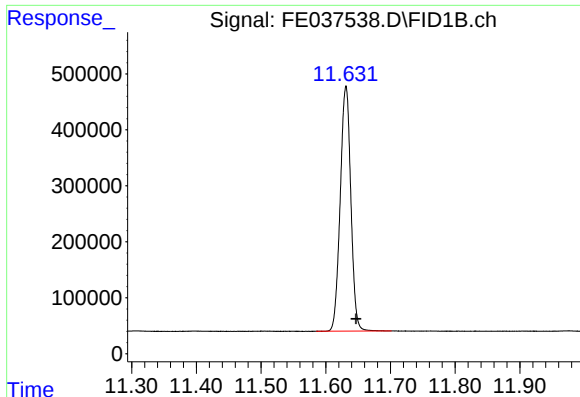

#9 ortho-Terphenyl (SURR)


R.T.: 11.631 min
Delta R.T.: -0.016 min
Response: 4981760
Conc: 29.48 ug/ml

Instrument :
FID_E
ClientSampleId :

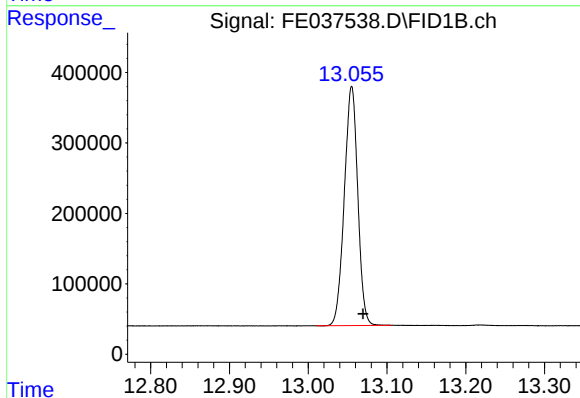


#12 1-chlorooctadecane (SURR)

R.T.: 13.055 min
Delta R.T.: -0.015 min
Response: 4035364
Conc: 31.36 ug/ml

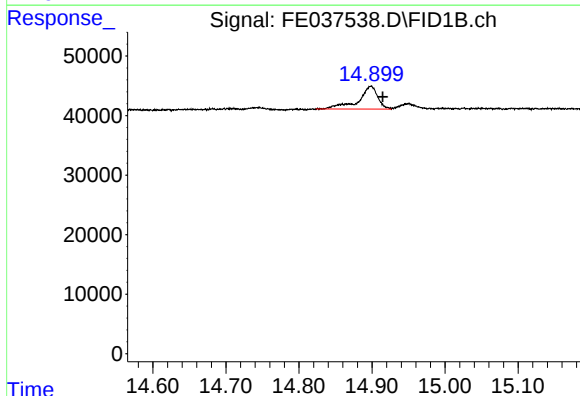


#14 n-Tetracosane (C24)

R.T.: 14.898 min
Delta R.T.: -0.016 min
Response: 70509
Conc: 0.47 ug/ml

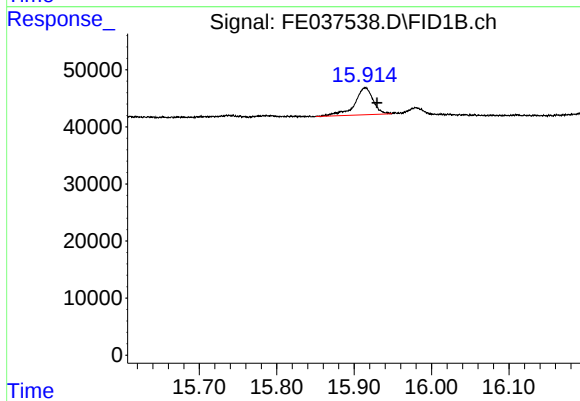

#15 n-Hexacosane (C26)


R.T.: 15.914 min
Delta R.T.: -0.015 min
Response: 78281
Conc: 0.54 ug/ml

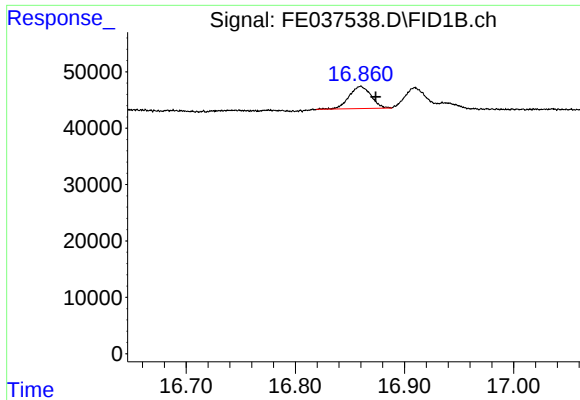

#16 n-Octacosane (C28)


R.T.: 16.860 min
Delta R.T.: -0.014 min
Response: 54840
Conc: 0.40 ug/ml

Instrument :
FID_E
ClientSampleId :

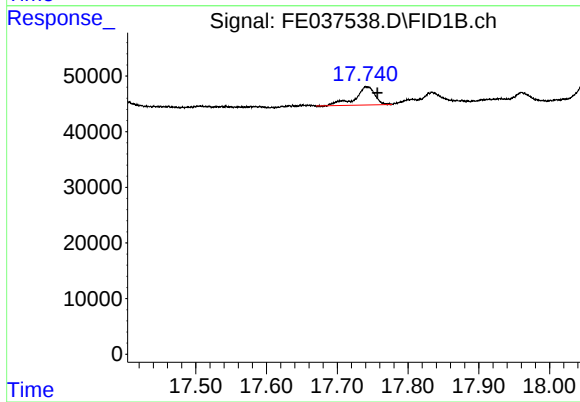

#17 n-Tricontane (C30)

R.T.: 17.741 min
Delta R.T.: -0.016 min
Response: 63705
Conc: 0.47 ug/ml

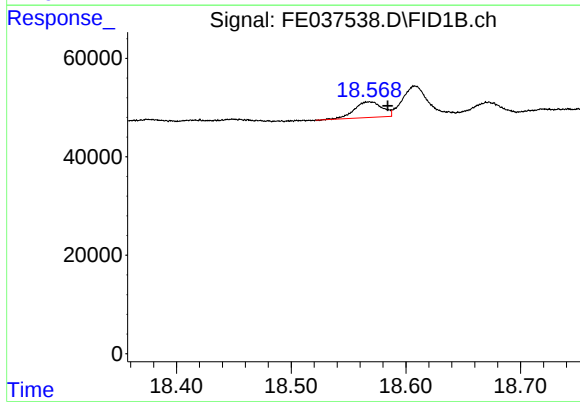

#18 n-Dotriacontane (C32)

R.T.: 18.568 min
Delta R.T.: -0.016 min
Response: 53878
Conc: 0.40 ug/ml