

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091323AL\
 Data File : FE044243.D
 Signal(s) : FID1B.ch
 Acq On : 13 Sep 2023 10:13
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 13 11:11:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 083023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 31 03:37:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T n-Tetratriacontane (C34)	19.760	51004	0.364 ug/ml
20) T n-Hexatriacontane (C36)	20.485	253815	1.851 ug/ml
22) T n-Tetracontane (C40)	22.119	1387767	10.037 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091323AL\
Data File : FE044243.D
Signal(s) : FID1B.ch
Acq On : 13 Sep 2023 10:13
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 11:11:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 083023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 31 03:37:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

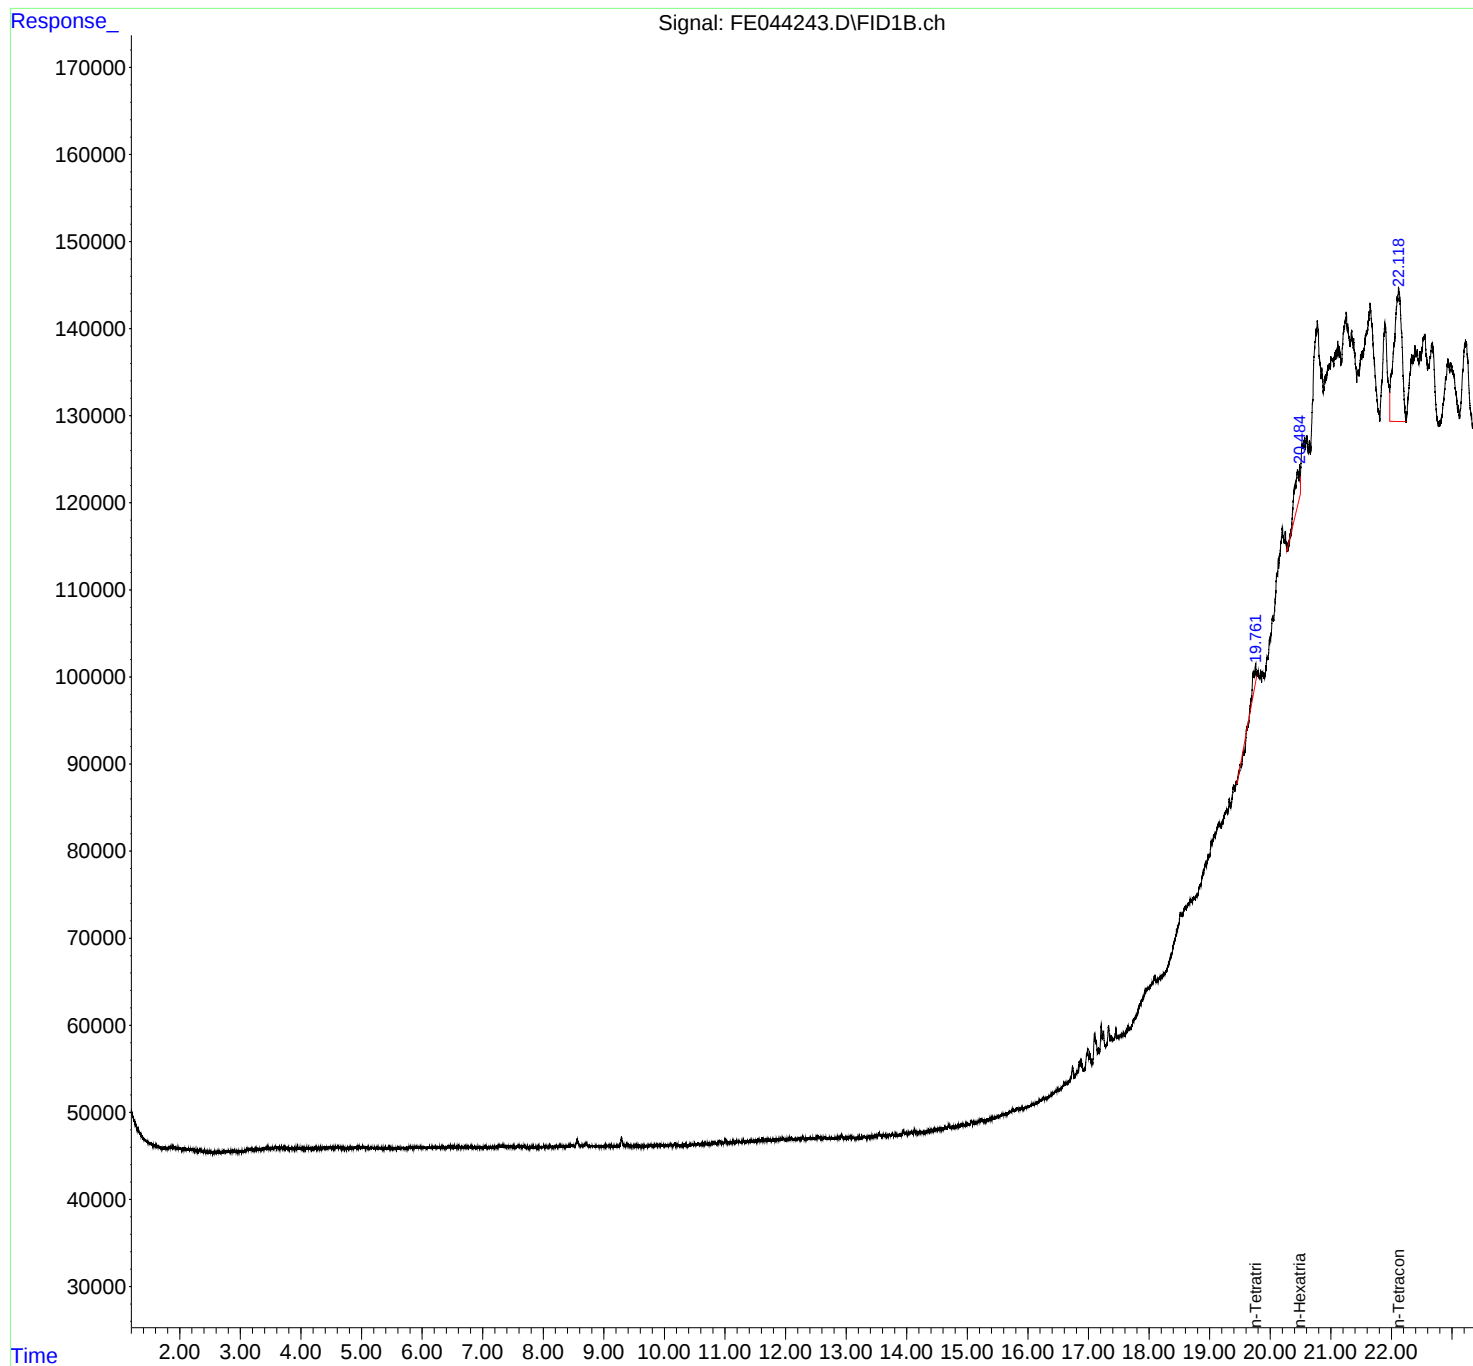


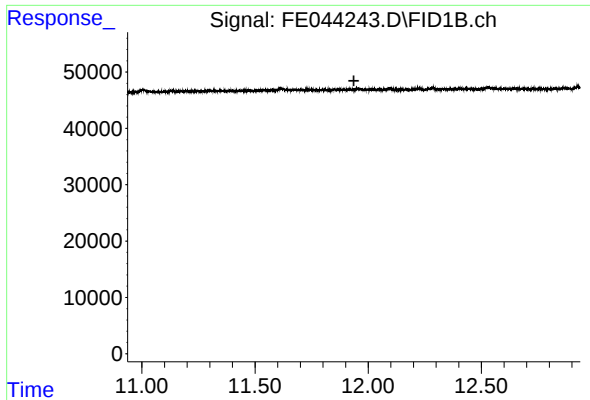

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.937 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

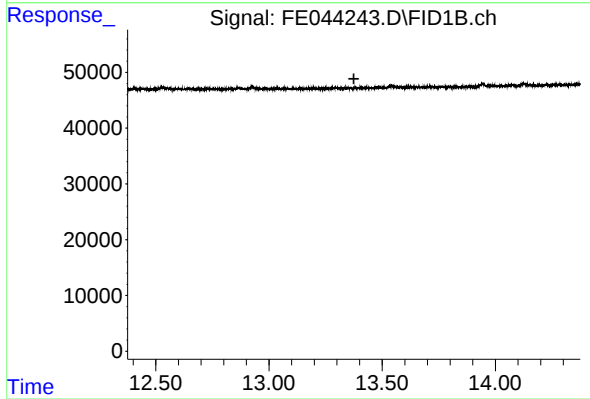


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.375 min
Response: 0
Conc: N.D.

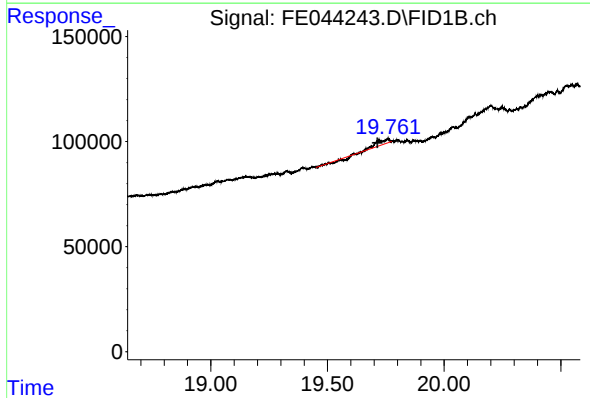


#19 n-Tetratriacontane (C34)

R.T.: 19.760 min
Delta R.T.: 0.045 min
Response: 51004
Conc: 0.36 ug/ml

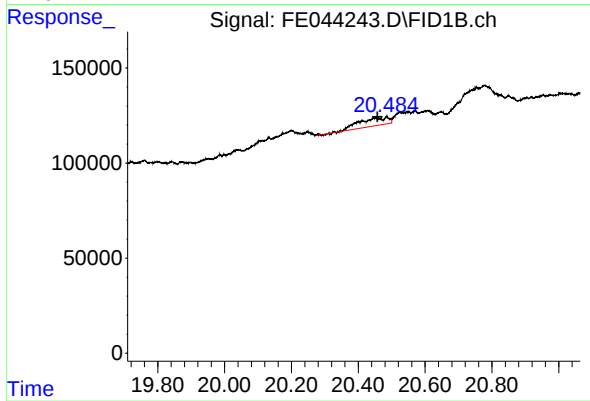

#20 n-Hexatriacontane (C36)

R.T.: 20.485 min
Delta R.T.: 0.028 min
Response: 253815
Conc: 1.85 ug/ml

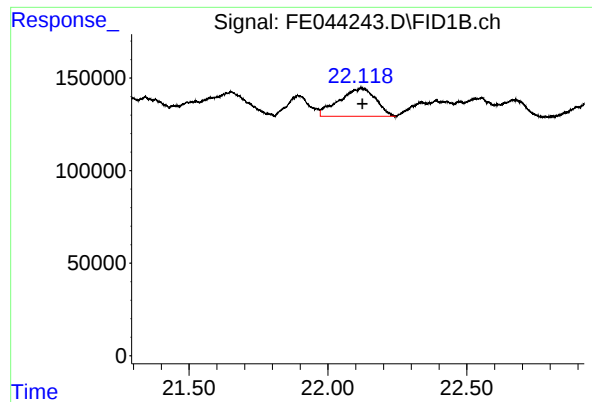

#22 n-Tetracontane (C40)

R.T.: 22.119 min
Delta R.T.: -0.005 min
Response: 1387767
Conc: 10.04 ug/ml

Instrument :

FID_E

ClientSampleId :