

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091323AL\  
 Data File : FE044249.D  
 Signal(s) : FID1B.ch  
 Acq On : 13 Sep 2023 17:06  
 Operator : YP\AJ  
 Sample : 04396-01  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 CHRT-24313

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 09/14/2023  
 Supervised By :Ankita Jodhani 09/14/2023

Integration File: autoint1.e  
 Quant Time: Sep 13 17:58:47 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 083023.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Aug 31 03:37:37 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 9) S ortho-Terphenyl (SURR)    | 11.968 | 7243890    | 38.236 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 76.47%        |
| 12) S 1-chlorooctadecane (S... | 13.411 | 5759341    | 41.690 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 83.38%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091323AL\  
Data File : FE044249.D  
Signal(s) : FID1B.ch  
Acq On : 13 Sep 2023 17:06  
Operator : YP\AJ  
Sample : 04396-01  
Misc :  
ALS Vial : 16 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
CHRT-24313


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/14/2023  
Supervised By :Ankita Jodhani 09/14/2023

Integration File: autoint1.e  
Quant Time: Sep 13 17:58:47 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 083023.  
Quant Title : GC Extractables  
QLast Update : Thu Aug 31 03:37:37 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

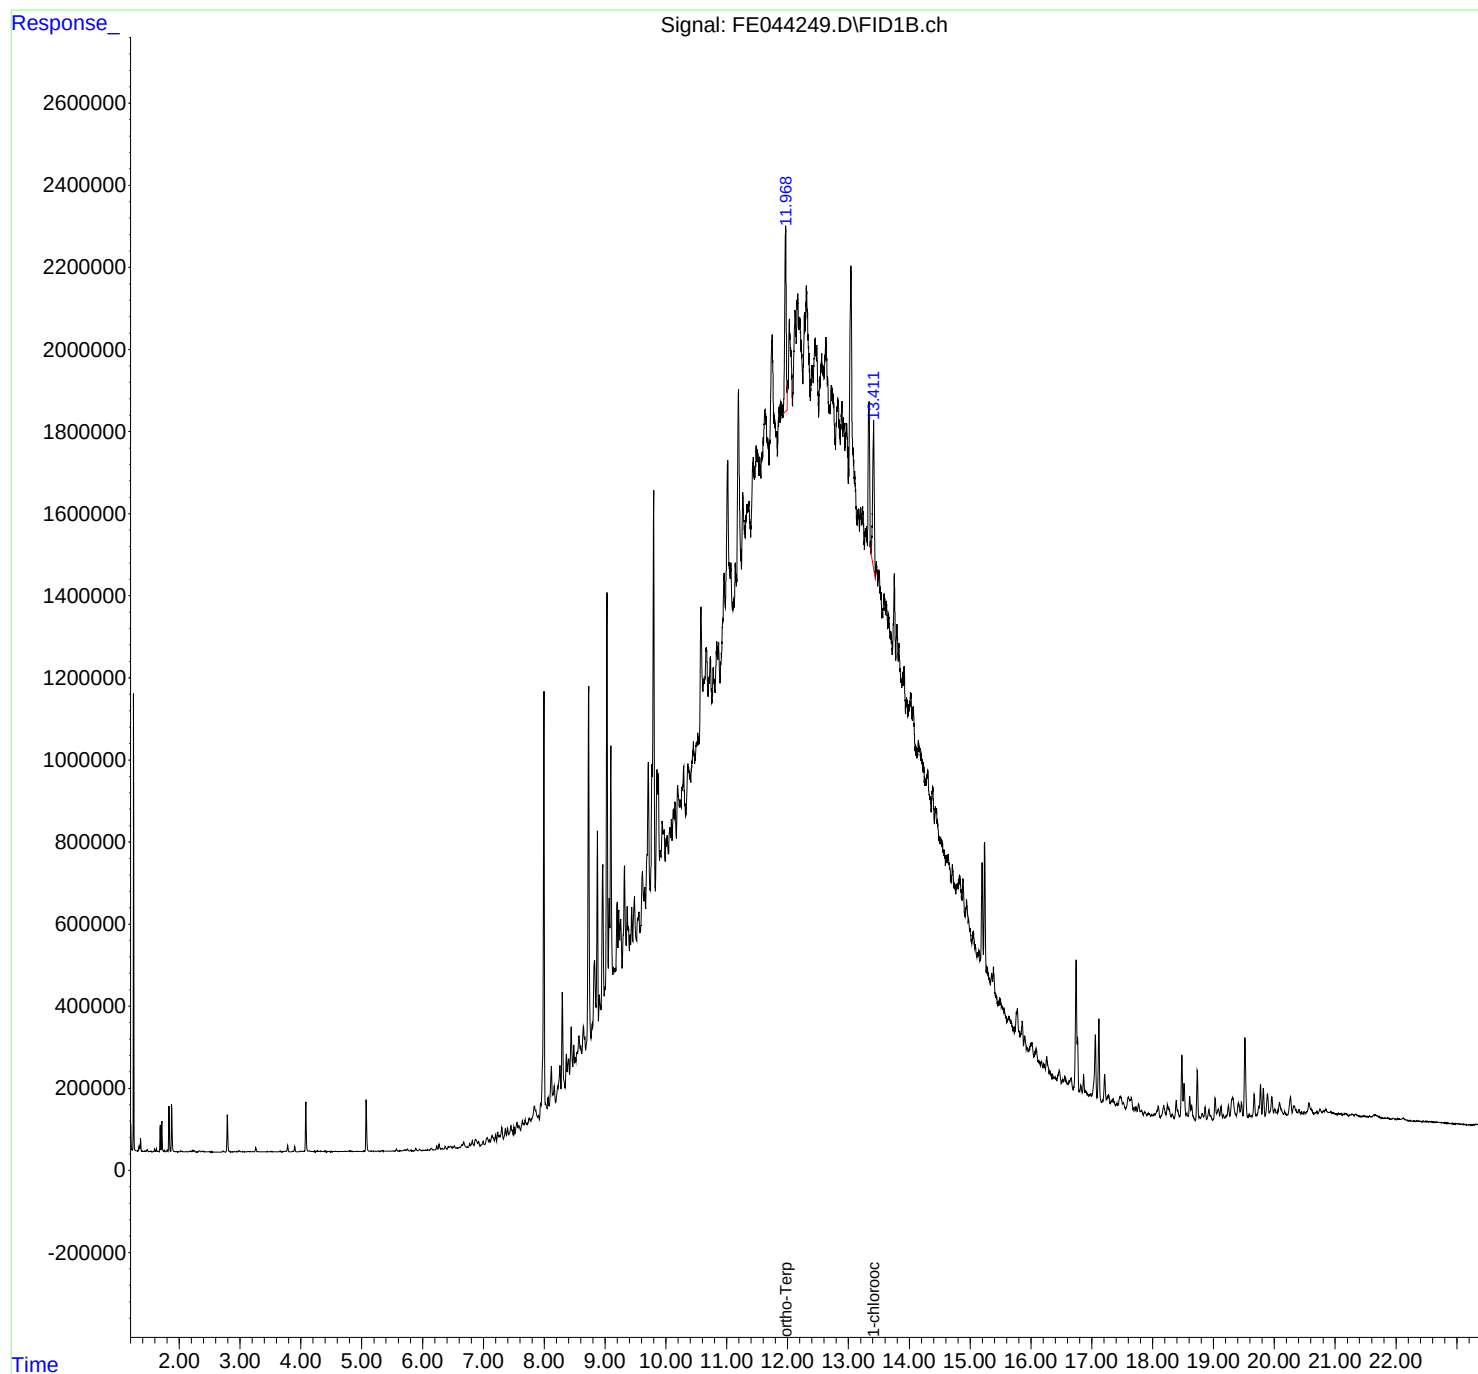

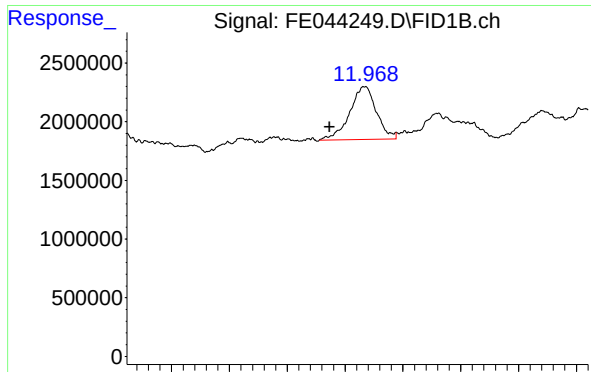


#9 ortho-Terphenyl (SURR)

R.T.: 11.968 min  
Delta R.T.: 0.031 min  
Response: 7243890  
Conc: 38.24 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
CHRT-24313

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/14/2023  
Supervised By :Ankita Jodhani 09/14/2023

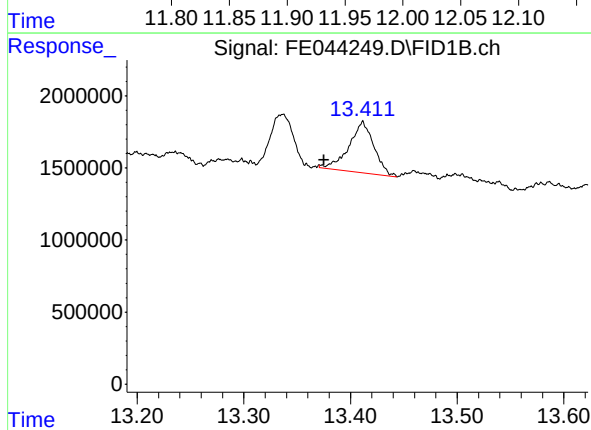

#12 1-chlorooctadecane (SURR)

R.T.: 13.411 min  
Delta R.T.: 0.036 min  
Response: 5759341  
Conc: 41.69 ug/ml m