

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091422AL\
 Data File : FE037541.D
 Signal(s) : FID1B.ch
 Acq On : 14 Sep 2022 08:52
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 15 04:46:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.598	118571	0.749 ug/ml
11) T	n-Heneicosane (C21)	13.212	128677	0.816 ug/ml
13) T	n-Docosane (C22)	13.797	105186	0.676 ug/ml
14) T	n-Tetracosane (C24)	14.894	122655	0.816 ug/ml
15) T	n-Hexacosane (C26)	15.913	78880	0.545 ug/ml
16) T	n-Octacosane (C28)	16.858	58194	0.420 ug/ml
17) T	n-Tricontane (C30)	17.741	63183	0.464 ug/ml
18) T	n-Dotriacontane (C32)	18.565	127398	0.954 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091422AL\
Data File : FE037541.D
Signal(s) : FID1B.ch
Acq On : 14 Sep 2022 08:52
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 15 04:46:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

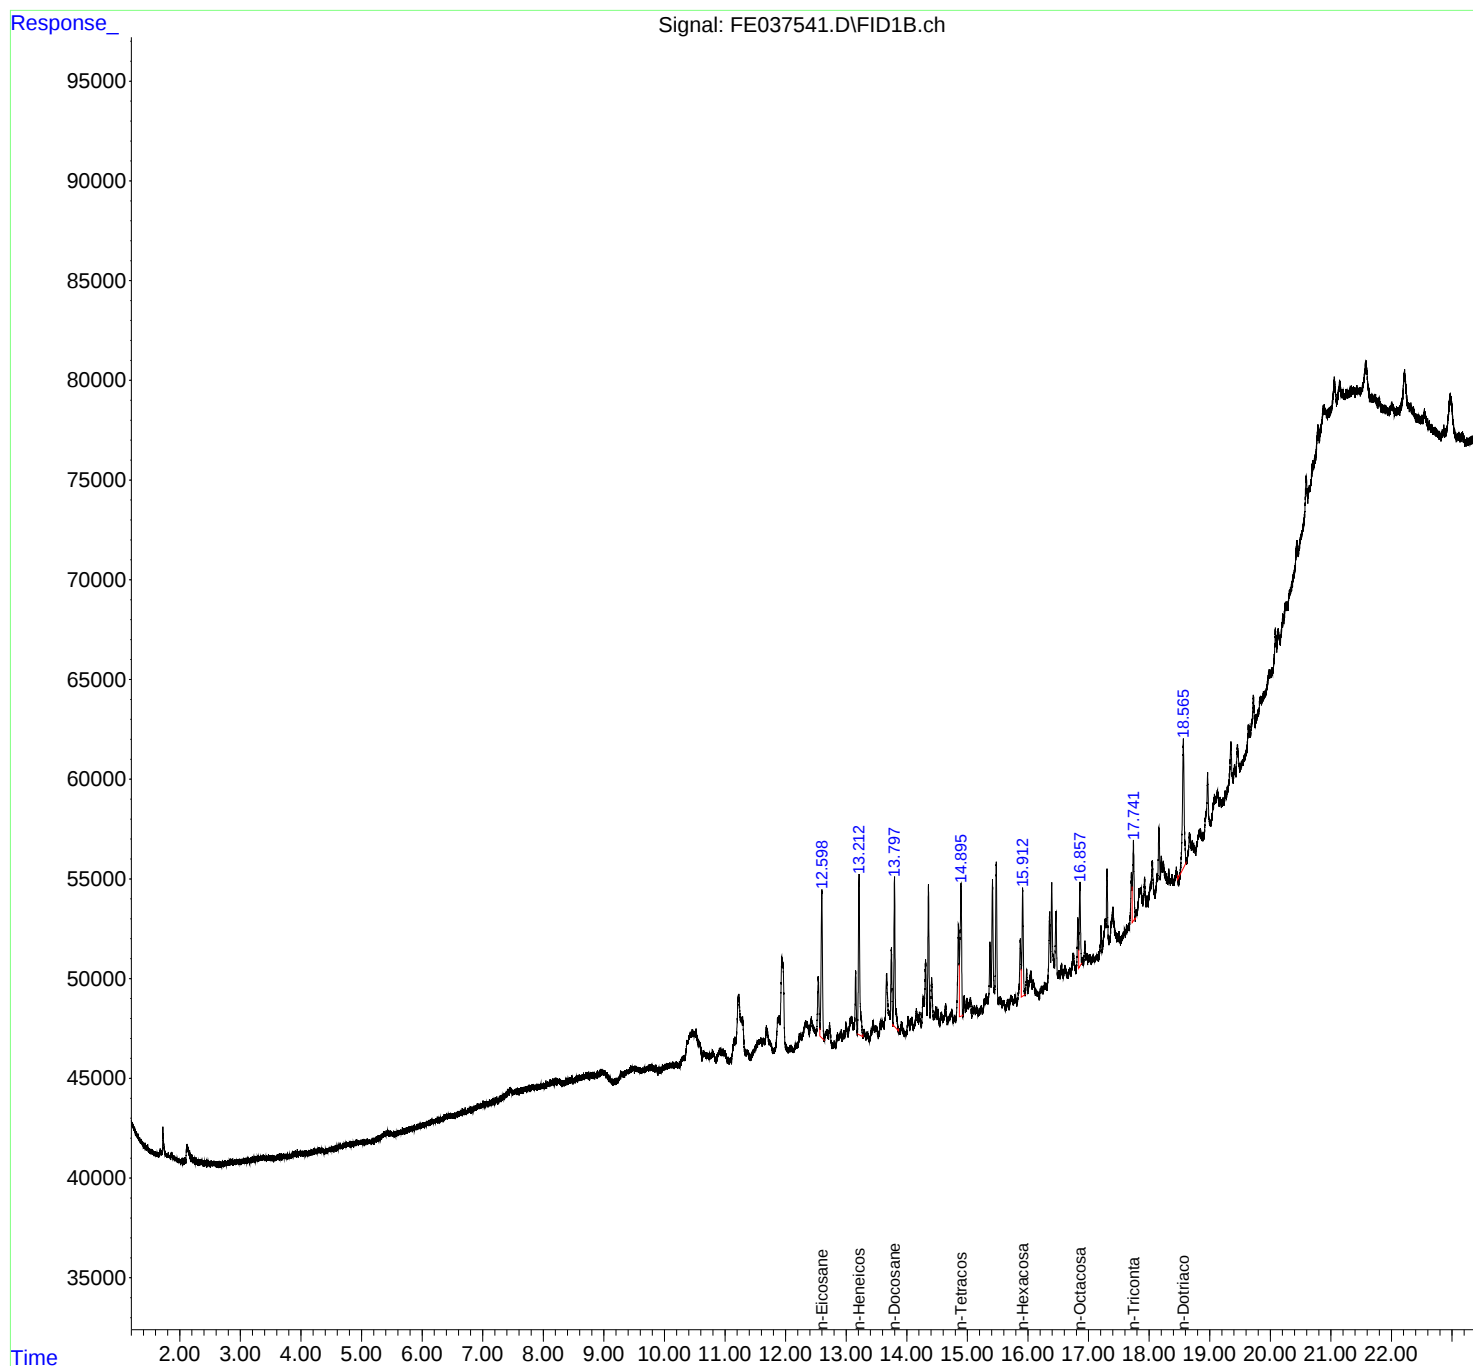


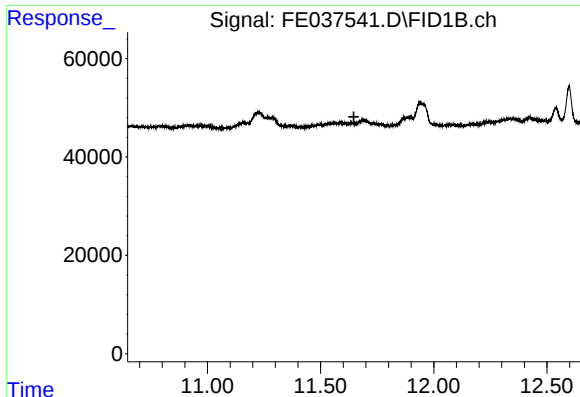

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.647 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

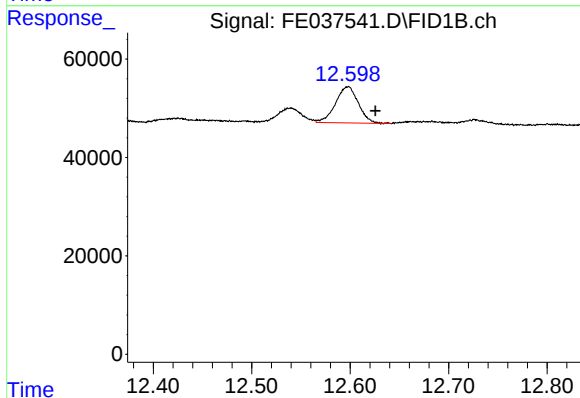


#10 n-Eicosane (C20)

R.T.: 12.598 min
Delta R.T.: -0.027 min
Response: 118571
Conc: 0.75 ug/ml

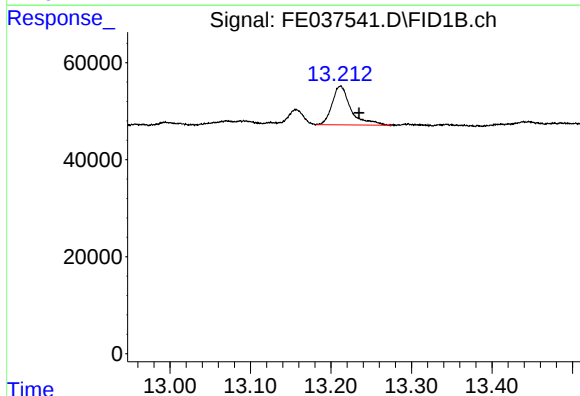


#11 n-Heneicosane (C21)

R.T.: 13.212 min
Delta R.T.: -0.023 min
Response: 128677
Conc: 0.82 ug/ml

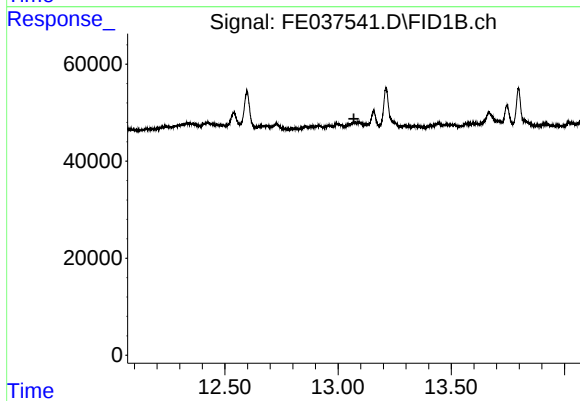

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.070 min
Response: 0
Conc: N.D.

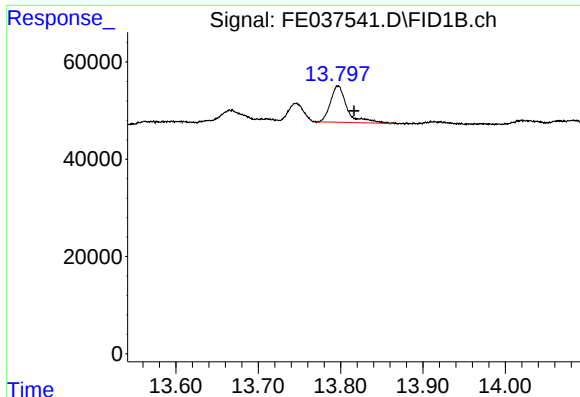

#13 n-Docosane (C22)


R.T.: 13.797 min
Delta R.T.: -0.019 min
Response: 105186
Conc: 0.68 ug/ml

Instrument :
FID_E
ClientSampleId :

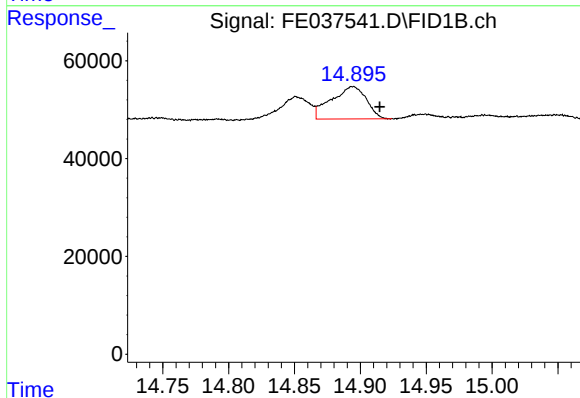


#14 n-Tetracosane (C24)

R.T.: 14.894 min
Delta R.T.: -0.020 min
Response: 122655
Conc: 0.82 ug/ml

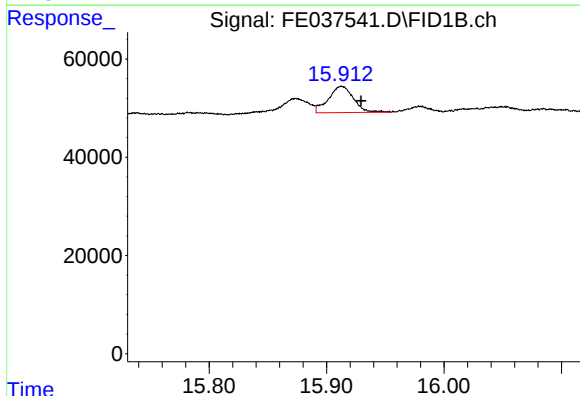


#15 n-Hexacosane (C26)

R.T.: 15.913 min
Delta R.T.: -0.017 min
Response: 78880
Conc: 0.54 ug/ml

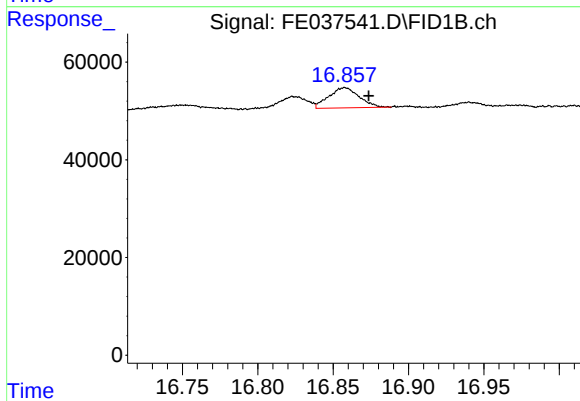

#16 n-Octacosane (C28)


R.T.: 16.858 min
Delta R.T.: -0.016 min
Response: 58194
Conc: 0.42 ug/ml

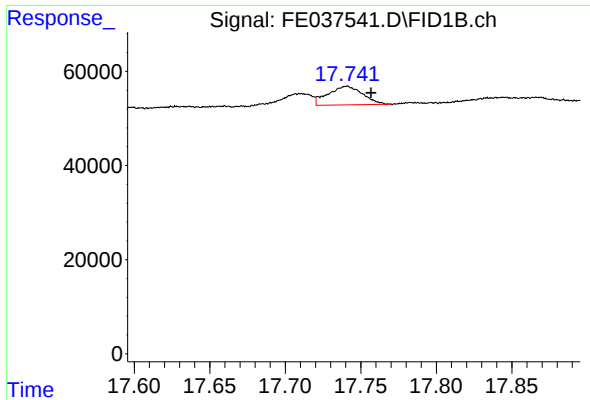

#17 n-Tricontane (C30)

R.T.: 17.741 min
Delta R.T.: -0.016 min
Response: 63183
Conc: 0.46 ug/ml

Instrument :
FID_E
ClientSampleId :

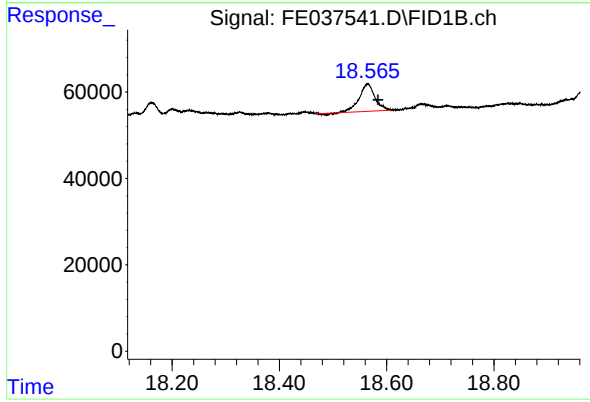

#18 n-Dotriacontane (C32)

R.T.: 18.565 min
Delta R.T.: -0.019 min
Response: 127398
Conc: 0.95 ug/ml