

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091521\
 Data File : FE034328.D
 Signal(s) : FID1B.CH
 Acq On : 15 Sep 2021 12:35
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 16 01:17:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE090821.M
 Quant Title :
 QLast Update : Thu Sep 09 02:48:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.406	6631375	17.732 ug/ml
12) N-OCTACOSANE	16.805	6058619	16.330 ug/ml
13) N-TRIACONTANE	17.691	203492	0.564 ug/ml
14) N-DOTRIACONTANE	18.520	309649	0.877 ug/ml
15) N-TETRATRIACONTANE	19.300	254195	0.809 ug/ml
16) N-HEXATRIACONTANE	20.039	320799	1.079 ug/ml
17) N-OCTATRIACONTANE	20.764	537490	2.013 ug/ml
18) N-TETRACONTANE	21.653	409413	1.528 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091521\
Data File : FE034328.D
Signal(s) : FID1B.CH
Acq On : 15 Sep 2021 12:35
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 01:17:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE090821.M
Quant Title :
QLast Update : Thu Sep 09 02:48:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

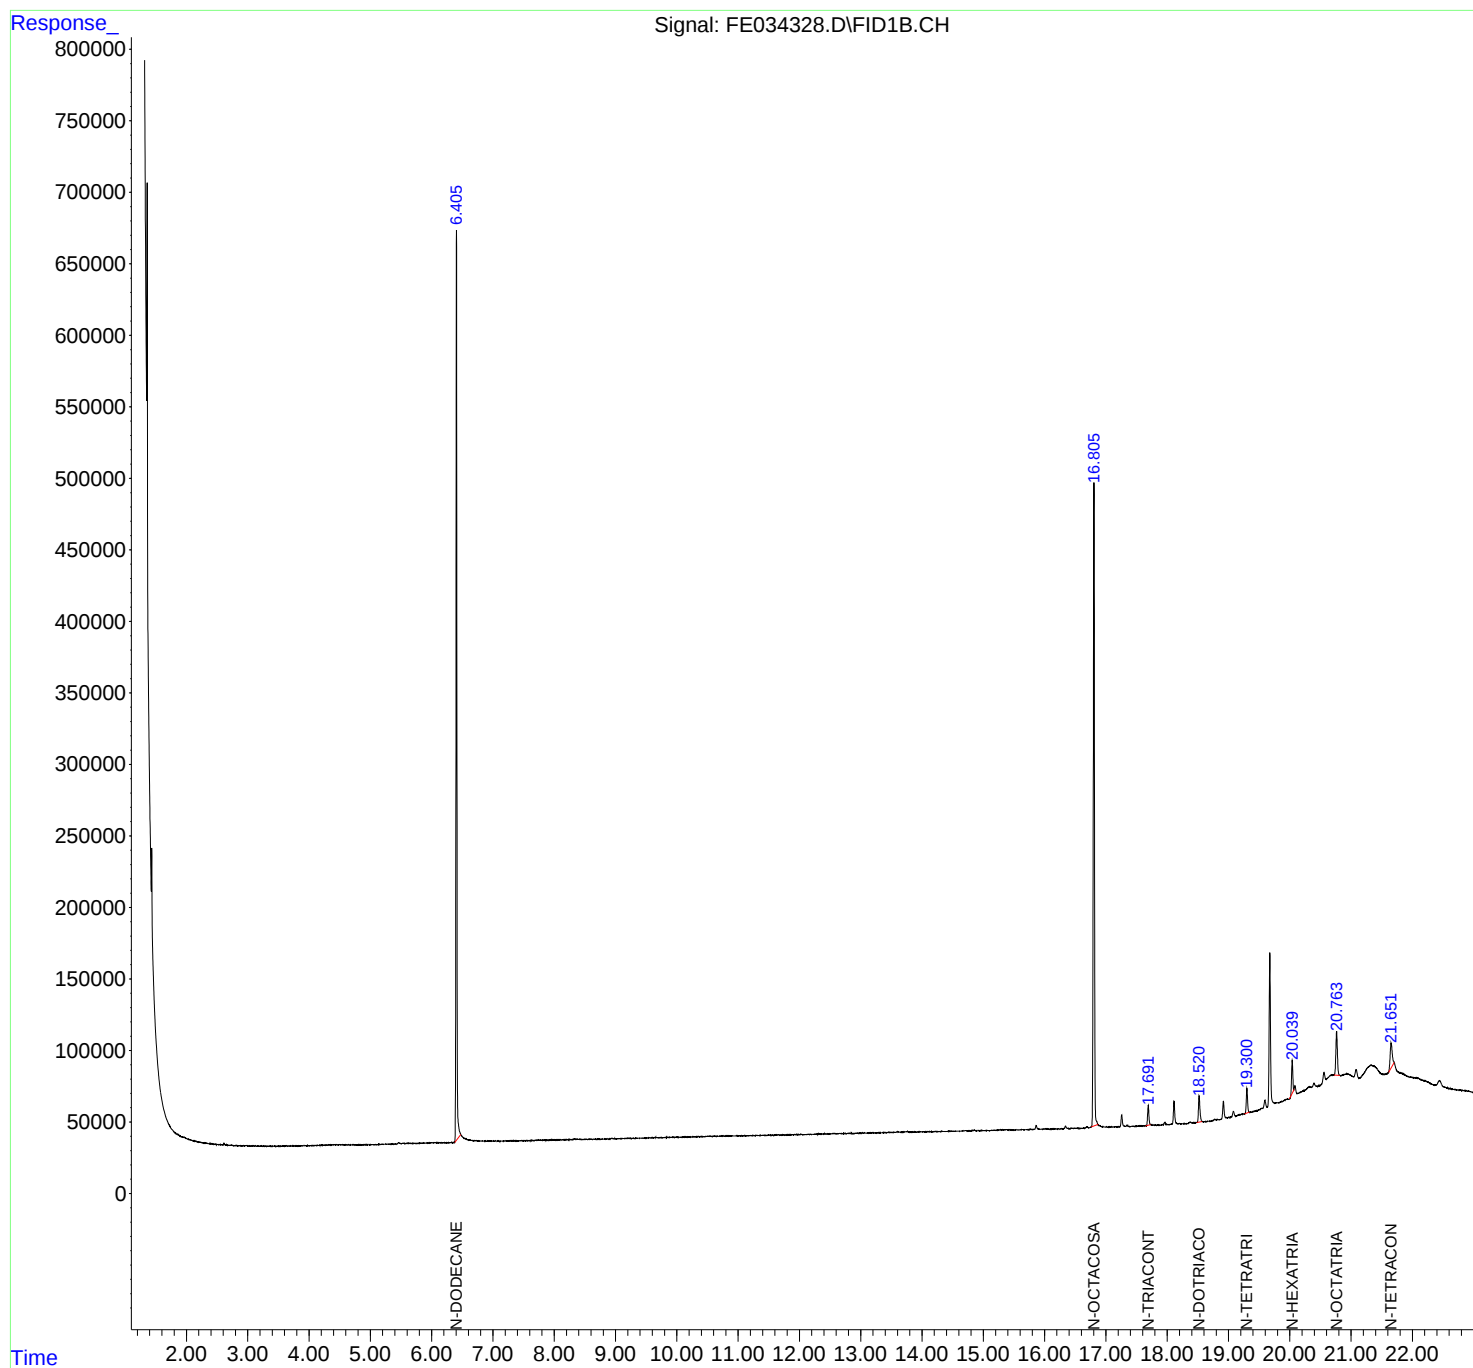


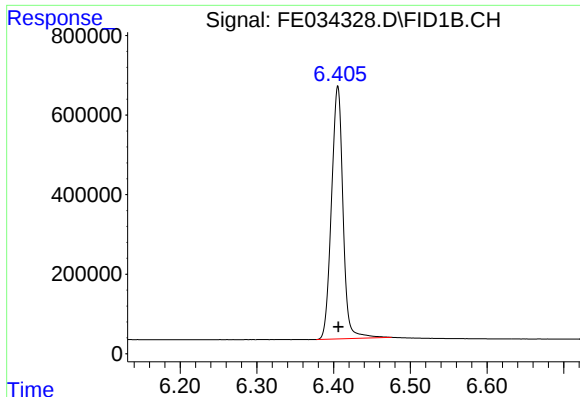

#3 N-DODECANE


R.T.: 6.406 min
Delta R.T.: 0.000 min
Response: 6631375
Conc: 17.73 ug/ml

Instrument :
FID_E
ClientSampleId :

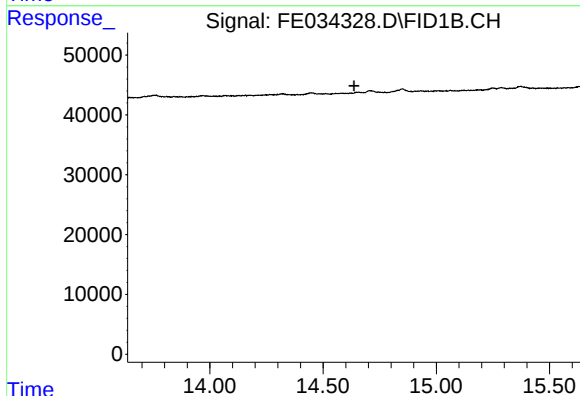


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.636 min
Response: 0
Conc: N.D.

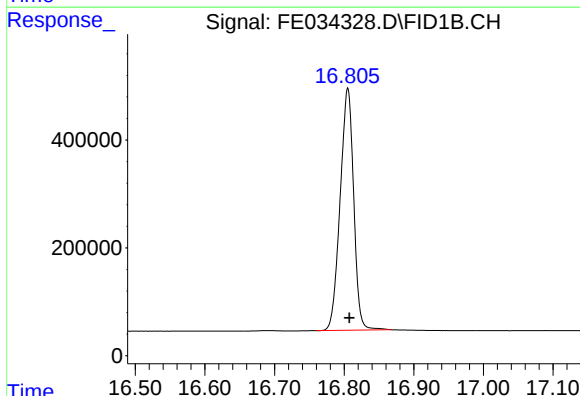


#12 N-OCTACOSANE

R.T.: 16.805 min
Delta R.T.: -0.002 min
Response: 6058619
Conc: 16.33 ug/ml

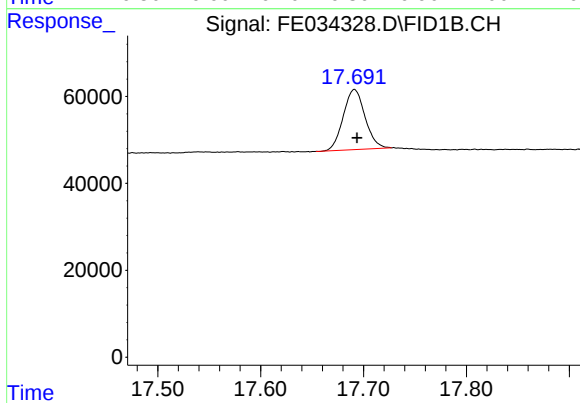

#13 N-TRIACONTANE


R.T.: 17.691 min
Delta R.T.: -0.002 min
Response: 203492
Conc: 0.56 ug/ml

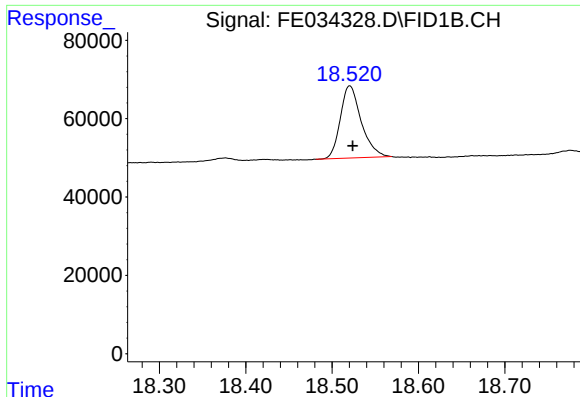

#14 N-DOTRIACONTANE


R.T.: 18.520 min
Delta R.T.: -0.003 min
Response: 309649
Conc: 0.88 ug/ml

Instrument :
FID_E
ClientSampleId :

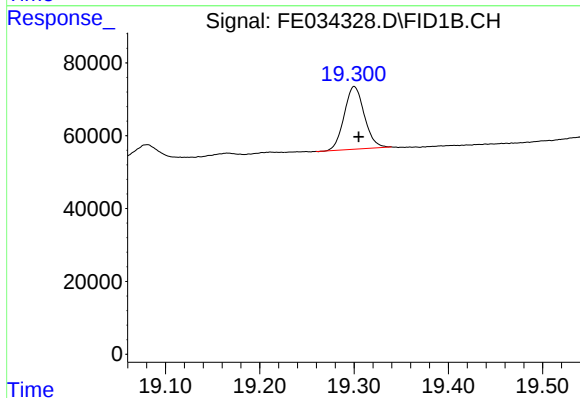


#15 N-TETRATRIACONTANE

R.T.: 19.300 min
Delta R.T.: -0.005 min
Response: 254195
Conc: 0.81 ug/ml

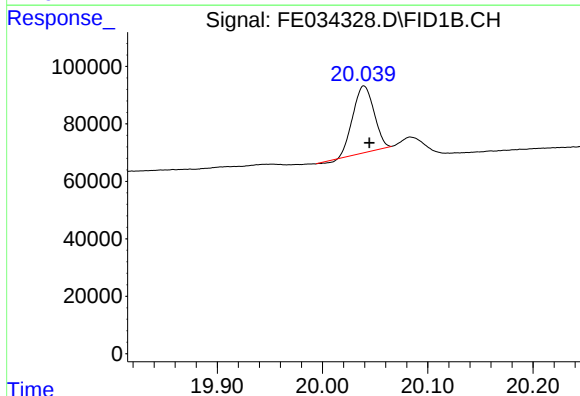


#16 N-HEXATRIACONTANE

R.T.: 20.039 min
Delta R.T.: -0.005 min
Response: 320799
Conc: 1.08 ug/ml

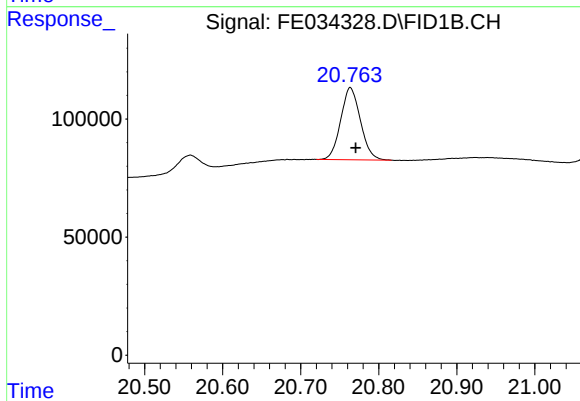

#17 N-OCTATRIACONTANE

R.T.: 20.764 min
Delta R.T.: -0.007 min
Response: 537490
Conc: 2.01 ug/ml

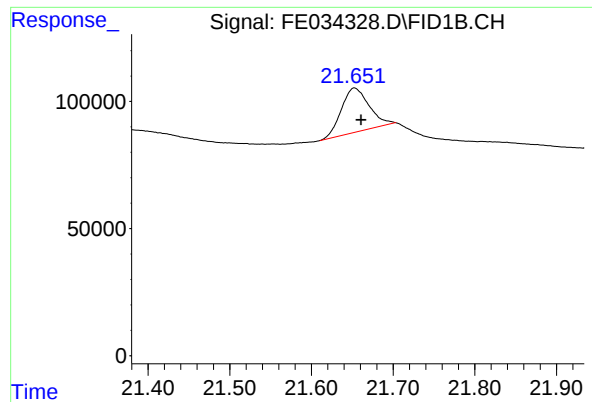

#18 N-TETRACONTANE

R.T.: 21.653 min
Delta R.T.: -0.008 min
Response: 409413
Conc: 1.53 ug/ml

Instrument :
FID_E
ClientSampleId :