

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091521\  
Data File : FE034336.D  
Signal(s) : FID1B.CH  
Acq On : 15 Sep 2021 17:18  
Operator : DD\AJ  
Sample : M3723-01 5X  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
BU-03-091321

Manual Integrations  
APPROVED

mohammad  
9/16/2021 1:29:23 PM

Integration File: Sample.e  
Quant Time: Sep 16 01:19:35 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE090821.M  
Quant Title :  
QLast Update : Thu Sep 09 02:48:26 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.635 | 1762322  | 5.289 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091521\  
Data File : FE034336.D  
Signal(s) : FID1B.CH  
Acq On : 15 Sep 2021 17:18  
Operator : DD\AJ  
Sample : M3723-01 5X  
Misc :  
ALS Vial : 12 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
BU-03-091321


Manual Integrations  
APPROVED

mohammad  
9/16/2021 1:29:23 PM

Integration File: Sample.e  
Quant Time: Sep 16 01:19:35 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE090821.M  
Quant Title :  
QLast Update : Thu Sep 09 02:48:26 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

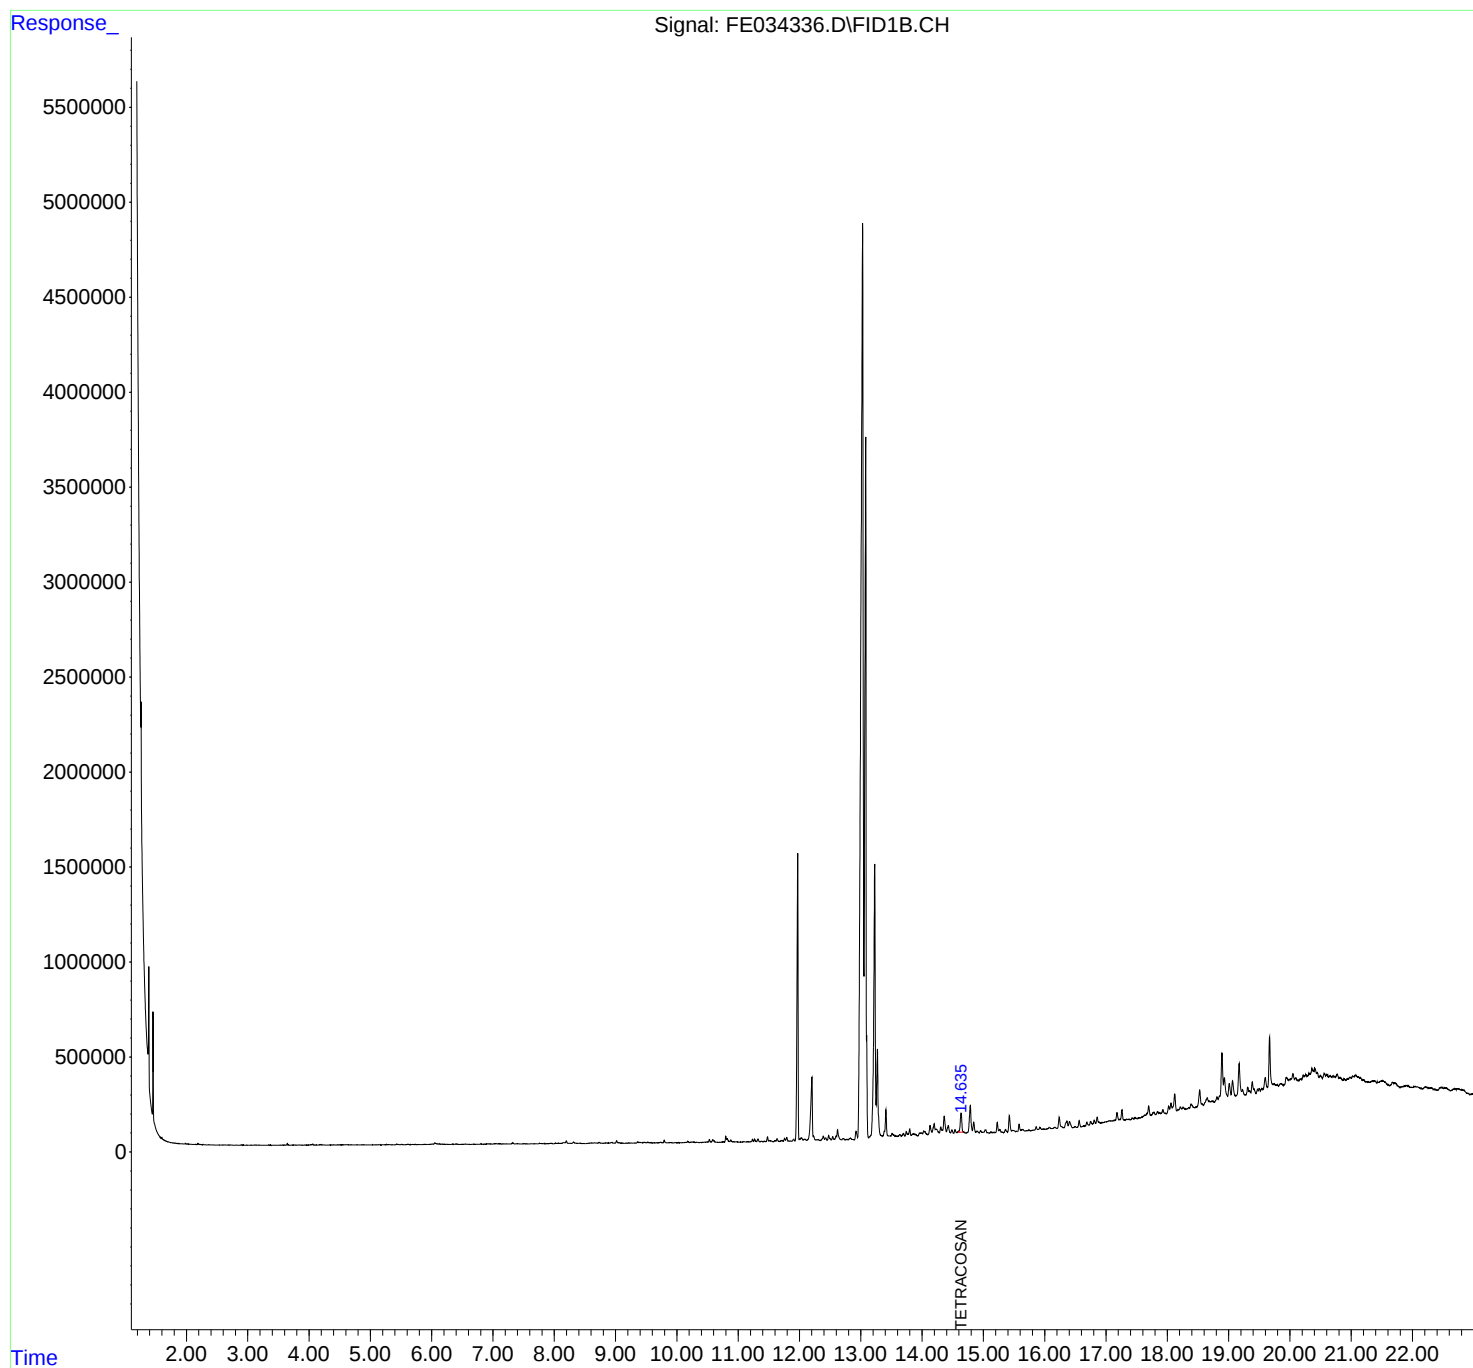

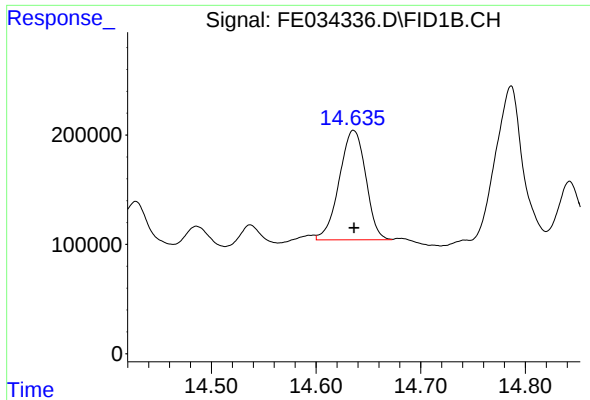

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.635 min  
Delta R.T.: -0.001 min  
Response: 1762322  
Conc: 5.29 ug/ml m

Instrument :  
FID\_E  
ClientSampleId :  
BU-03-091321

Manual Integrations  
APPROVED

mohammad  
9/16/2021 1:29:23 PM