

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091523AL\
 Data File : FE044324.D
 Signal(s) : FID1B.ch
 Acq On : 16 Sep 2023 01:15
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 16 03:47:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 083023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 31 03:37:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.704	395423	2.826 ug/ml
20) T	n-Hexatriacontane (C36)	20.445	5039	0.037 ug/ml
22) T	n-Tetracontane (C40)	22.118	135228	0.978 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091523AL\
Data File : FE044324.D
Signal(s) : FID1B.ch
Acq On : 16 Sep 2023 01:15
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:47:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 083023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 31 03:37:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

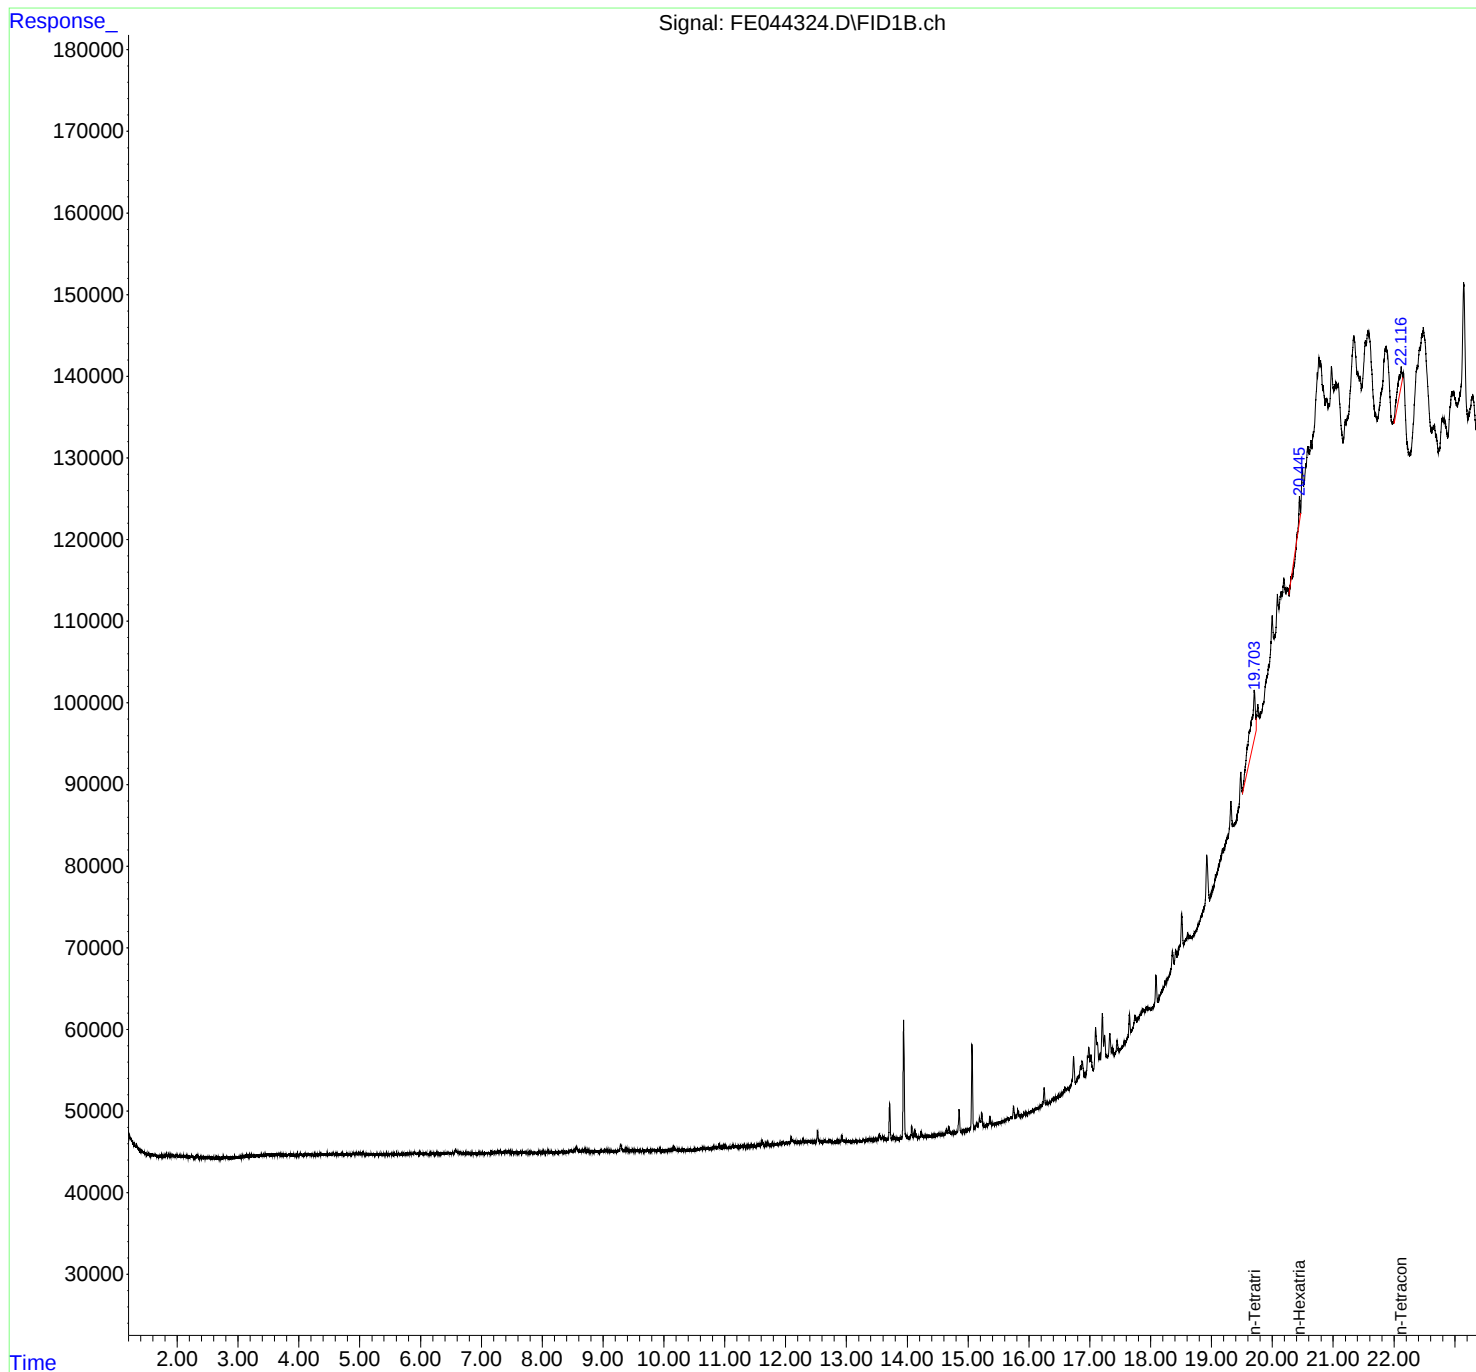


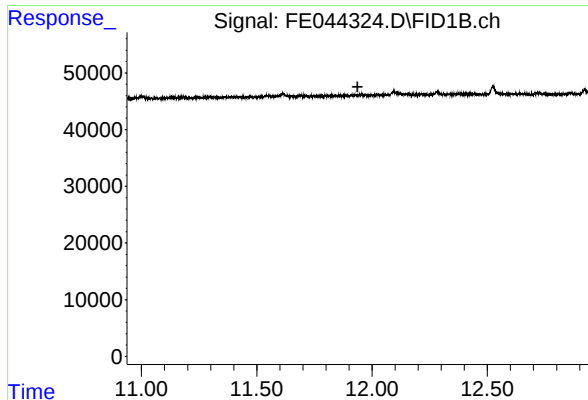

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.937 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

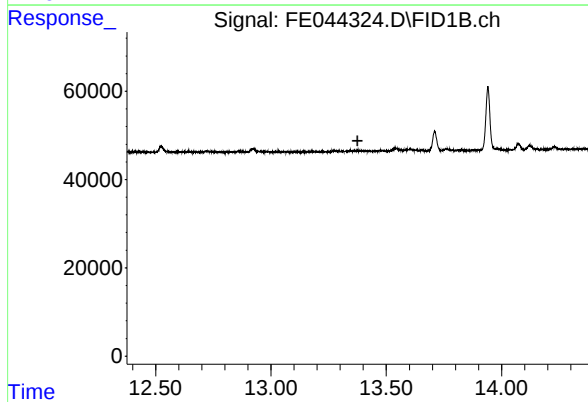


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.375 min
Response: 0
Conc: N.D.

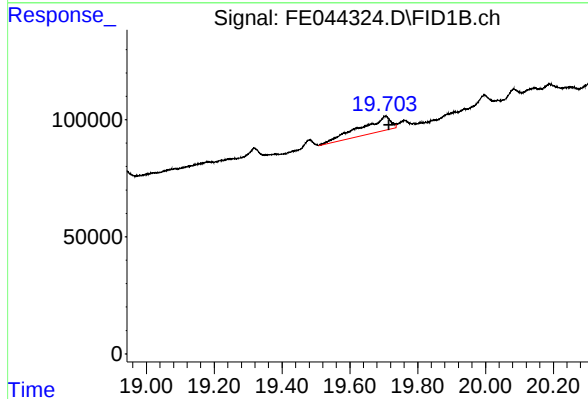


#19 n-Tetratriacontane (C34)

R.T.: 19.704 min
Delta R.T.: -0.011 min
Response: 395423
Conc: 2.83 ug/ml

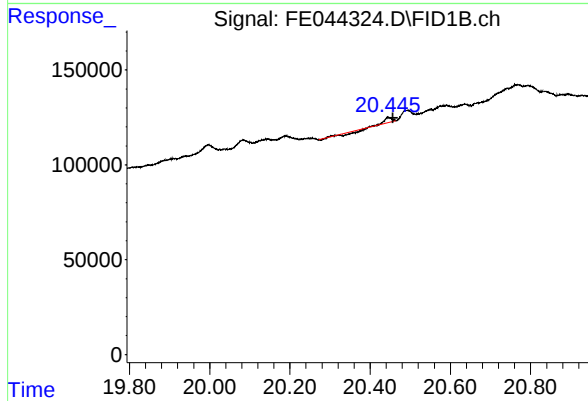

#20 n-Hexatriacontane (C36)

R.T.: 20.445 min
Delta R.T.: -0.012 min
Response: 5039
Conc: 0.04 ug/ml

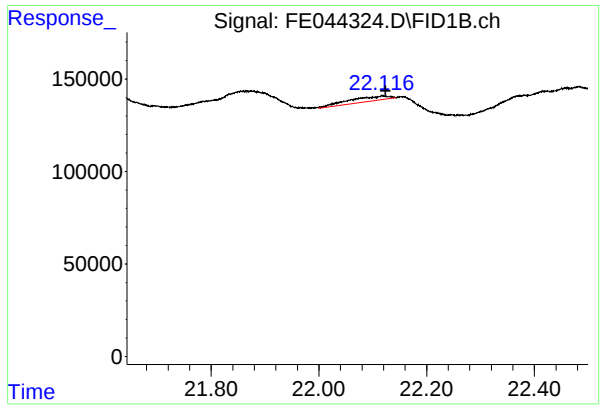

#22 n-Tetracontane (C40)

R.T.: 22.118 min
Delta R.T.: -0.006 min
Response: 135228
Conc: 0.98 ug/ml

Instrument :

FID_E

ClientSampleId :