

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091523AL\  
 Data File : FE044302.D  
 Signal(s) : FID1B.ch  
 Acq On : 15 Sep 2023 08:08  
 Operator : YP\AJ  
 Sample : 04409-10DL 10X  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 WC-4(0-6)COMPDL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 09/15/2023  
 Supervised By :Ankita Jodhani 09/15/2023

Integration File: autoint1.e  
 Quant Time: Sep 15 08:33:43 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 083023.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Aug 31 03:37:37 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.926 | 674624     | 3.561 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 7.12%        |
| 12) S 1-chlorooctadecane (S... | 13.365 | 527453     | 3.818 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 7.64%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE091523AL\  
Data File : FE044302.D  
Signal(s) : FID1B.ch  
Acq On : 15 Sep 2023 08:08  
Operator : YP\AJ  
Sample : 04409-10DL 10X  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

## Instrument :

FID\_E

## ClientSampleId :

WC-4(0-6)COMPDL

## Manual Integrations

## APPROVED

Reviewed By :Yogesh Patel 09/15/2023

Supervised By :Ankita Jodhani 09/15/2023

Integration File: autoint1.e

Quant Time: Sep 15 08:33:43 2023

Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 083023.

Quant Title : GC Extractables

QLast Update : Thu Aug 31 03:37:37 2023


Response via : Initial Calibration


Integrator: ChemStation

Volume Inj. : 1 ul

Signal Phase : Rxi-1ms

Signal Info : 20M x 0.18mm x 0.18um

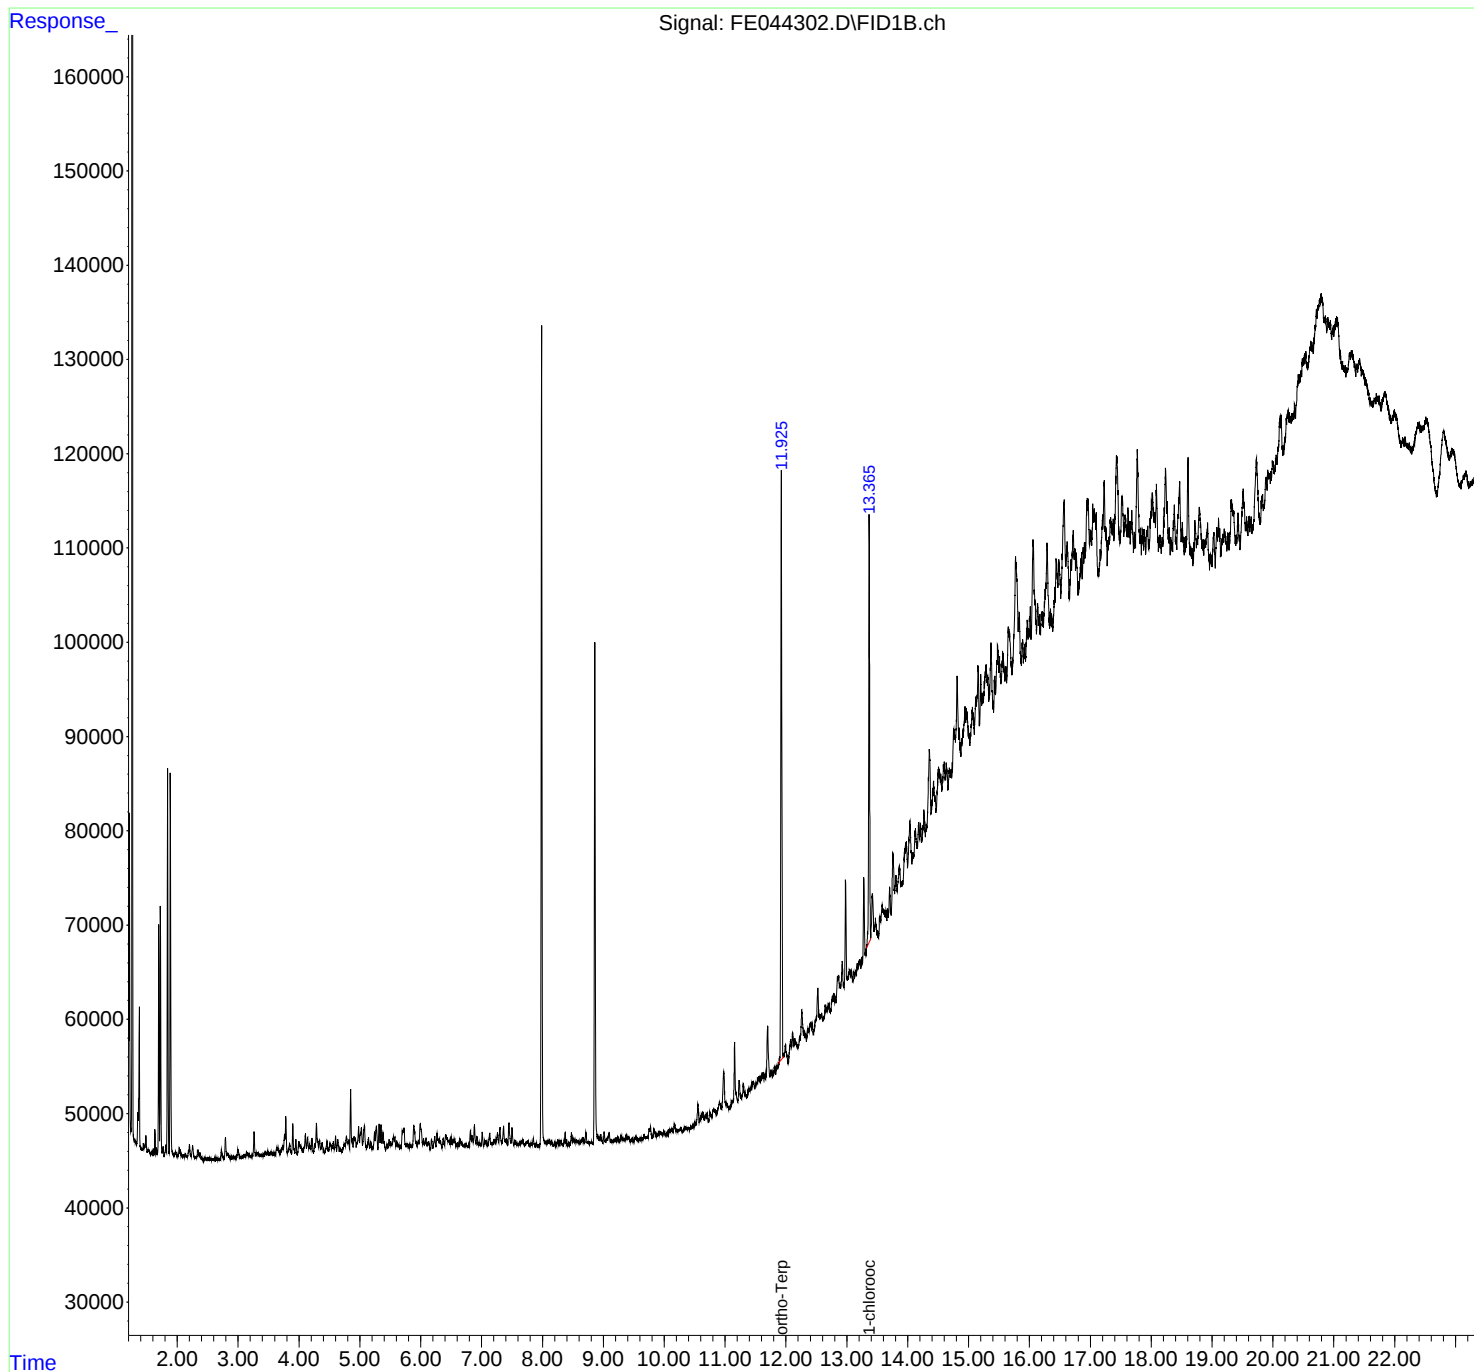

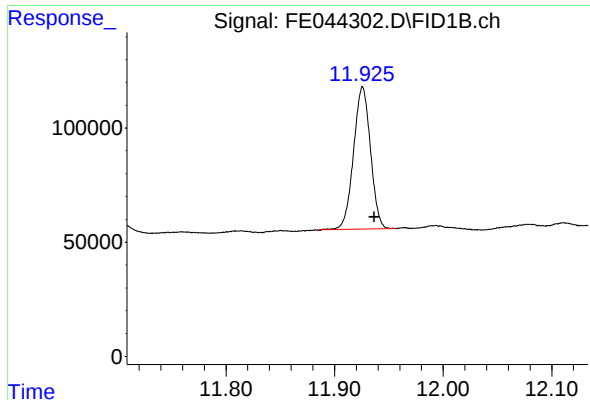


#9 ortho-Terphenyl (SURR)

R.T.: 11.926 min  
Delta R.T.: -0.011 min  
Response: 674624  
Conc: 3.56 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
WC-4(0-6)COMPDL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/15/2023  
Supervised By :Ankita Jodhani 09/15/2023

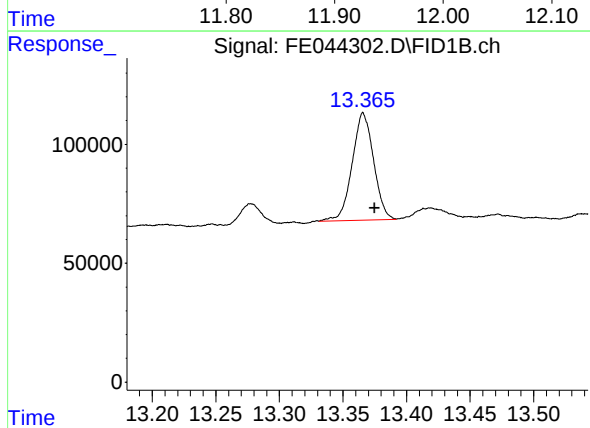

#12 1-chlorooctadecane (SURR)

R.T.: 13.365 min  
Delta R.T.: -0.010 min  
Response: 527453  
Conc: 3.82 ug/ml m