

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091621\
 Data File : FE034339.D
 Signal(s) : FID1B.CH
 Acq On : 16 Sep 2021 12:02
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 16 17:27:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE090821.M
 Quant Title :
 QLast Update : Thu Sep 09 02:48:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.525	447526	1.155 ug/ml
8) N-DOCOSANE	13.731	501279	1.312 ug/ml
10) N-TETRACOSANE	14.832	577301	1.512 ug/ml
11) N-HEXACOSANE	15.856	319324	0.851 ug/ml
12) N-OCTACOSANE	16.804	275682	0.743 ug/ml
13) N-TRIACONTANE	17.692	293977	0.815 ug/ml
14) N-DOTRIACONTANE	18.525	598227	1.694 ug/ml
16) N-HEXATRIACONTANE	20.084	312184	1.050 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091621\
Data File : FE034339.D
Signal(s) : FID1B.CH
Acq On : 16 Sep 2021 12:02
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 16 17:27:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE090821.M
Quant Title :
QLast Update : Thu Sep 09 02:48:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

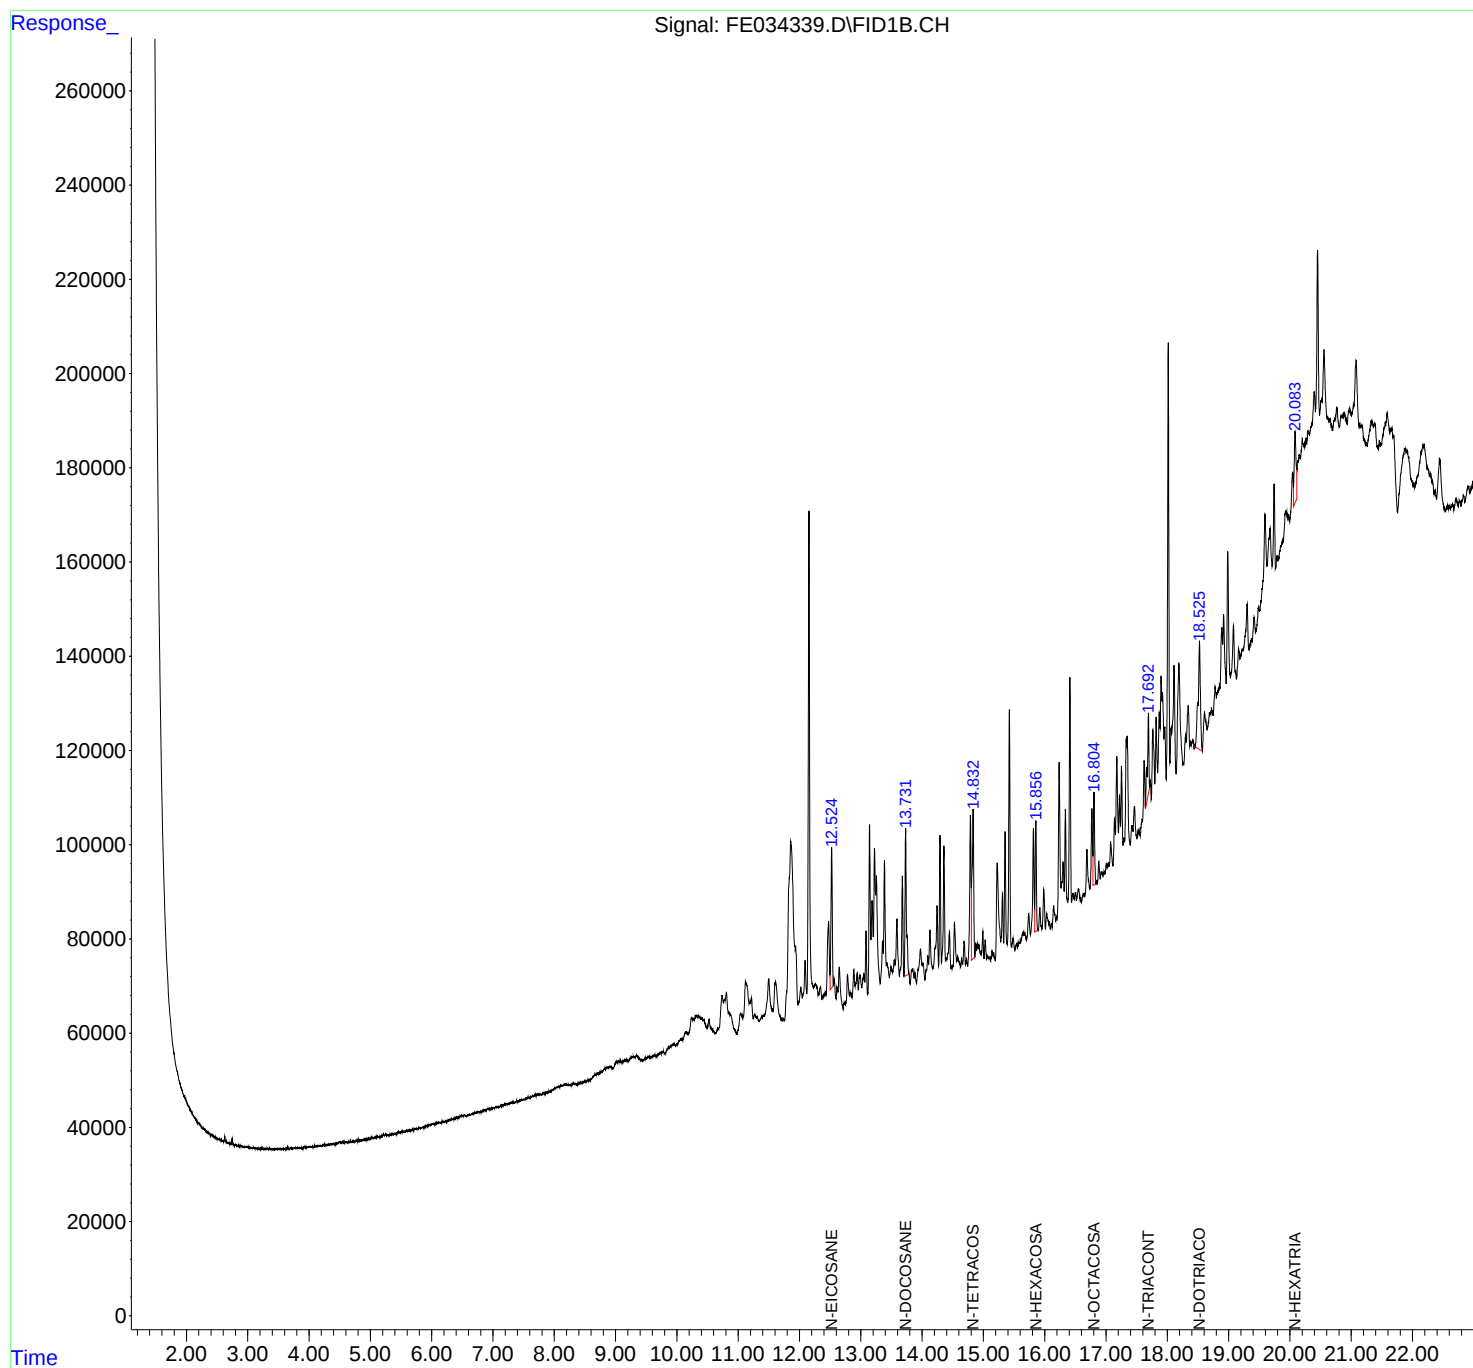


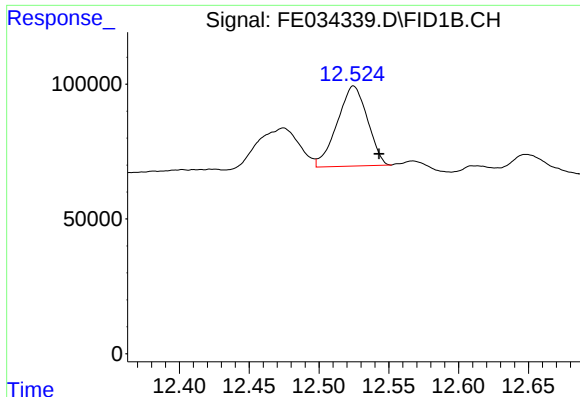

#7 N-EICOSANE


R.T.: 12.525 min
Delta R.T.: -0.018 min
Response: 447526
Conc: 1.15 ug/ml

Instrument :
FID_E
ClientSampleId :

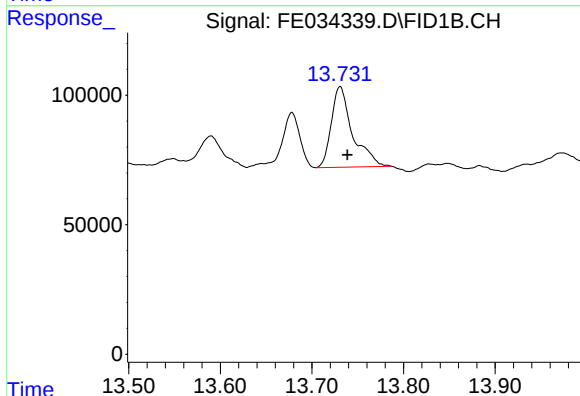


#8 N-DOCOSANE

R.T.: 13.731 min
Delta R.T.: -0.008 min
Response: 501279
Conc: 1.31 ug/ml

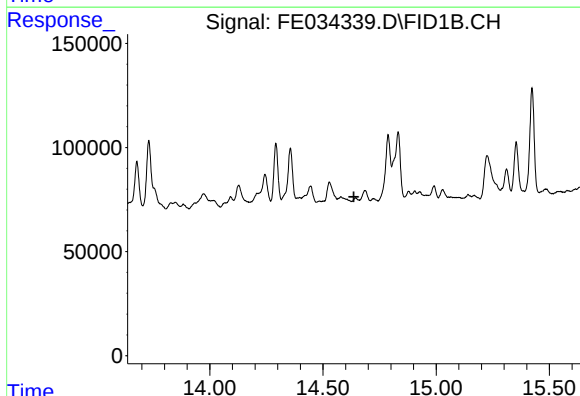


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.636 min
Response: 0
Conc: N.D.

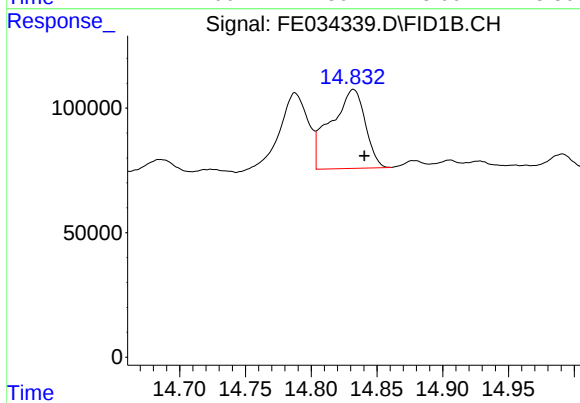

#10 N-TETRACOSANE


R.T.: 14.832 min
Delta R.T.: -0.008 min
Response: 577301
Conc: 1.51 ug/ml

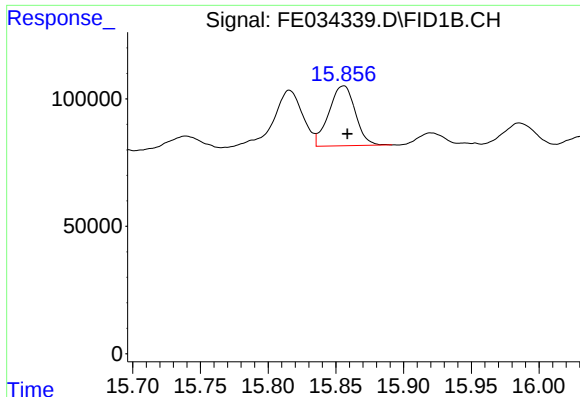

#11 N-HEXACOSANE


R.T.: 15.856 min
Delta R.T.: -0.003 min
Response: 319324
Conc: 0.85 ug/ml

Instrument :
FID_E
ClientSampleId :

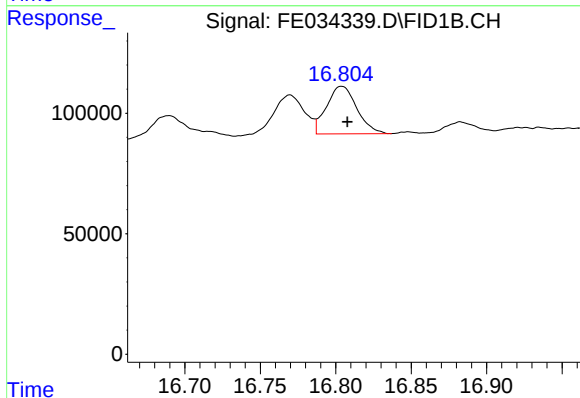


#12 N-OCTACOSANE

R.T.: 16.804 min
Delta R.T.: -0.004 min
Response: 275682
Conc: 0.74 ug/ml

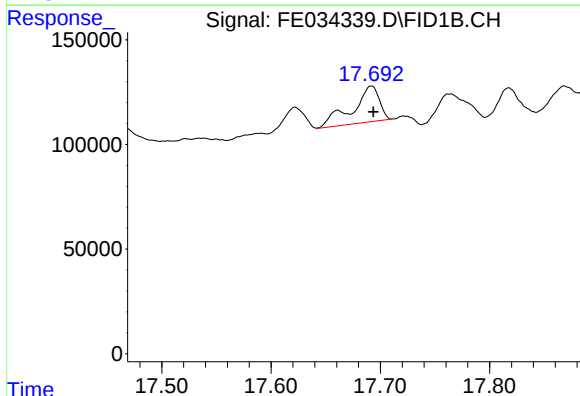


#13 N-TRIACONTANE

R.T.: 17.692 min
Delta R.T.: -0.002 min
Response: 293977
Conc: 0.82 ug/ml

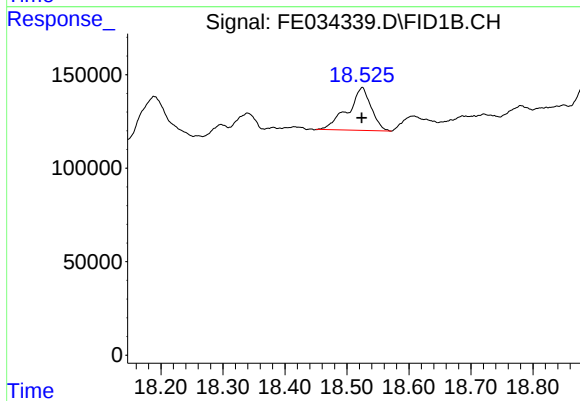

#14 N-DOTRIACONTANE

R.T.: 18.525 min
Delta R.T.: 0.001 min
Response: 598227
Conc: 1.69 ug/ml

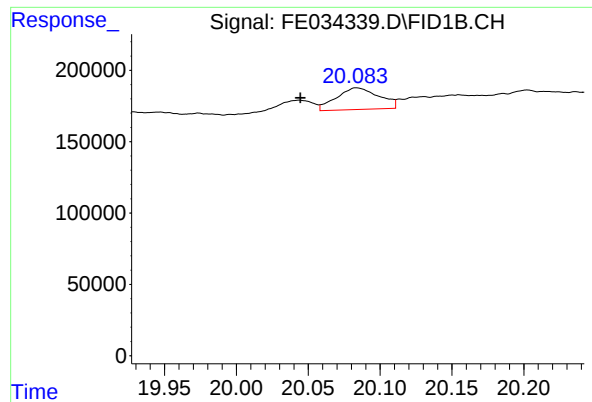

#16 N-HEXATRIACONTANE

R.T.: 20.084 min
Delta R.T.: 0.039 min
Response: 312184
Conc: 1.05 ug/ml

Instrument :
FID_E
ClientSampleId :