

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091621\
 Data File : FE034350.D
 Signal(s) : FID1B.CH
 Acq On : 16 Sep 2021 18:19
 Operator : DD\AJ
 Sample : M3757-01 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 17 01:20:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE090821.M
 Quant Title :
 QLast Update : Thu Sep 09 02:48:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	602965	1.810 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.807	22123	0.060 ug/ml
13) N-TRIACONTANE	17.694	253815	0.704 ug/ml
14) N-DOTRIACONTANE	18.525	458987	1.300 ug/ml
15) N-TETRATRIACONTANE	19.306	307772	0.980 ug/ml
16) N-HEXATRIACONTANE	20.050	427709	1.438 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091621\
Data File : FE034350.D
Signal(s) : FID1B.CH
Acq On : 16 Sep 2021 18:19
Operator : DD\AJ
Sample : M3757-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 17 01:20:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE090821.M
Quant Title :
QLast Update : Thu Sep 09 02:48:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

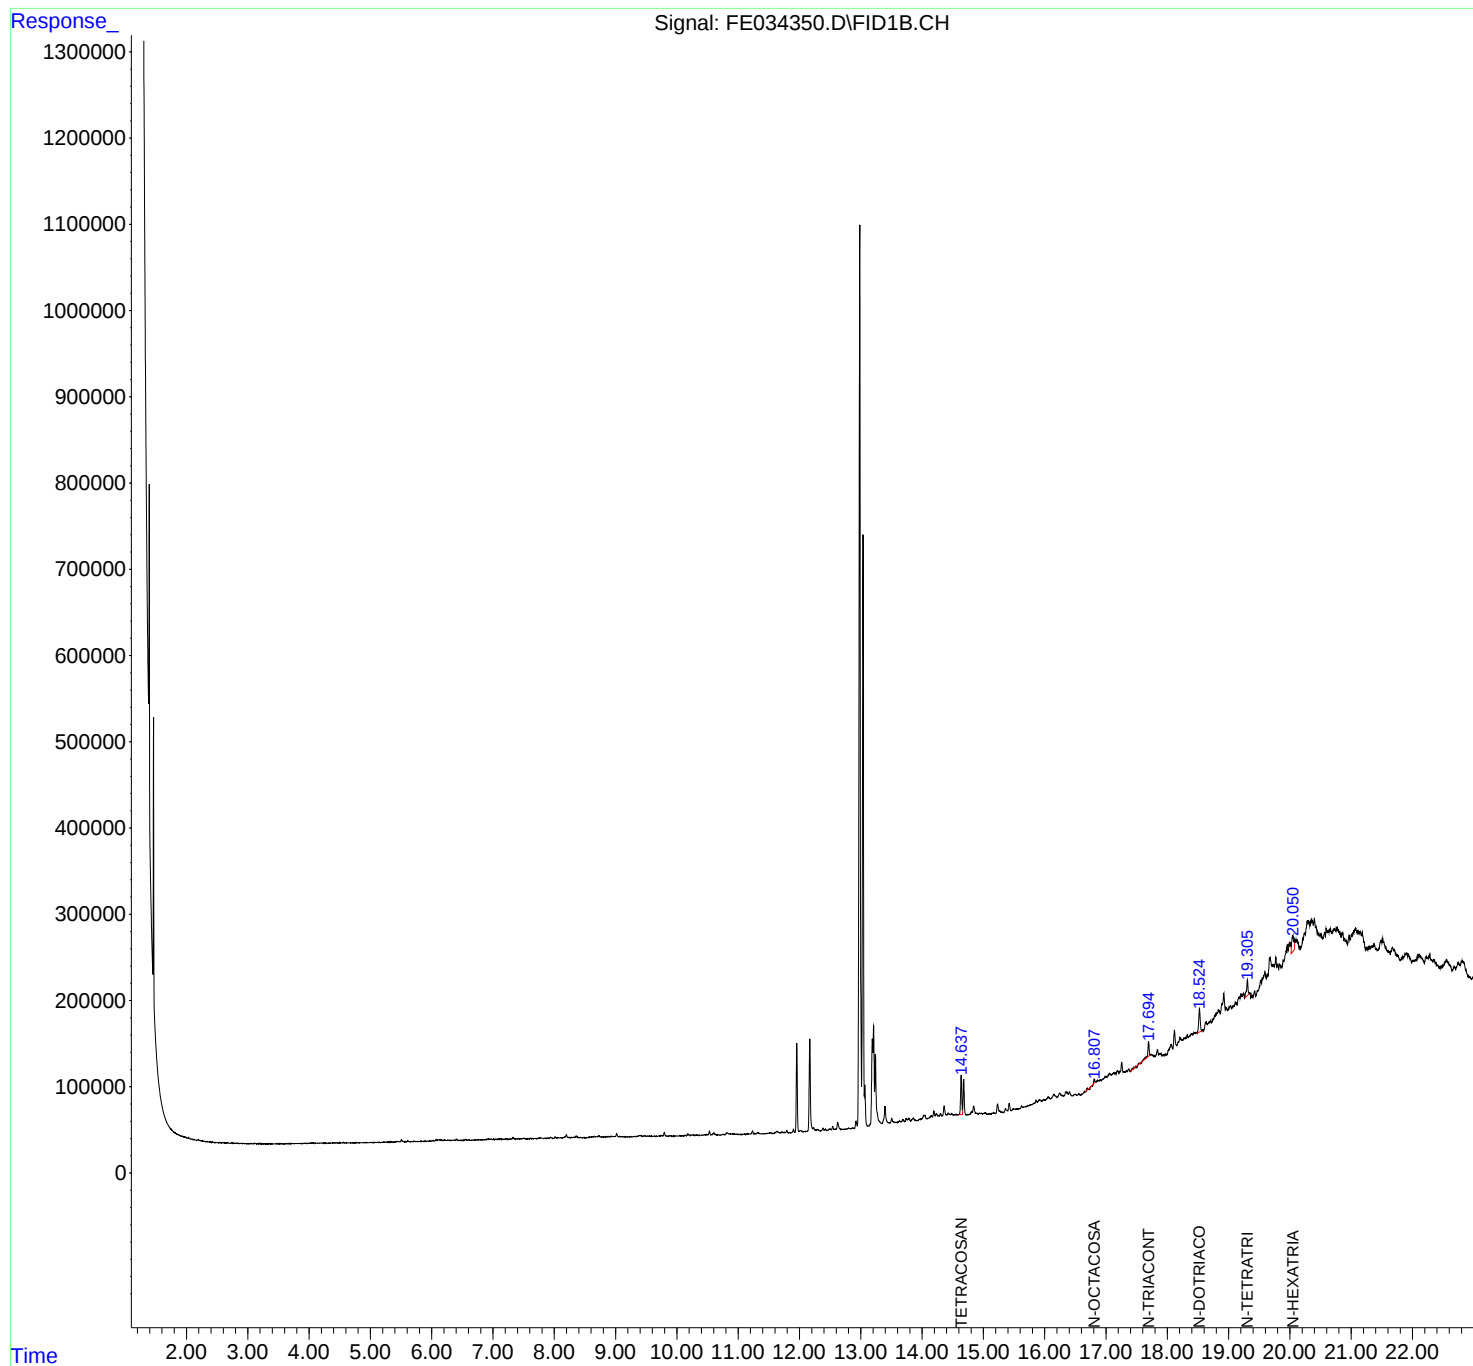


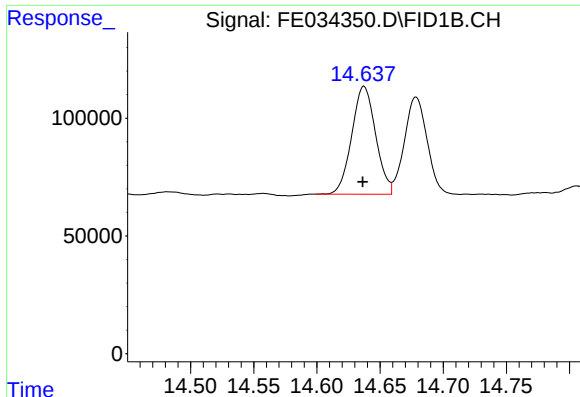

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.637 min
Delta R.T.: 0.000 min
Response: 602965
Conc: 1.81 ug/ml

Instrument :
FID_E
ClientSampleId :

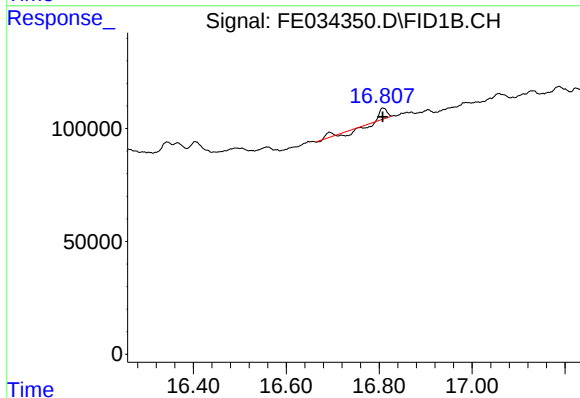


#12 N-OCTACOSANE

R.T.: 16.807 min
Delta R.T.: 0.000 min
Response: 22123
Conc: 0.06 ug/ml

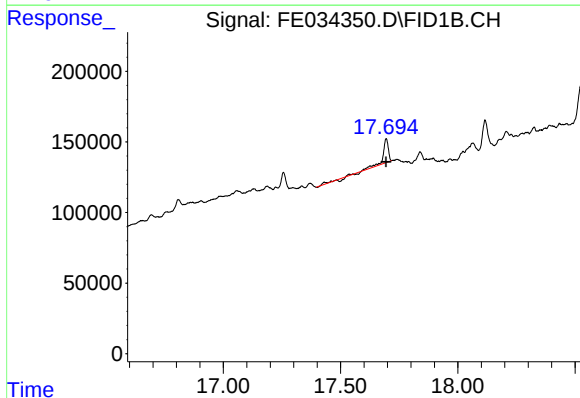


#13 N-TRIACONTANE

R.T.: 17.694 min
Delta R.T.: 0.000 min
Response: 253815
Conc: 0.70 ug/ml

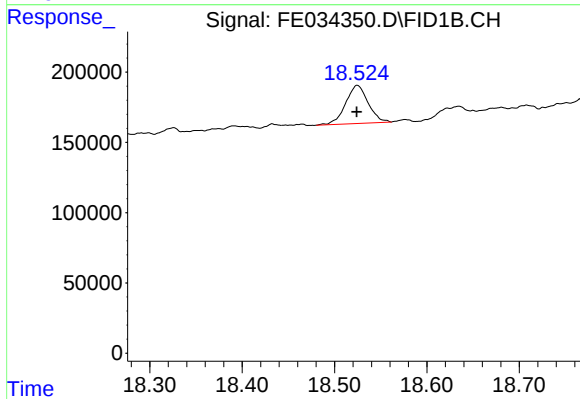

#14 N-DOTRIACONTANE

R.T.: 18.525 min
Delta R.T.: 0.000 min
Response: 458987
Conc: 1.30 ug/ml

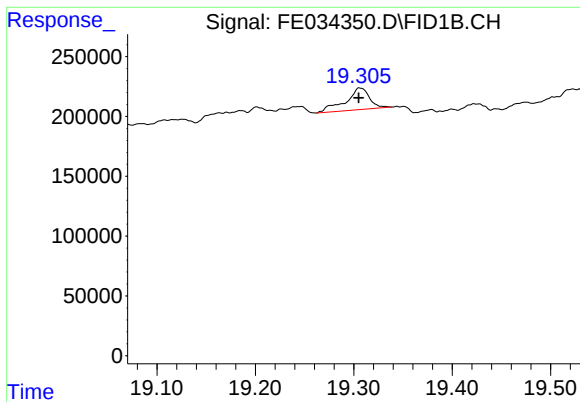

#15 N-TETRATRIACONTANE


R.T.: 19.306 min

Delta R.T.: 0.001 min

Response: 307772

Conc: 0.98 ug/ml

Instrument :
FID_E
ClientSampleId :

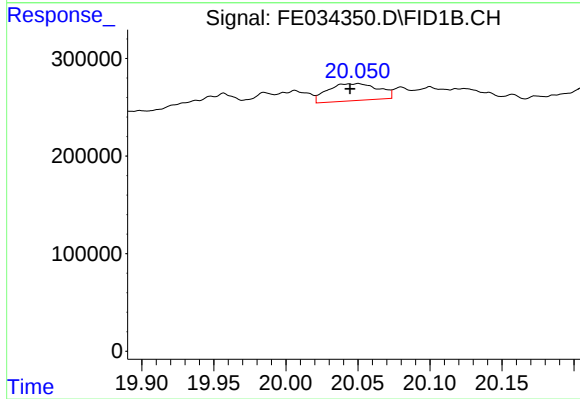

#16 N-HEXATRIACONTANE

R.T.: 20.050 min

Delta R.T.: 0.006 min

Response: 427709

Conc: 1.44 ug/ml