

Data Path : Z:\bestpcbsrv\HPCHEM1\FID E\Data\FE091718\
Data File : FE028653.D
Signal(s) : FID1B.CH
Acq On : 17 Sep 2018 15:10
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 18 07:13:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.969	3482024	12.425 ug/ml
Target Compounds				
10)	N-TETRACOSANE	15.147	4270568	18.073 ug/ml
12)	N-DOTRIACONTANE	18.871	830243	4.528 ug/ml
14)	N-HEXATRIACONTANE	20.404	369395	2.805 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID E\Data\FE091718\
Data File : FE028653.D
Signal(s) : FID1B.CH
Acq On : 17 Sep 2018 15:10
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 18 07:13:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

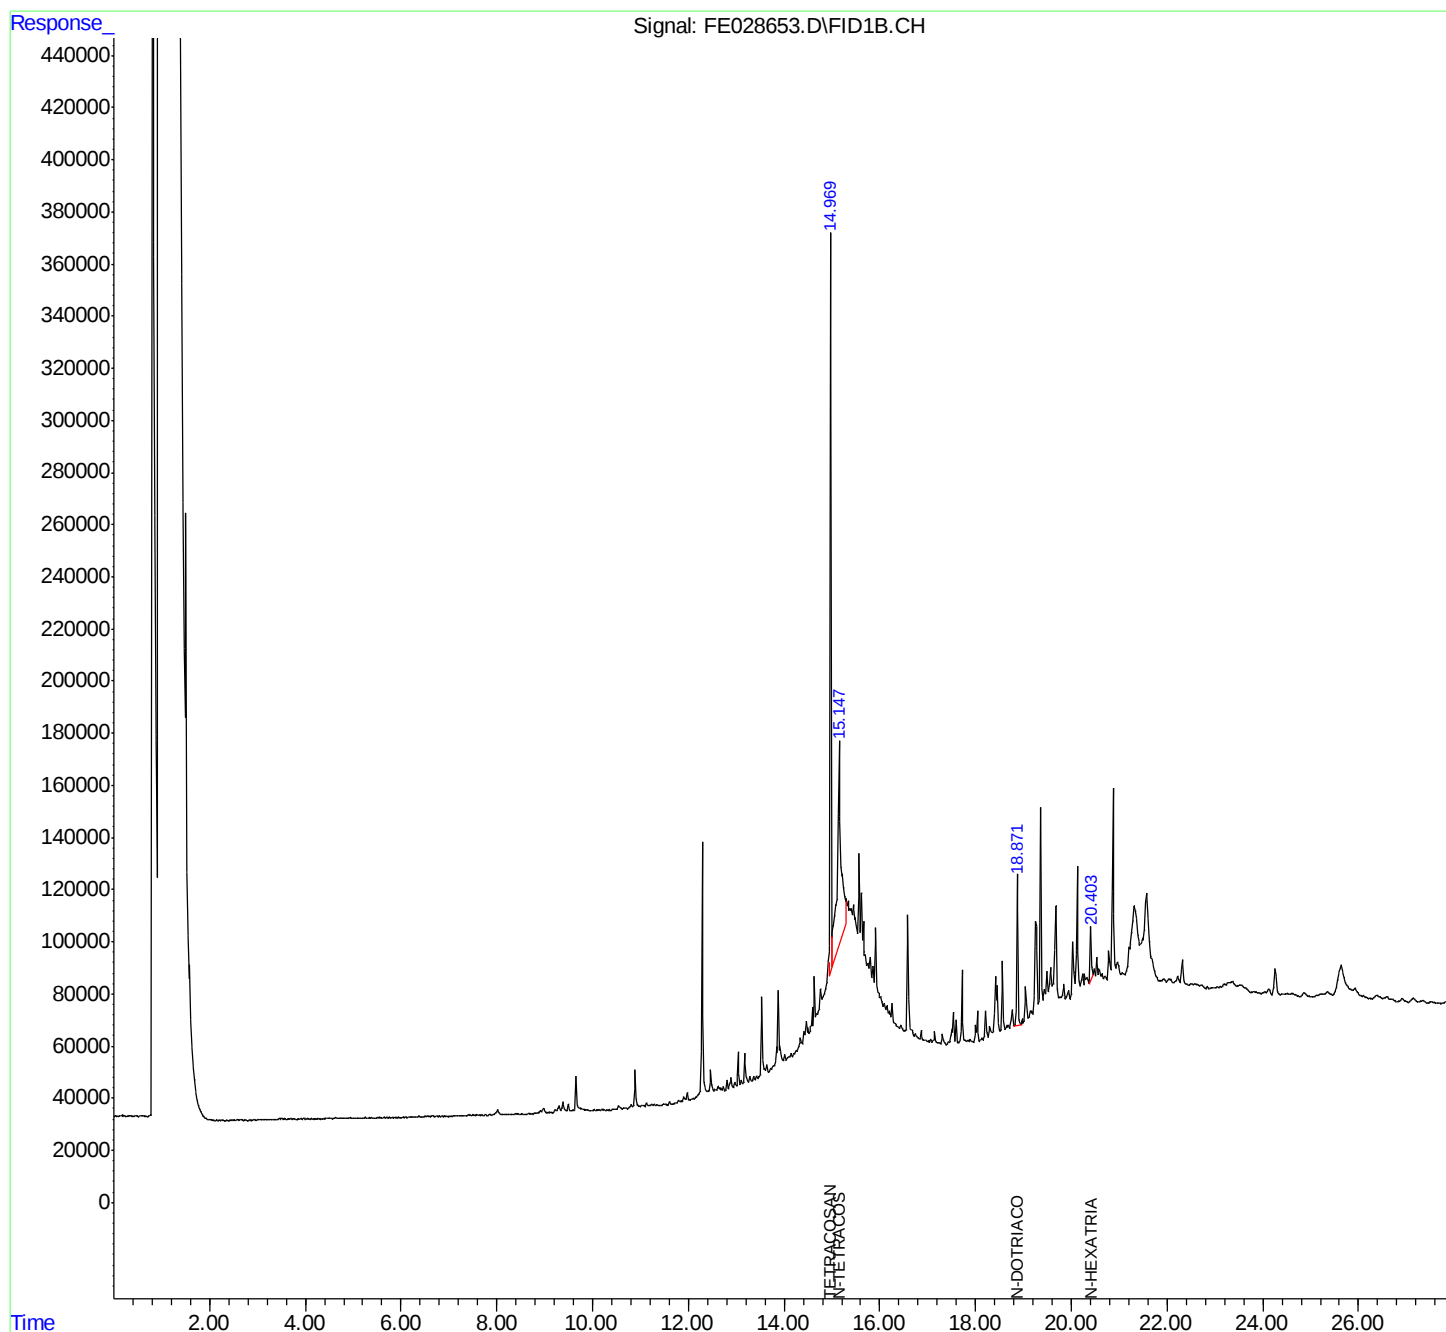

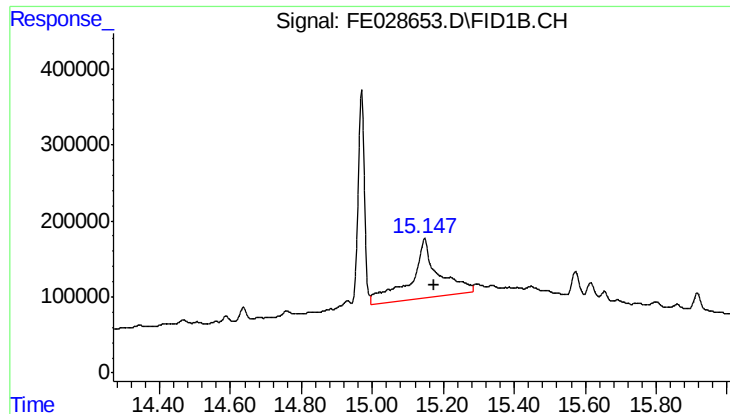


#10 N-TETRACOSANE

R.T.: 15.147 min
Delta R.T.: -0.025 min
Response: 4270568
Conc: 18.07 ug/ml

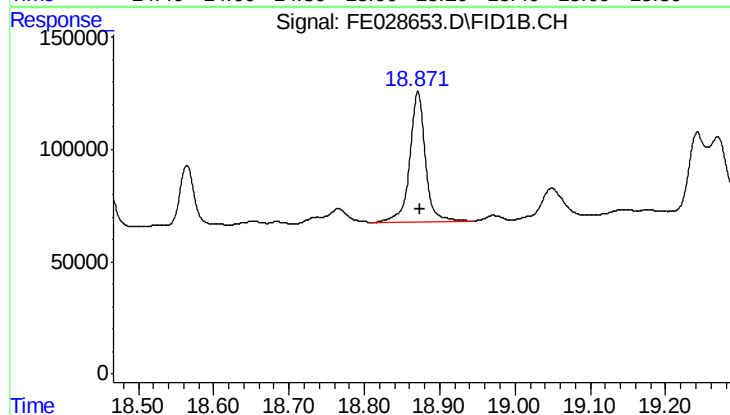


#12 N-DOTRIACONTANE

R.T.: 18.871 min
Delta R.T.: -0.003 min
Response: 830243
Conc: 4.53 ug/ml

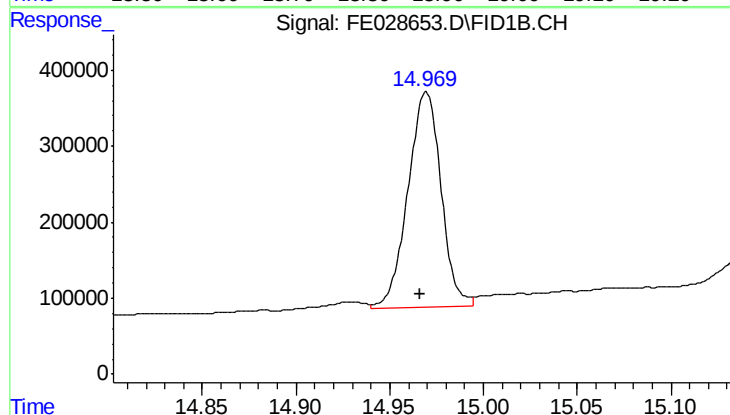

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.969 min
Delta R.T.: 0.004 min
Response: 3482024
Conc: 12.42 ug/ml

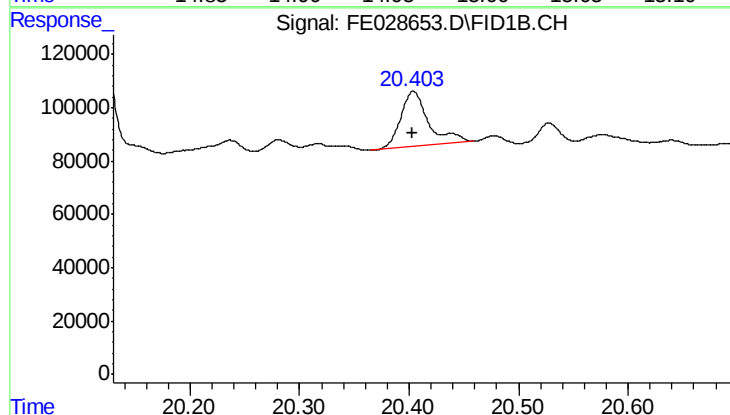

#14 N-HEXATRIACONTANE

R.T.: 20.404 min
Delta R.T.: 0.002 min
Response: 369395
Conc: 2.80 ug/ml