

Data Path : Z:\bestpcbsrv\HPCHEM1\FID E\Data\FE091718\
 Data File : FE028655.D
 Signal(s) : FID1B.CH
 Acq On : 17 Sep 2018 16:27
 Operator : AJ\SJ
 Sample : J4941-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 18 07:14:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
 Quant Title :
 QLast Update : Tue Aug 21 14:35:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.943	13003182	46.399 ug/ml
Target Compounds				
6)	N-TETRADECANE	8.485	1074295	6.438 ug/ml
7)	N-HEXADECANE	10.073	24138901	126.895 ug/ml
8)	N-OCTADECANE	11.524	35536821	168.758 ug/ml
9)	N-EICOSANE	12.875	19025129	83.481 ug/ml
10)	N-TETRACOSANE	15.186	8511390	36.019 ug/ml
11)	N-OCTACOSANE	17.158	2195647	9.877 ug/ml
12)	N-DOTRIACONTANE	18.883	2223369	12.127 ug/ml
14)	N-HEXATRIACONTANE	20.414	800394	6.077 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID E\Data\FE091718\
Data File : FE028655.D
Signal(s) : FID1B.CH
Acq On : 17 Sep 2018 16:27
Operator : AJ\SJ
Sample : J4941-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 18 07:14:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

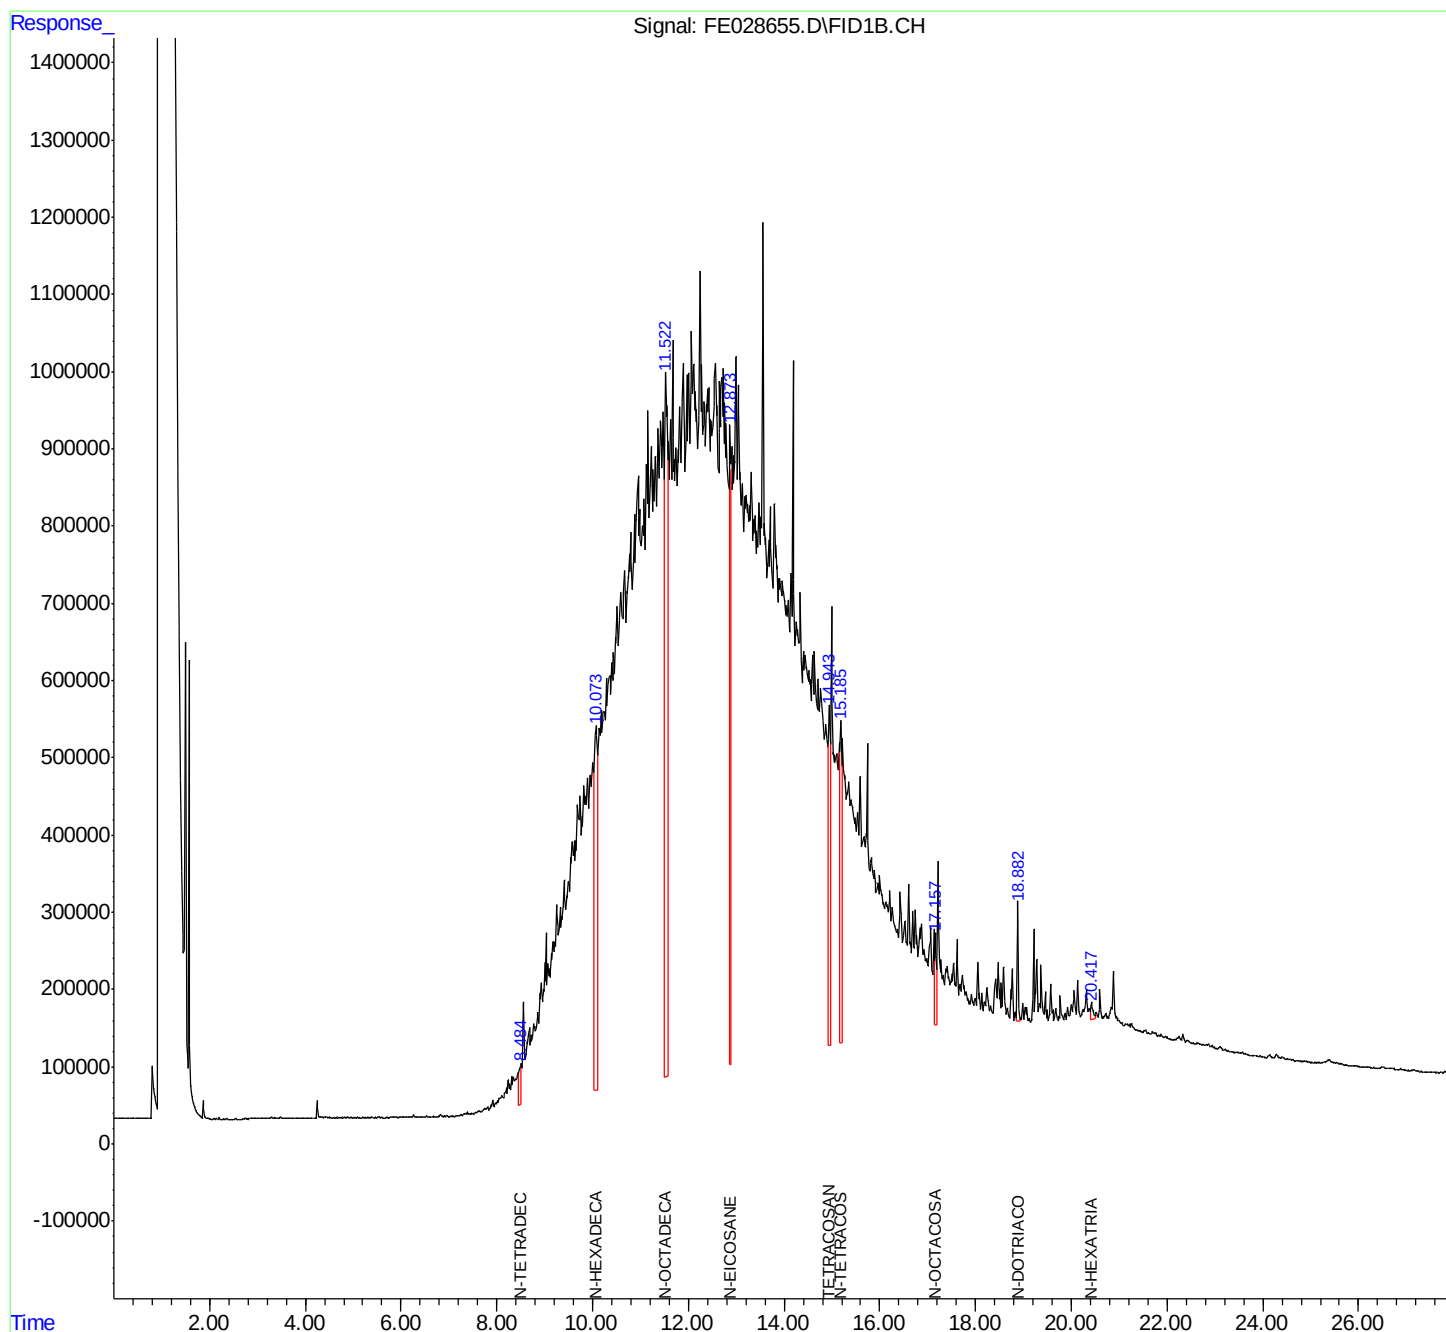

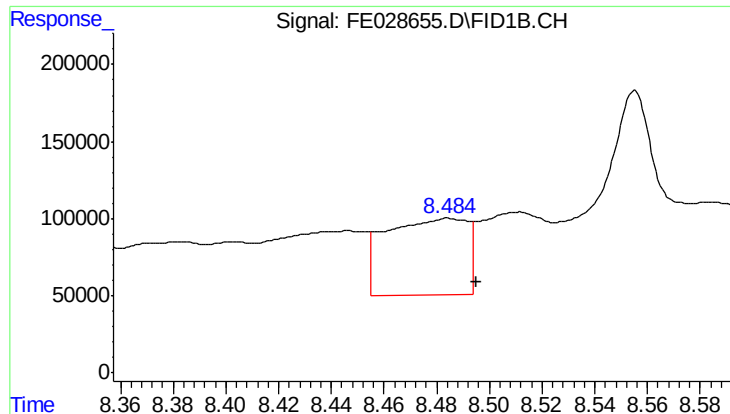


#6 N-TETRADECANE

R.T.: 8.485 min
Delta R.T.: -0.010 min
Response: 1074295
Conc: 6.44 ug/ml

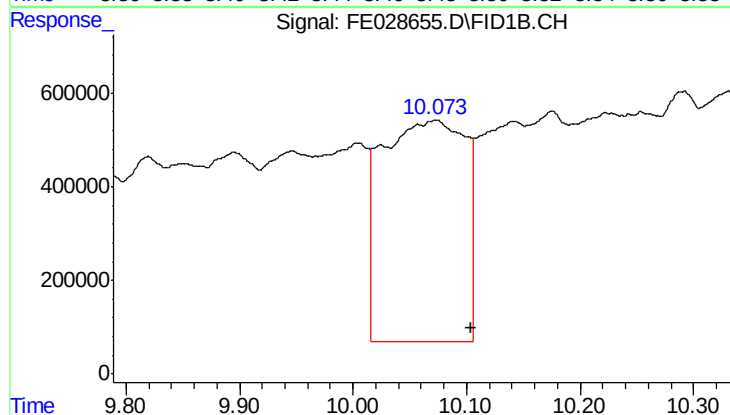


#7 N-HEXADECANE

R.T.: 10.073 min
Delta R.T.: -0.032 min
Response: 24138901
Conc: 126.89 ug/ml

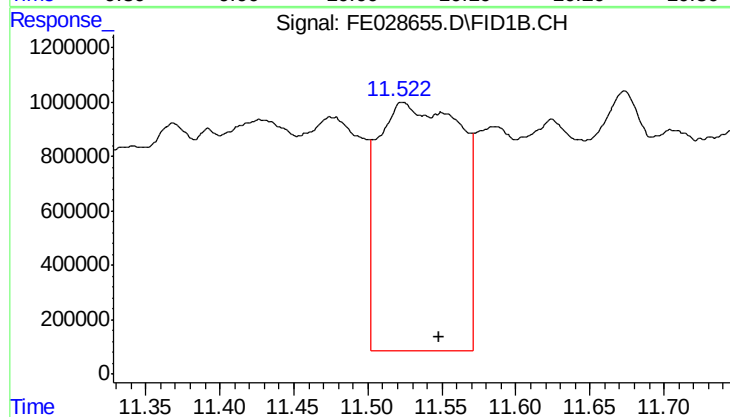


#8 N-OCTADECANE

R.T.: 11.524 min
Delta R.T.: -0.024 min
Response: 35536821
Conc: 168.76 ug/ml

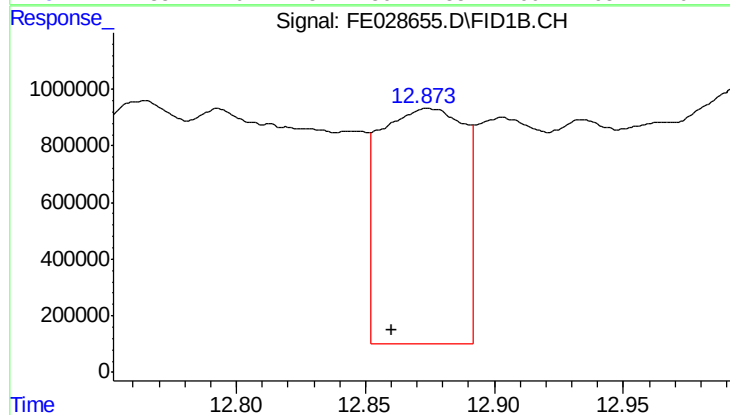


#9 N-EICOSANE

R.T.: 12.875 min
Delta R.T.: 0.015 min
Response: 19025129
Conc: 83.48 ug/ml

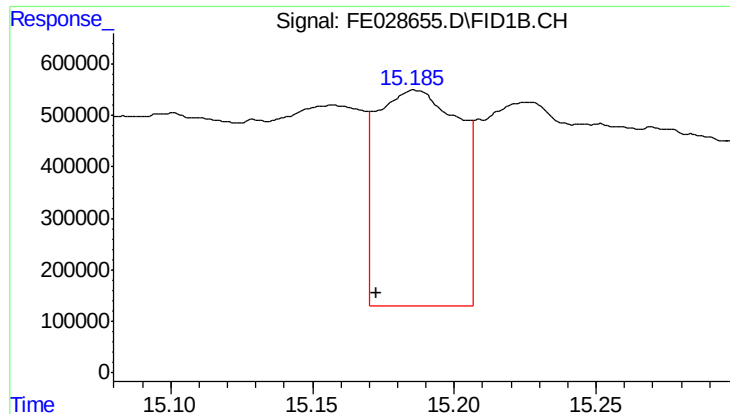


#10 N-TETRACOSANE

R.T.: 15.186 min
Delta R.T.: 0.014 min
Response: 8511390
Conc: 36.02 ug/ml

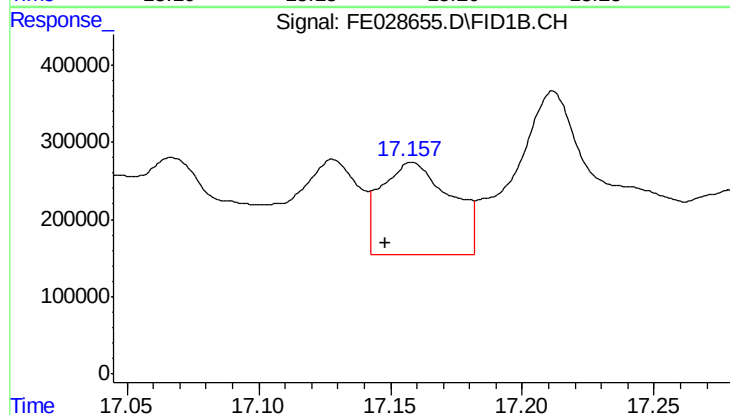


#11 N-OCTACOSANE

R.T.: 17.158 min
Delta R.T.: 0.010 min
Response: 2195647
Conc: 9.88 ug/ml

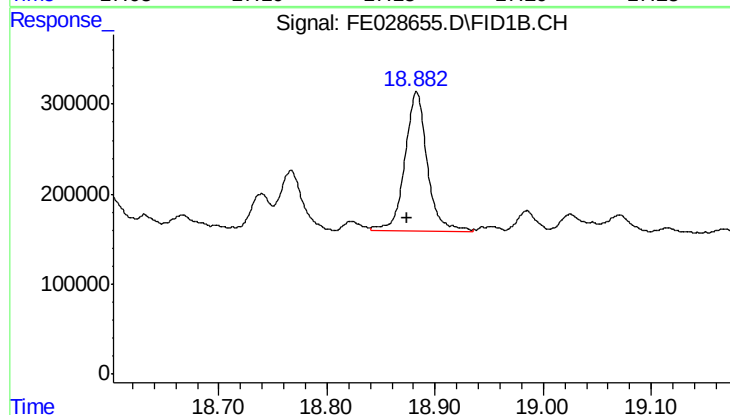


#12 N-DOTRIACONTANE

R.T.: 18.883 min
Delta R.T.: 0.009 min
Response: 2223369
Conc: 12.13 ug/ml

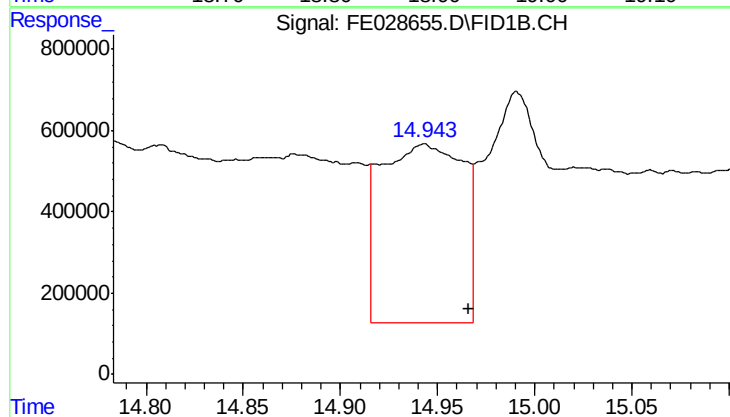

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.943 min
Delta R.T.: -0.023 min
Response: 13003182
Conc: 46.40 ug/ml

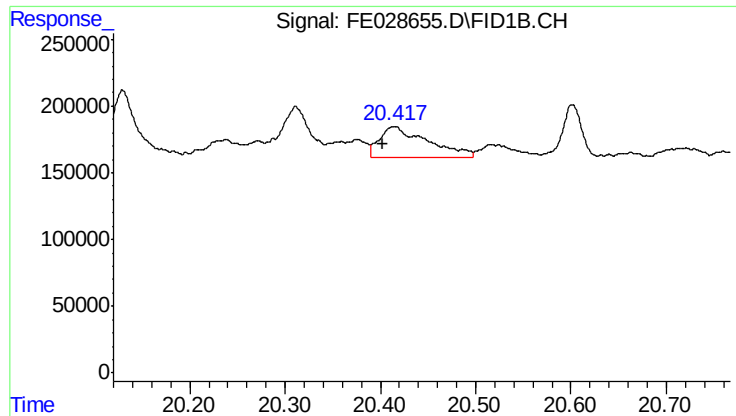

#14 N-HEXATRIACONTANE

R.T.: 20.414 min
Delta R.T.: 0.012 min
Response: 800394
Conc: 6.08 ug/ml