

Data Path : Z:\bestpcbsrv\HPCHEM1\FID E\Data\FE091718\
 Data File : FE028657.D
 Signal(s) : FID1B.CH
 Acq On : 17 Sep 2018 17:43
 Operator : AJ\SJ
 Sample : J4943-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 18 07:14:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
 Quant Title :
 QLast Update : Tue Aug 21 14:35:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.973	11098746	39.604 ug/ml
Target Compounds				
6)	N-TETRADECANE	8.552	553193	3.315 ug/ml
7)	N-HEXADECANE	10.130	1441238	7.576 ug/ml
8)	N-OCTADECANE	11.553	5315902	25.244 ug/ml
9)	N-EICOSANE	12.871	4335540	19.024 ug/ml
10)	N-TETRACOSANE	15.159	4113030	17.406 ug/ml
11)	N-OCTACOSANE	17.151	351146	1.580 ug/ml
12)	N-DOTRIACONTANE	18.883	1505213	8.210 ug/ml
14)	N-HEXATRIACONTANE	20.415	932106	7.077 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID E\Data\FE091718\
Data File : FE028657.D
Signal(s) : FID1B.CH
Acq On : 17 Sep 2018 17:43
Operator : AJ\SJ
Sample : J4943-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 18 07:14:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

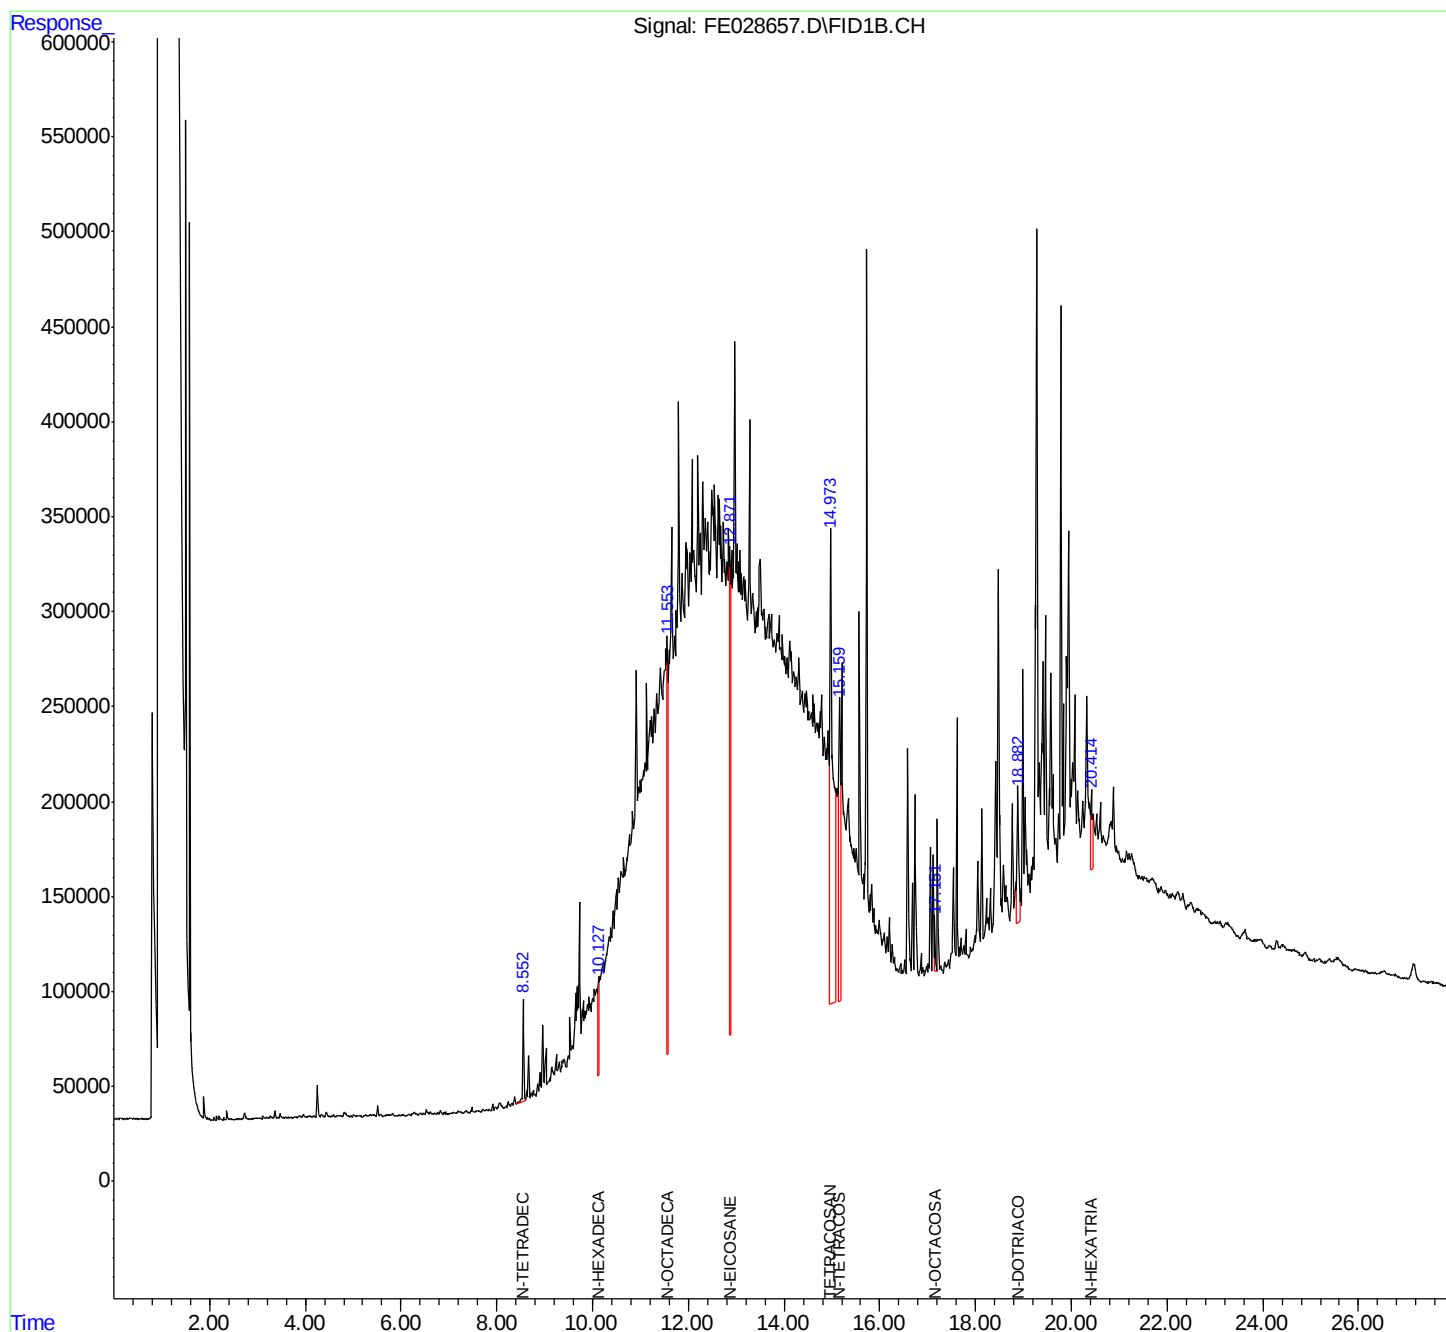

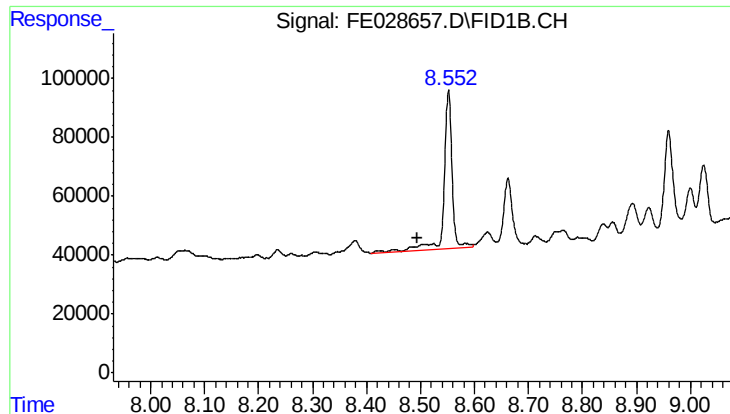


#6 N-TETRADECANE

R.T.: 8.552 min
Delta R.T.: 0.057 min
Response: 553193
Conc: 3.31 ug/ml

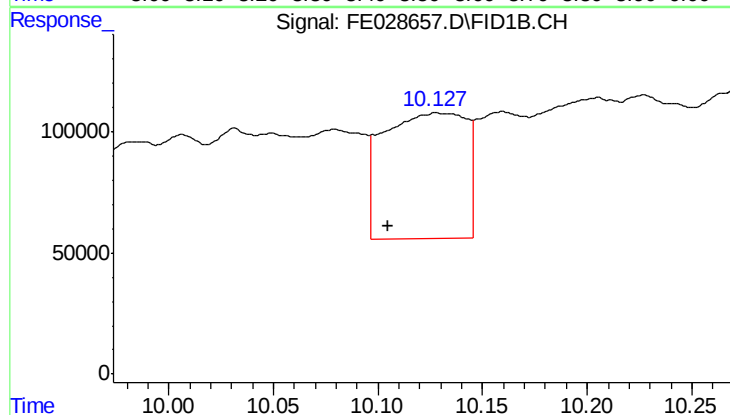


#7 N-HEXADECANE

R.T.: 10.130 min
Delta R.T.: 0.025 min
Response: 1441238
Conc: 7.58 ug/ml

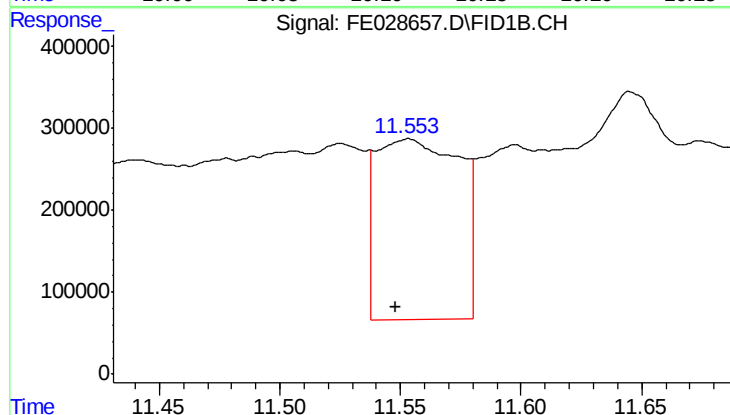


#8 N-OCTADECANE

R.T.: 11.553 min
Delta R.T.: 0.005 min
Response: 5315902
Conc: 25.24 ug/ml

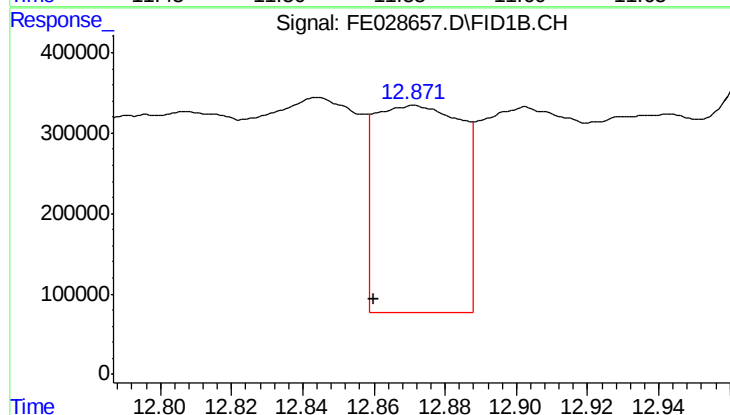


#9 N-EICOSANE

R.T.: 12.871 min
Delta R.T.: 0.011 min
Response: 4335540
Conc: 19.02 ug/ml

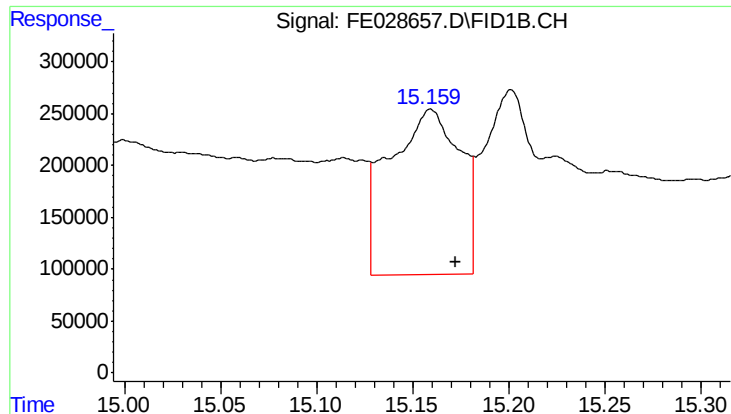


#10 N-TETRACOSANE

R.T.: 15.159 min
Delta R.T.: -0.013 min
Response: 4113030
Conc: 17.41 ug/ml

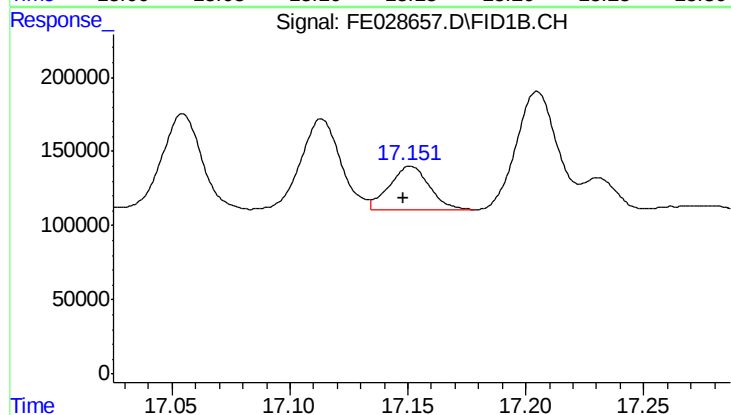


#11 N-OCTACOSANE

R.T.: 17.151 min
Delta R.T.: 0.003 min
Response: 351146
Conc: 1.58 ug/ml

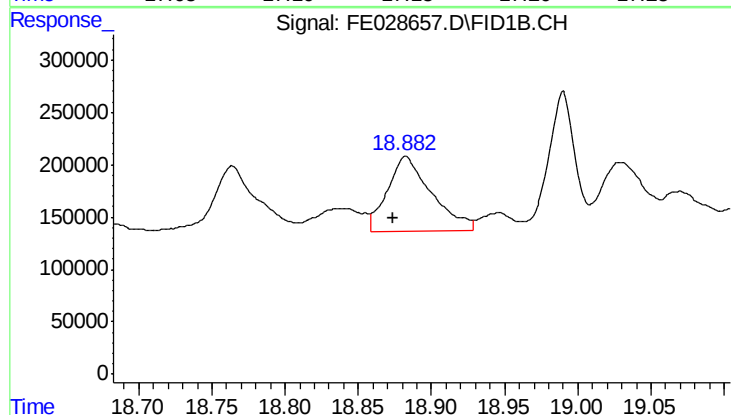


#12 N-DOTRIACONTANE

R.T.: 18.883 min
Delta R.T.: 0.009 min
Response: 1505213
Conc: 8.21 ug/ml

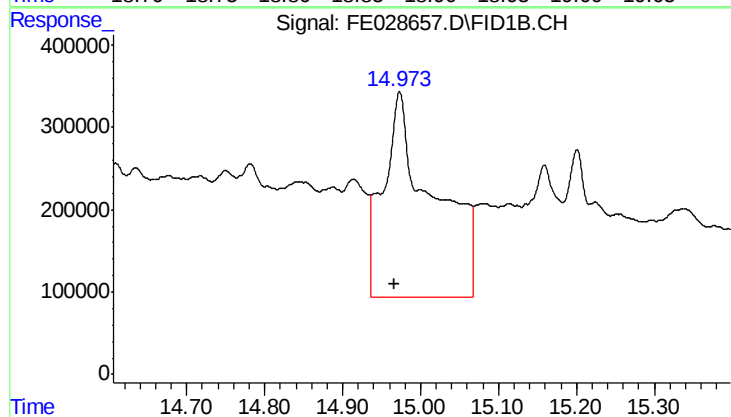

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.973 min
Delta R.T.: 0.007 min
Response: 11098746
Conc: 39.60 ug/ml

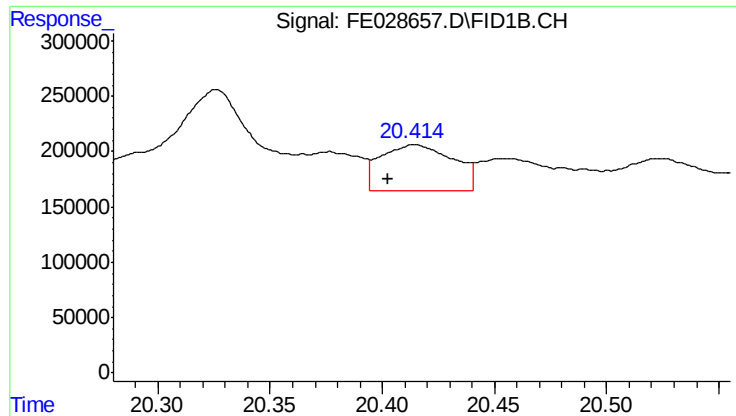

#14 N-HEXATRIACONTANE

R.T.: 20.415 min
Delta R.T.: 0.012 min
Response: 932106
Conc: 7.08 ug/ml