

Data Path : Z:\bestpcbsrv\HPCHEM1\FID E\Data\FE091718\
 Data File : FE028660.D
 Signal(s) : FID1B.CH
 Acq On : 17 Sep 2018 19:38
 Operator : AJ\SJ
 Sample : J4947-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 18 07:14:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
 Quant Title :
 QLast Update : Tue Aug 21 14:35:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.985	88014963	314.063 ug/ml
Target Compounds				
4)	N-UNDECANE	5.691	375592	2.599 ug/ml
5)	N-DODECANE	6.676	626014	4.154 ug/ml
6)	N-TETRADECANE	8.486	1978084	11.853 ug/ml
7)	N-HEXADECANE	10.123	88351815	464.452 ug/ml
8)	N-OCTADECANE	11.528	262184239	1245.068 ug/ml
9)	N-EICOSANE	12.849	114162339	500.938 ug/ml
10)	N-TETRACOSANE	15.177	42136903	178.319 ug/ml
11)	N-OCTACOSANE	17.157	22393892	100.740 ug/ml
12)	N-DOTRIACONTANE	18.843	14231646	77.624 ug/ml
14)	N-HEXATRIACONTANE	20.428	9633542	73.140 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID E\Data\FE091718\
Data File : FE028660.D
Signal(s) : FID1B.CH
Acq On : 17 Sep 2018 19:38
Operator : AJ\SJ
Sample : J4947-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 18 07:14:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

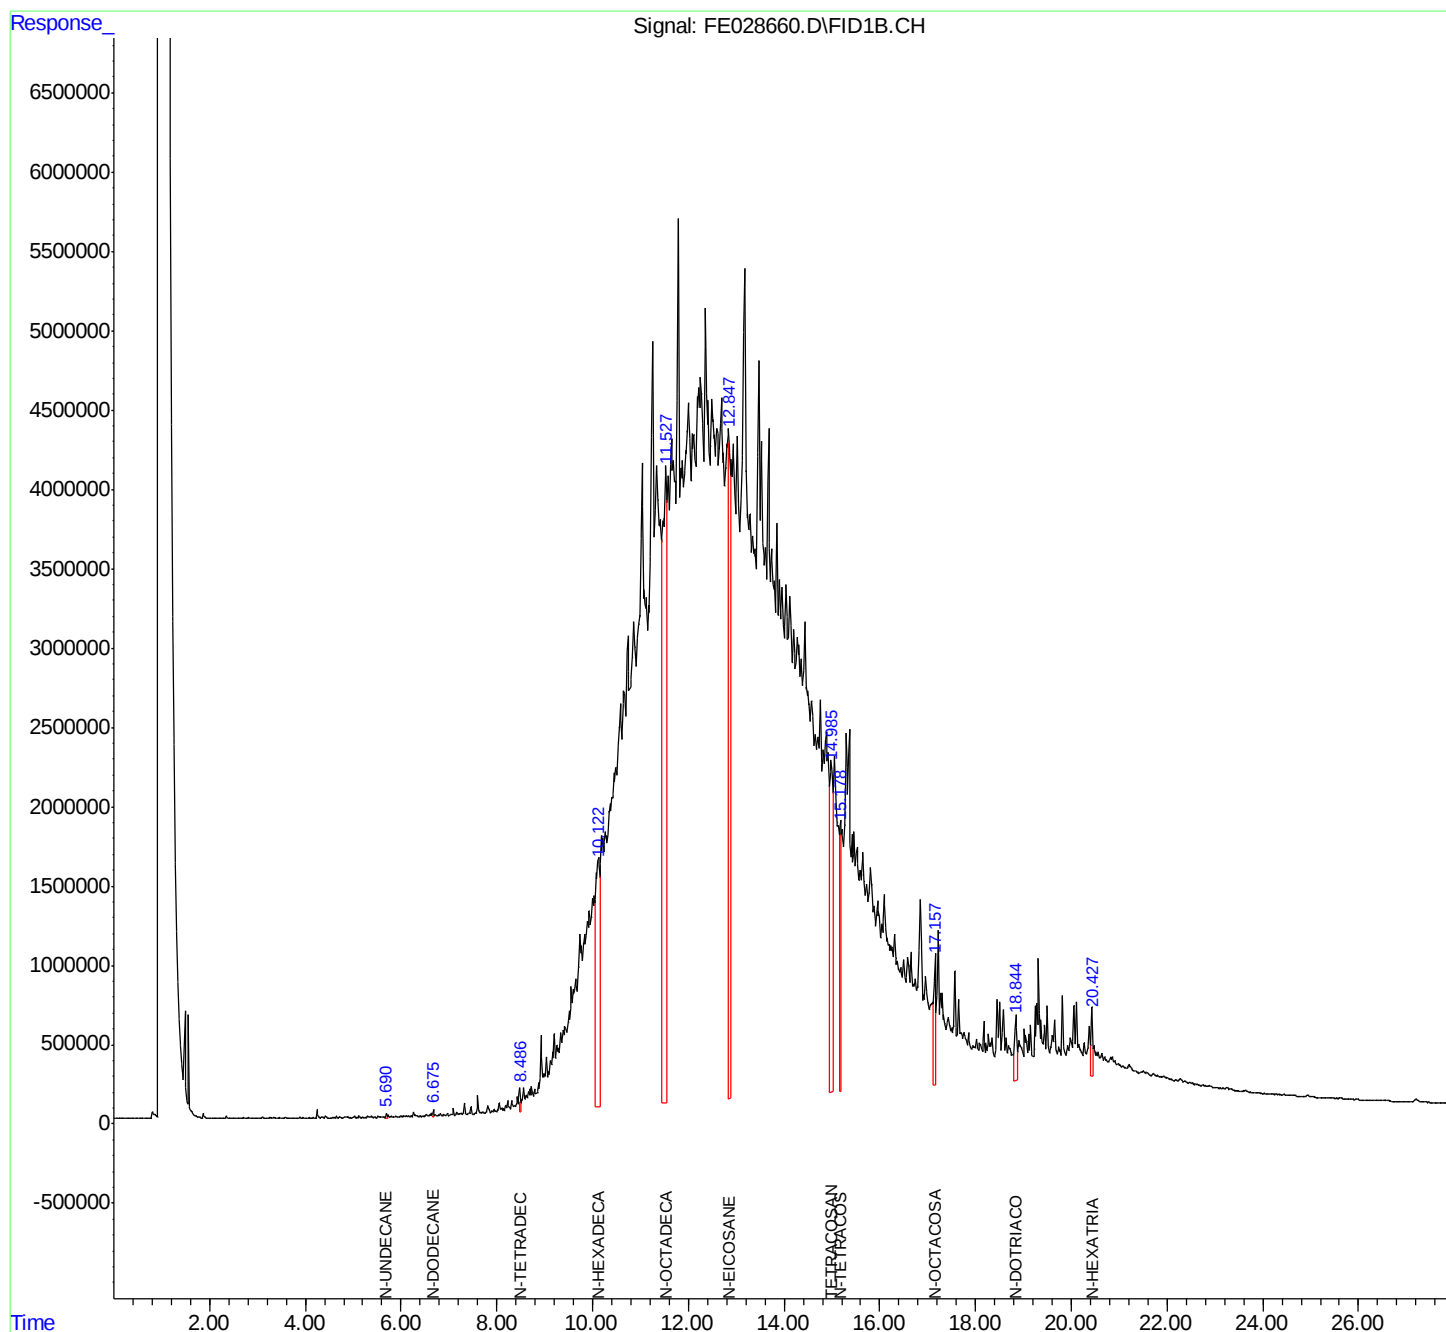

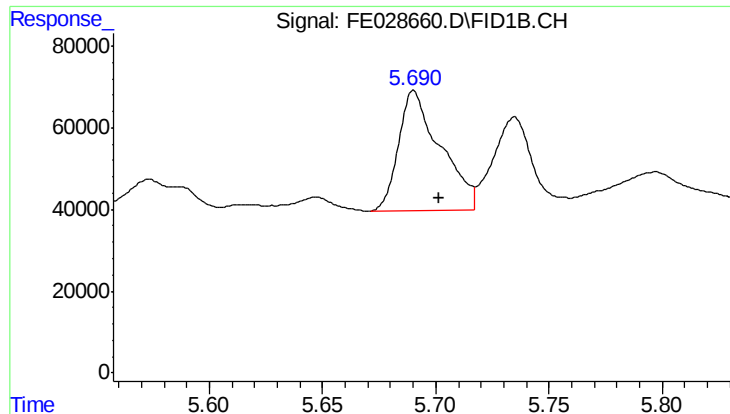


#4 N-UNDECANE

R.T.: 5.691 min
Delta R.T.: -0.011 min
Response: 375592
Conc: 2.60 ug/ml

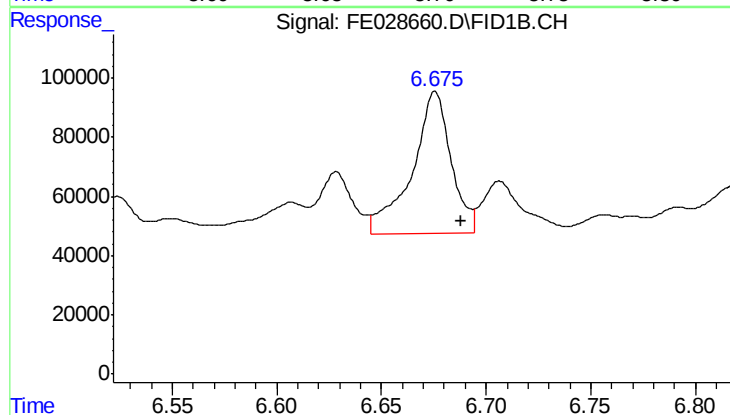


#5 N-DODECANE

R.T.: 6.676 min
Delta R.T.: -0.013 min
Response: 626014
Conc: 4.15 ug/ml

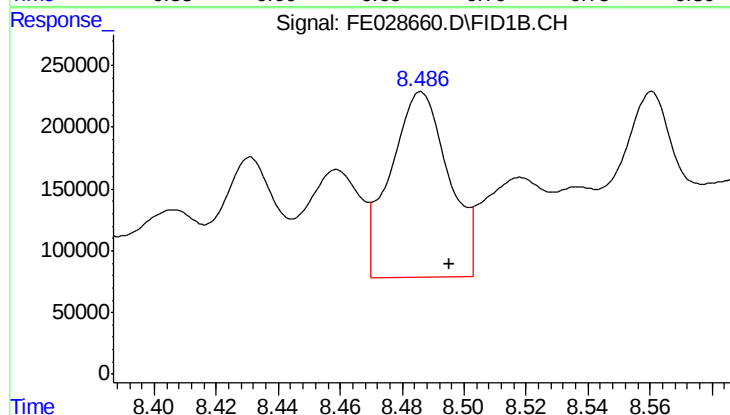


#6 N-TETRADECANE

R.T.: 8.486 min
Delta R.T.: -0.009 min
Response: 1978084
Conc: 11.85 ug/ml

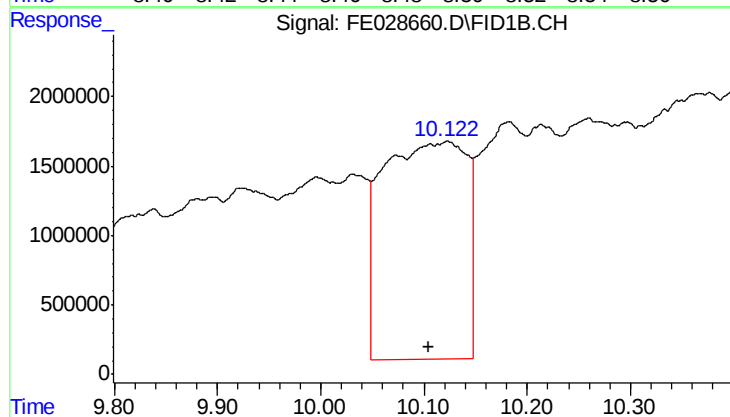


#7 N-HEXADECANE

R.T.: 10.123 min
Delta R.T.: 0.018 min
Response: 88351815
Conc: 464.45 ug/ml

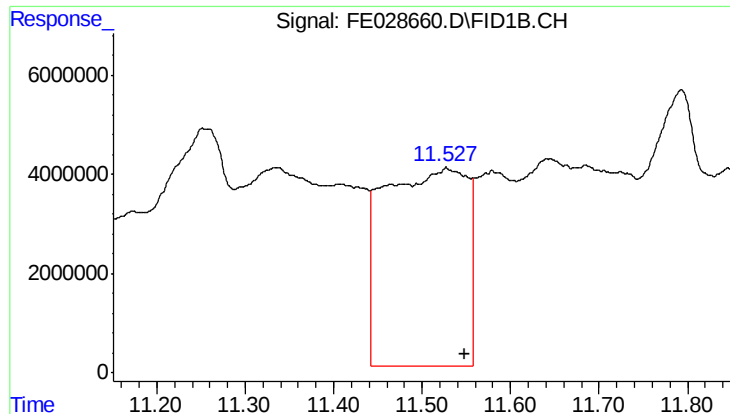


#8 N-OCTADECANE

R.T.: 11.528 min
Delta R.T.: -0.020 min
Response: 262184239
Conc: 1245.07 ug/ml

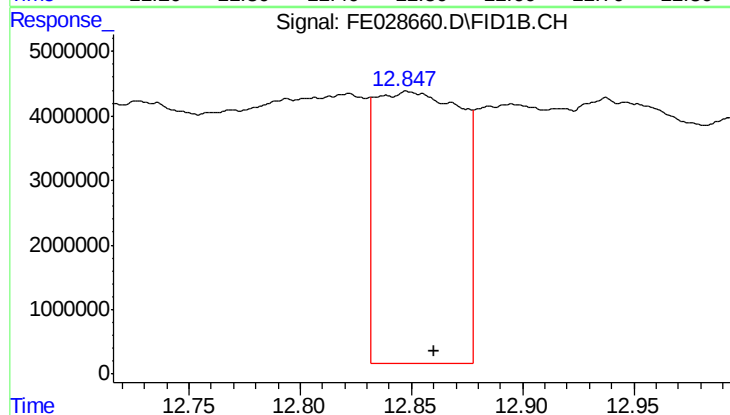


#9 N-EICOSANE

R.T.: 12.849 min
Delta R.T.: -0.011 min
Response: 114162339
Conc: 500.94 ug/ml

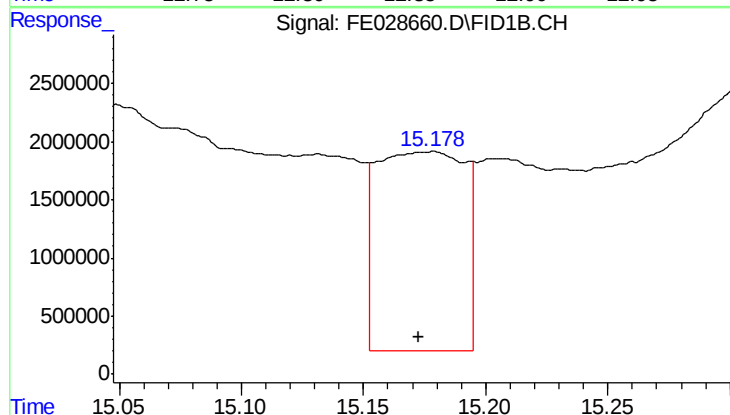


#10 N-TETRACOSANE

R.T.: 15.177 min
Delta R.T.: 0.004 min
Response: 42136903
Conc: 178.32 ug/ml

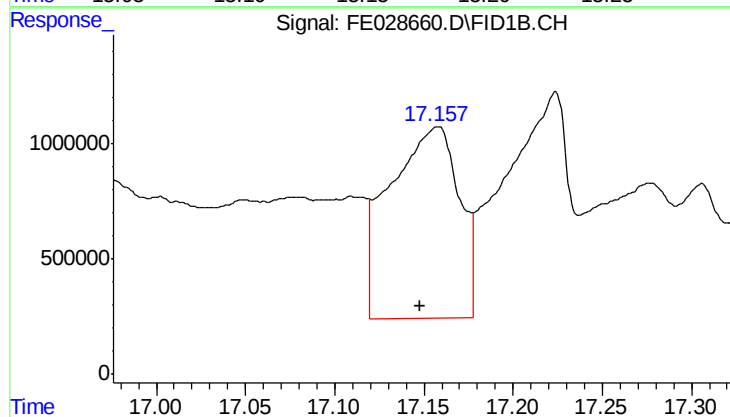


#11 N-OCTACOSANE

R.T.: 17.157 min
Delta R.T.: 0.009 min
Response: 22393892
Conc: 100.74 ug/ml

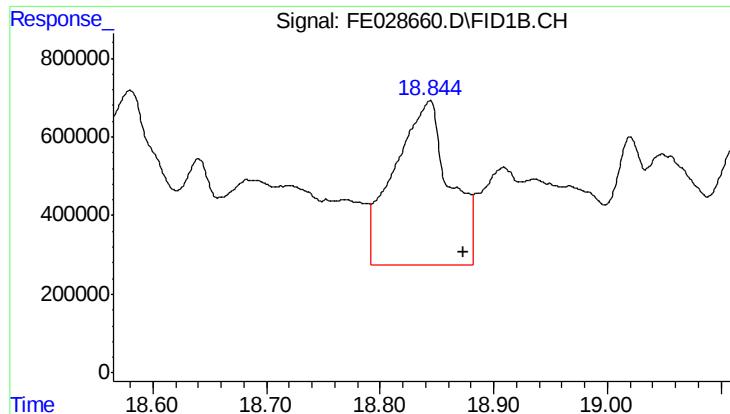


#12 N-DOTRIACONTANE

R.T.: 18.843 min
Delta R.T.: -0.031 min
Response: 14231646
Conc: 77.62 ug/ml

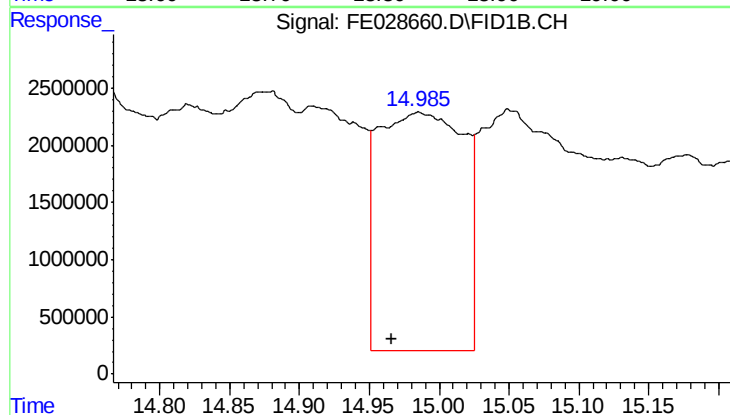

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.985 min
Delta R.T.: 0.019 min
Response: 88014963
Conc: 314.06 ug/ml

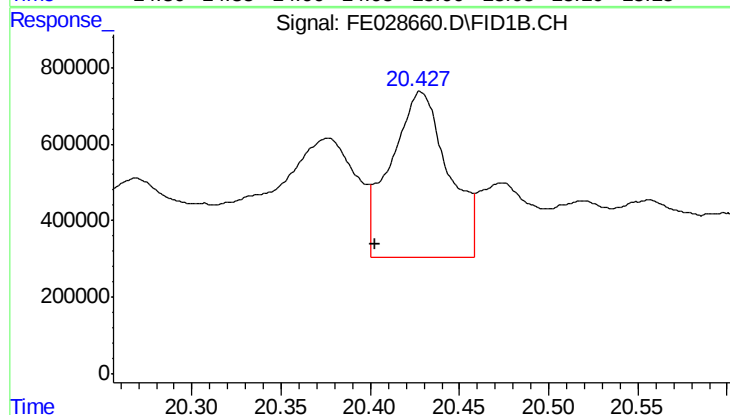

#14 N-HEXATRIACONTANE

R.T.: 20.428 min
Delta R.T.: 0.026 min
Response: 9633542
Conc: 73.14 ug/ml