

Data Path : Z:\bestpcbsrv\HPCHEM1\FID E\Data\FE091718\
 Data File : FE028664.D
 Signal(s) : FID1B.CH
 Acq On : 17 Sep 2018 22:11
 Operator : AJ\SJ
 Sample : J4952-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 18 07:15:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
 Quant Title :
 QLast Update : Tue Aug 21 14:35:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
6) N-TETRADECANE	8.553	780117	4.675 ug/ml
7) N-HEXADECANE	10.060	1595301	8.386 ug/ml
9) N-EICOSANE	12.859	571651	2.508 ug/ml
10) N-TETRACOSANE	15.189	466190	1.973 ug/ml
11) N-OCTACOSANE	17.108	714135	3.213 ug/ml
12) N-DOTRIACONTANE	18.873	921475	5.026 ug/ml
14) N-HEXATRIACONTANE	20.403	177784	1.350 ug/ml
15) N-TETRACONTANE	22.207	603190	5.226 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID E\Data\FE091718\
Data File : FE028664.D
Signal(s) : FID1B.CH
Acq On : 17 Sep 2018 22:11
Operator : AJ\SJ
Sample : J4952-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 18 07:15:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE082118.M
Quant Title :
QLast Update : Tue Aug 21 14:35:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

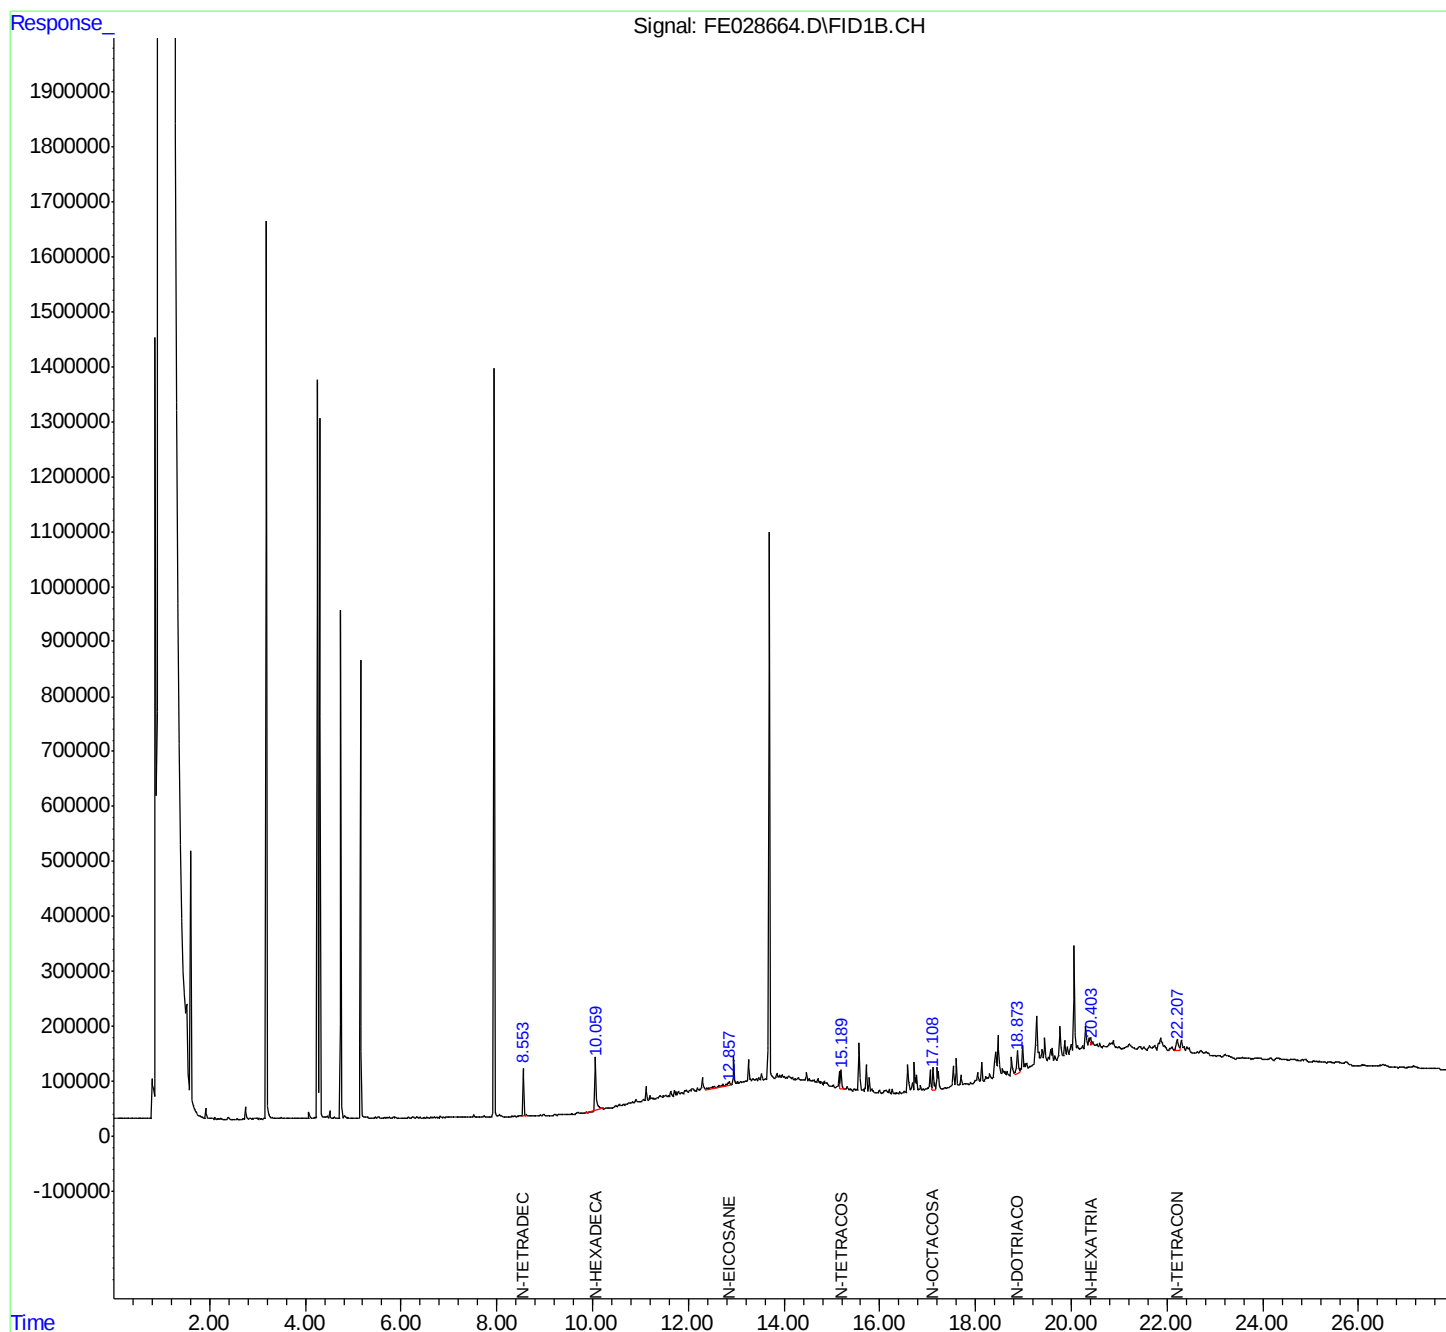

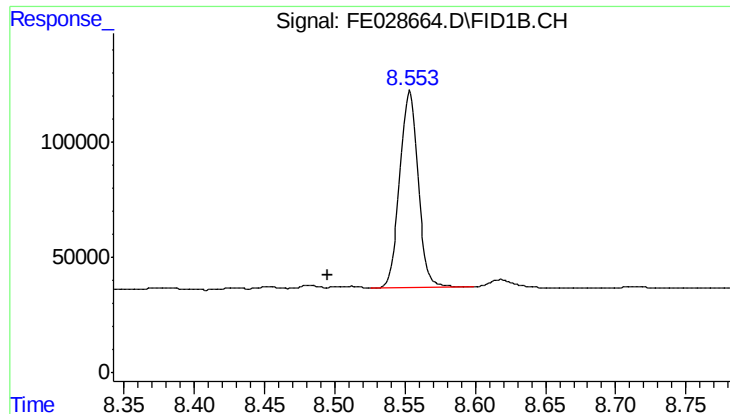


#6 N-TETRADECANE

R.T.: 8.553 min
Delta R.T.: 0.058 min
Response: 780117
Conc: 4.67 ug/ml

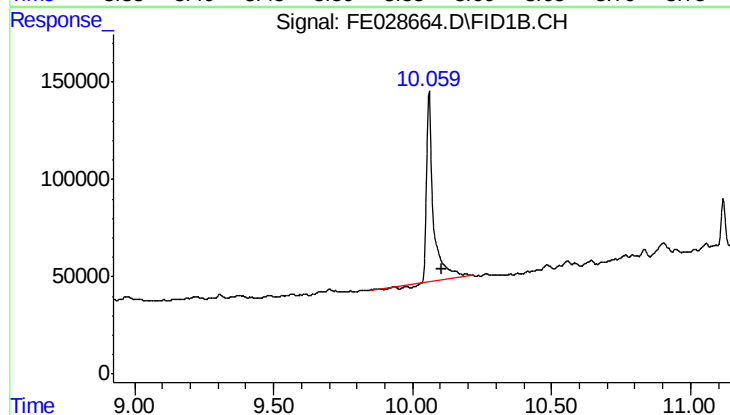


#7 N-HEXADECANE

R.T.: 10.060 min
Delta R.T.: -0.045 min
Response: 1595301
Conc: 8.39 ug/ml

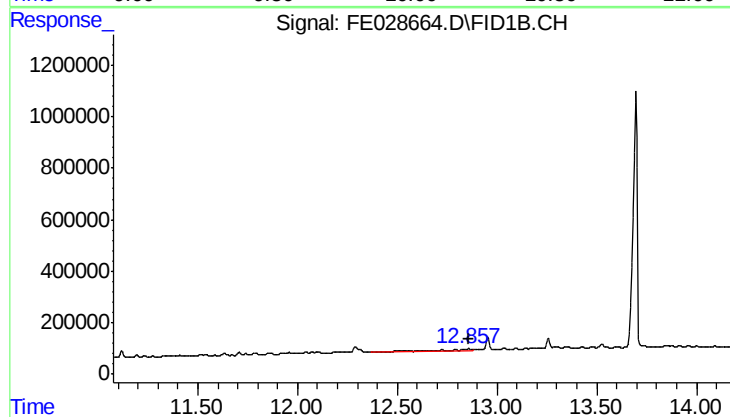


#9 N-EICOSANE

R.T.: 12.859 min
Delta R.T.: -0.001 min
Response: 571651
Conc: 2.51 ug/ml

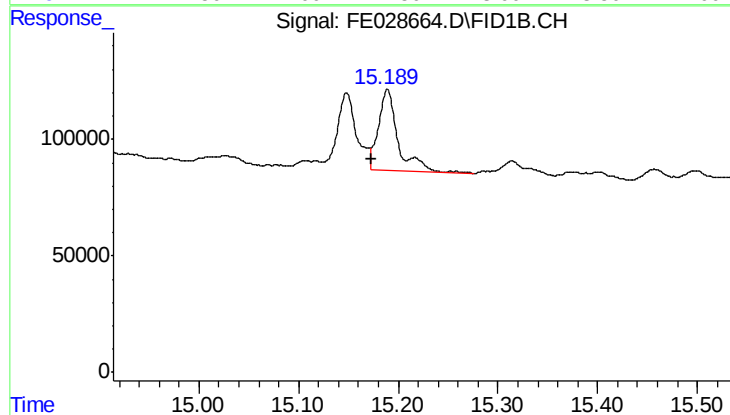


#10 N-TETRACOSANE

R.T.: 15.189 min
Delta R.T.: 0.016 min
Response: 466190
Conc: 1.97 ug/ml

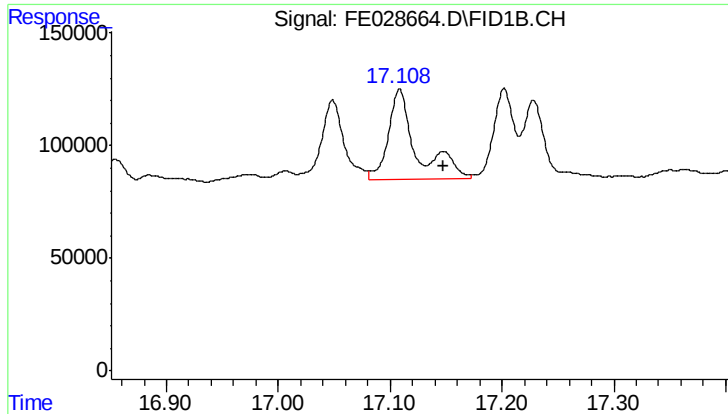


#11 N-OCTACOSANE

R.T.: 17.108 min
Delta R.T.: -0.040 min
Response: 714135
Conc: 3.21 ug/ml

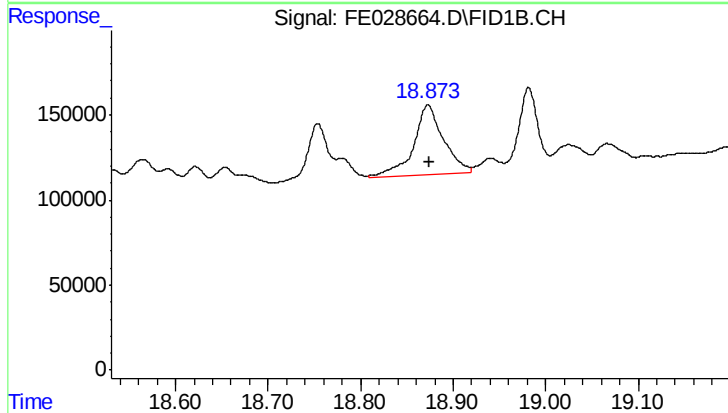


#12 N-DOTRIACONTANE

R.T.: 18.873 min
Delta R.T.: 0.000 min
Response: 921475
Conc: 5.03 ug/ml

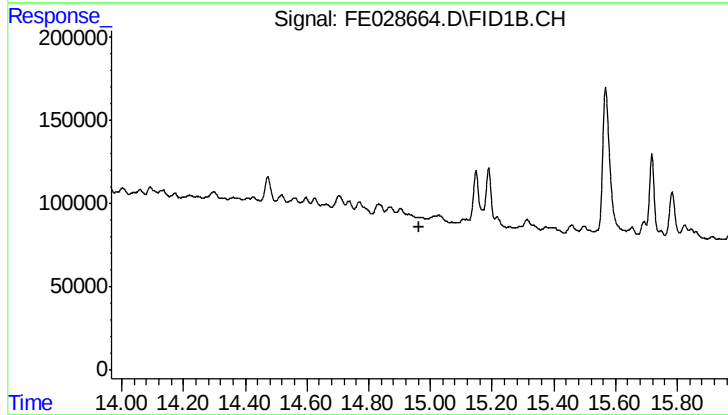


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.966 min
Response: 0
Conc: N.D.

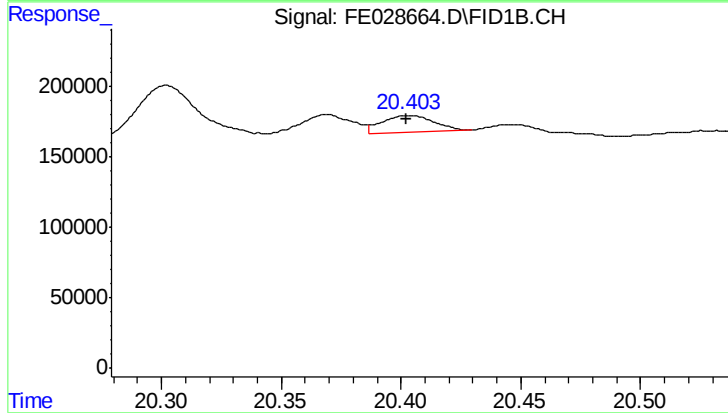

#14 N-HEXATRIACONTANE

R.T.: 20.403 min
Delta R.T.: 0.000 min
Response: 177784
Conc: 1.35 ug/ml

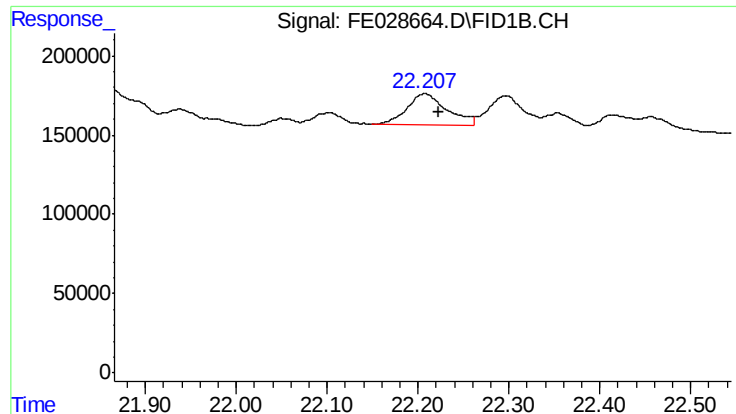

#15 N-TETRACONTANE

R.T.: 22.207 min
Delta R.T.: -0.015 min
Response: 603190
Conc: 5.23 ug/ml