

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091719\
Data File : FE030498.D
Signal(s) : FID1B.CH
Acq On : 17 Sep 2019 14:28
Operator : DD\AJ
Sample : K4897-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 18 02:04:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.538	3387831	17.024 ug/ml
Target Compounds				
9)	N-EICOSANE	12.434	44531	0.232 ug/ml
10)	N-TETRACOSANE	14.736	178797	0.933 ug/ml
11)	N-OCTACOSANE	16.752	120223	0.639 ug/ml
12)	N-DOTRIACONTANE	18.424	422600	2.378 ug/ml
14)	N-HEXATRIACONTANE	19.953	83118	0.524 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE091719\
Data File : FE030498.D
Signal(s) : FID1B.CH
Acq On : 17 Sep 2019 14:28
Operator : DD\AJ
Sample : K4897-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 18 02:04:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE090819.M
Quant Title :
QLast Update : Mon Sep 09 04:07:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

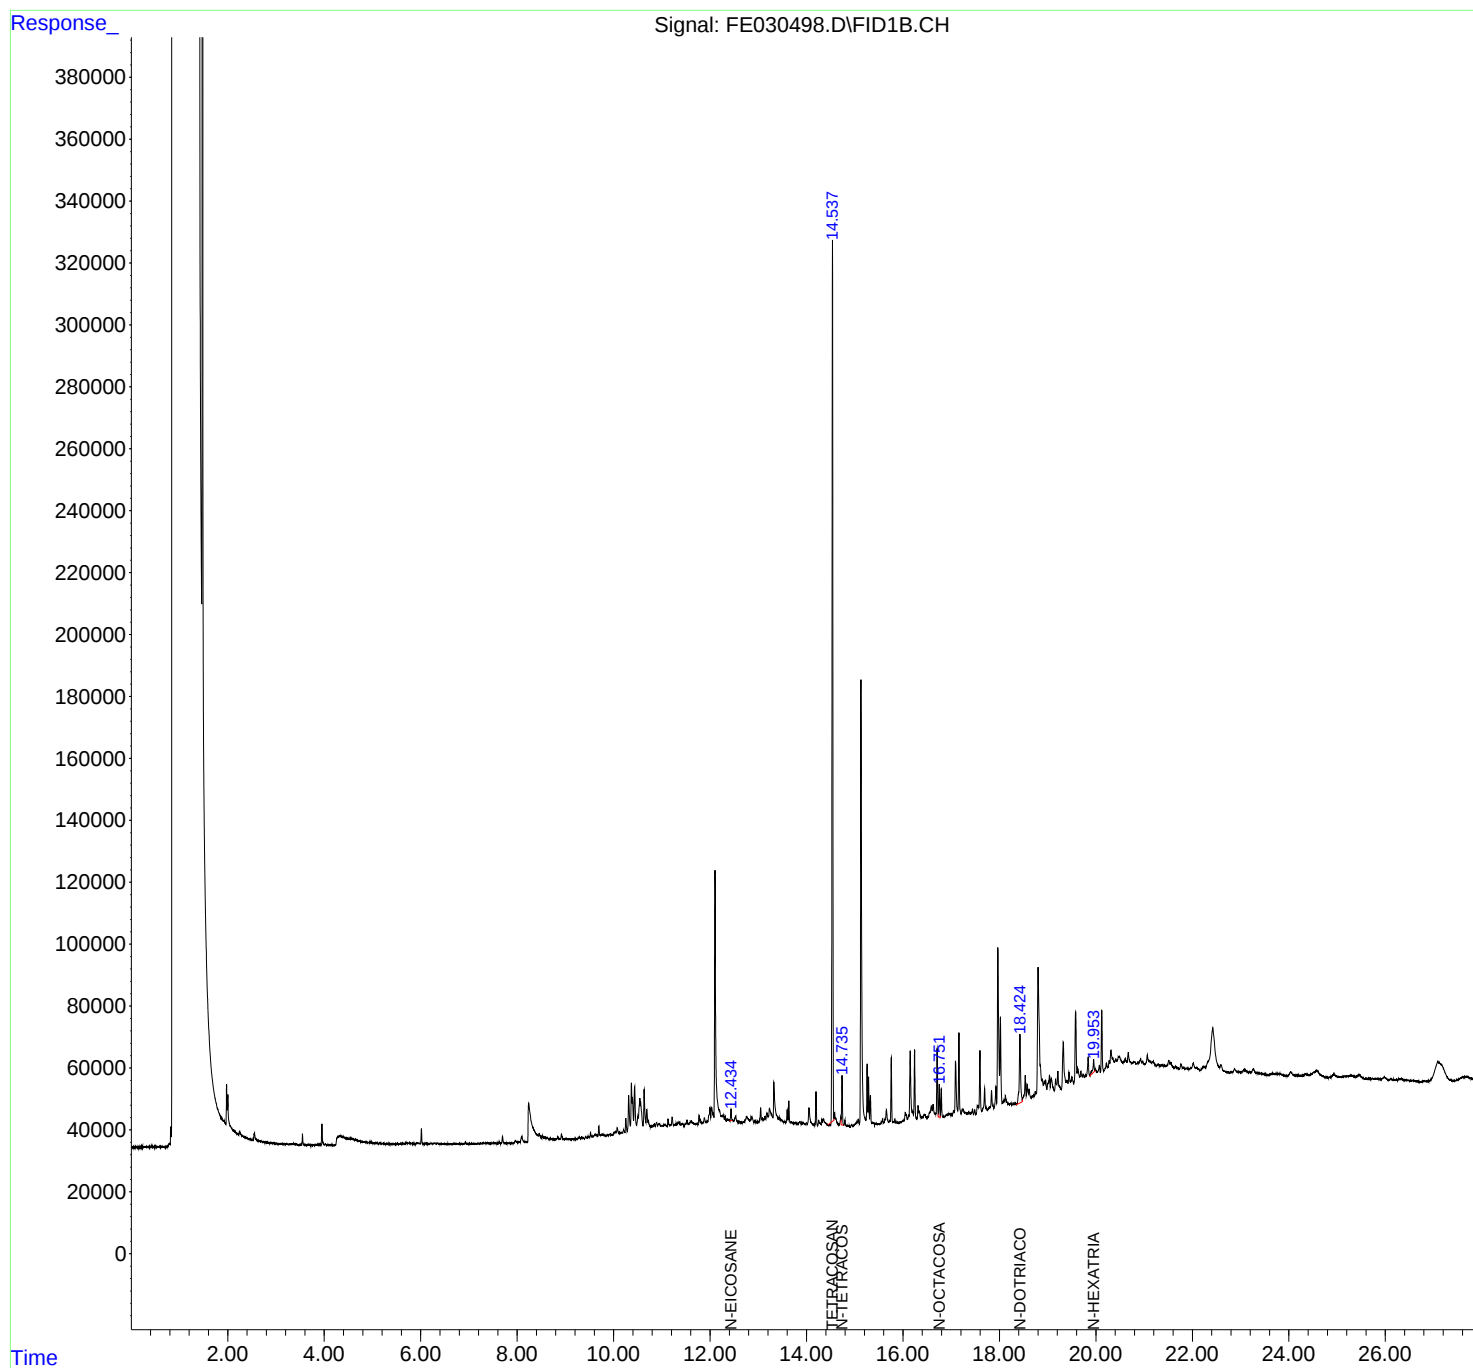

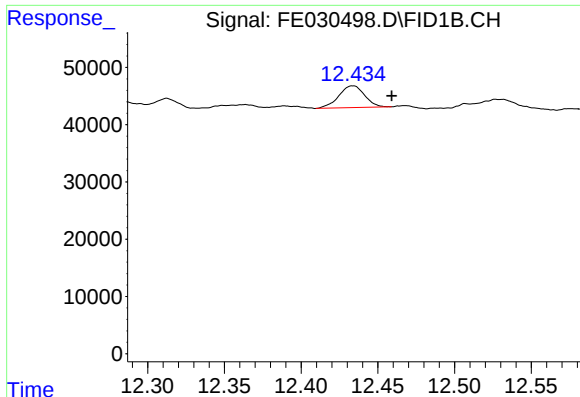


#9 N-EICOSANE

R.T.: 12.434 min
Delta R.T.: -0.025 min
Response: 44531
Conc: 0.23 ug/ml

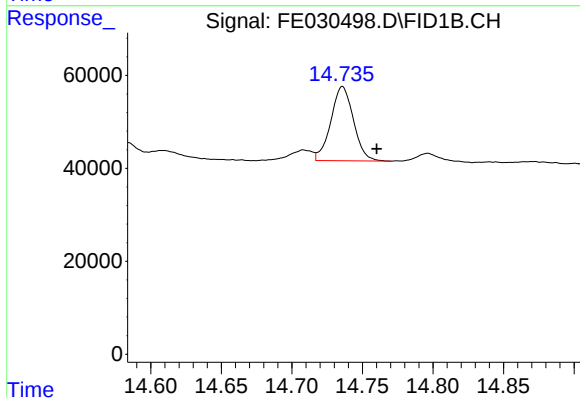


#10 N-TETRACOSANE

R.T.: 14.736 min
Delta R.T.: -0.024 min
Response: 178797
Conc: 0.93 ug/ml

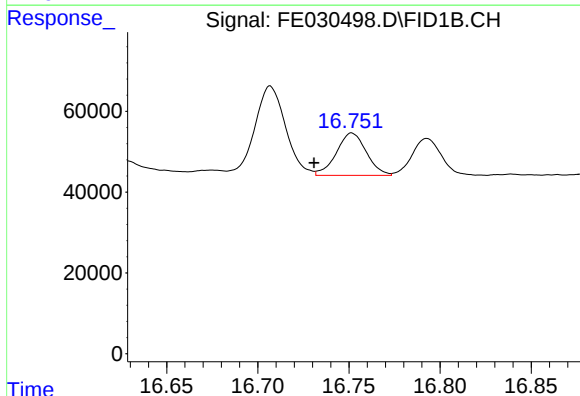


#11 N-OCTACOSANE

R.T.: 16.752 min
Delta R.T.: 0.021 min
Response: 120223
Conc: 0.64 ug/ml

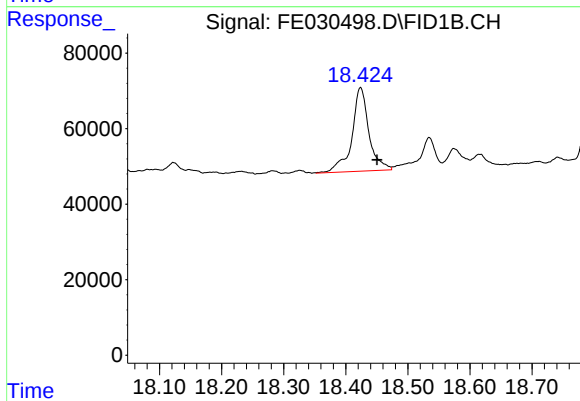


#12 N-DOTRIACONTANE

R.T.: 18.424 min
Delta R.T.: -0.027 min
Response: 422600
Conc: 2.38 ug/ml

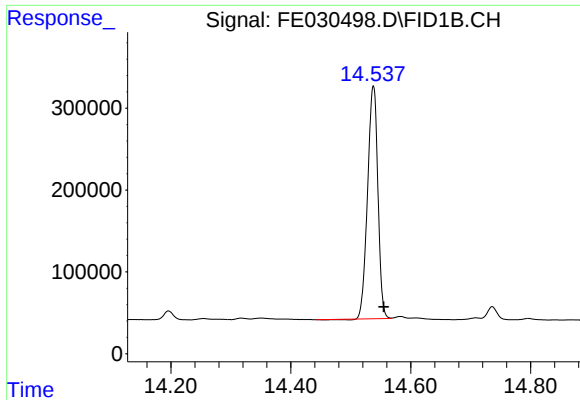

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.538 min
Delta R.T.: -0.017 min
Response: 3387831
Conc: 17.02 ug/ml

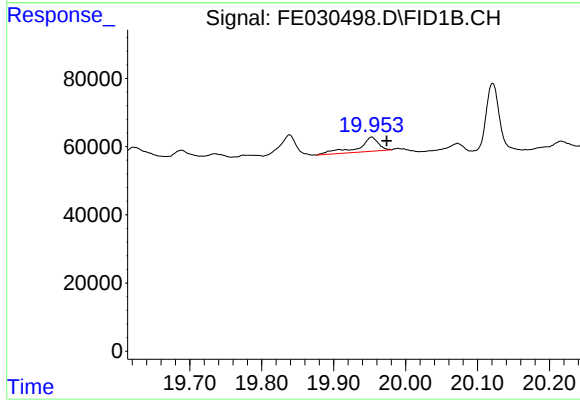

#14 N-HEXATRIACONTANE

R.T.: 19.953 min
Delta R.T.: -0.021 min
Response: 83118
Conc: 0.52 ug/ml